

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021622\
 Data File : BP009174.D
 Acq On : 16 Feb 2022 12:28
 Operator : CG/JU
 Sample : PB142687BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB142687BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009174.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.387	401	408	436	rBV	2918115	5184714	29.26%	7.975%
2	6.981	672	679	715	rBV	2689395	5224299	29.48%	8.036%
3	7.787	809	816	834	rBV	617754	1081535	6.10%	1.664%
4	8.951	1006	1014	1043	rBV	1689086	3365047	18.99%	5.176%
5	10.587	1284	1292	1317	rBV	715126	1529708	8.63%	2.353%
6	13.051	1703	1711	1747	rBV	5669890	9487717	53.54%	14.593%
7	14.434	1939	1946	1966	rBV	1403096	2364026	13.34%	3.636%
8	15.933	2194	2201	2235	rBV	4564487	8062325	45.50%	12.401%
9	17.192	2408	2415	2433	rBV	1748681	3148808	17.77%	4.843%
10	19.757	2845	2851	2866	rBV	13871687	17720046	100.00%	27.256%
11	21.292	3107	3112	3122	rBV	2743876	3876248	21.87%	5.962%
12	23.680	3511	3518	3531	rBV2	1710808	3969710	22.40%	6.106%




Sum of corrected areas: 65014183

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021622\
Data File : BP009174.D
Acq On : 16 Feb 2022 12:28
Operator : CG/JU
Sample : PB142687BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142687BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

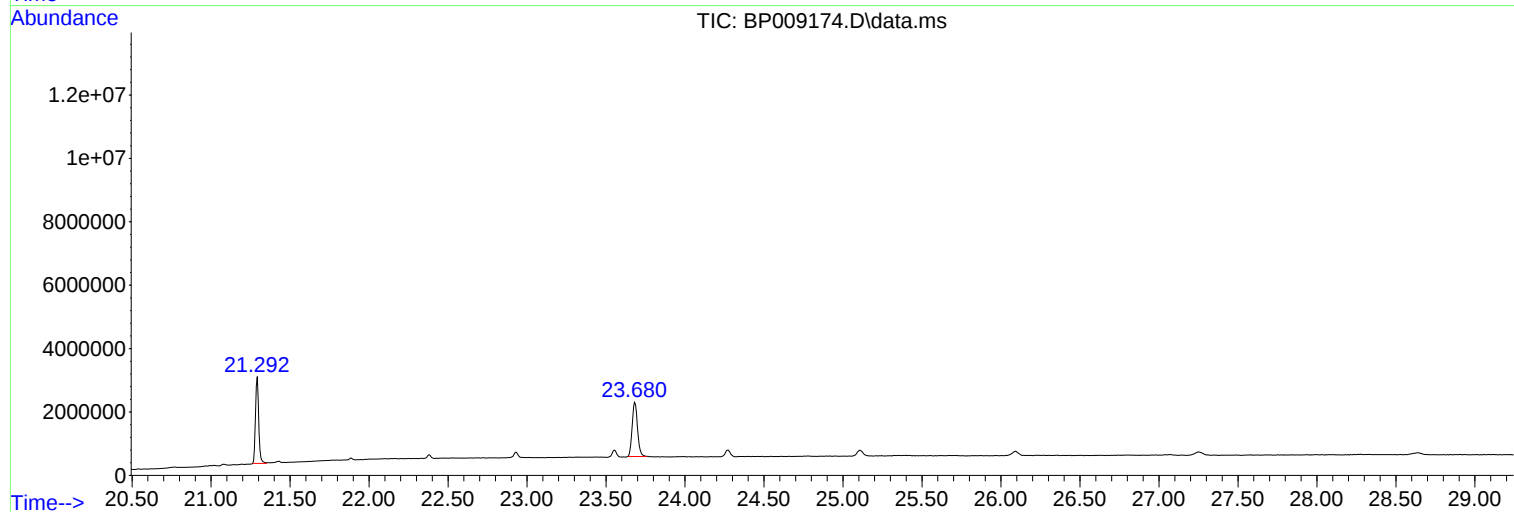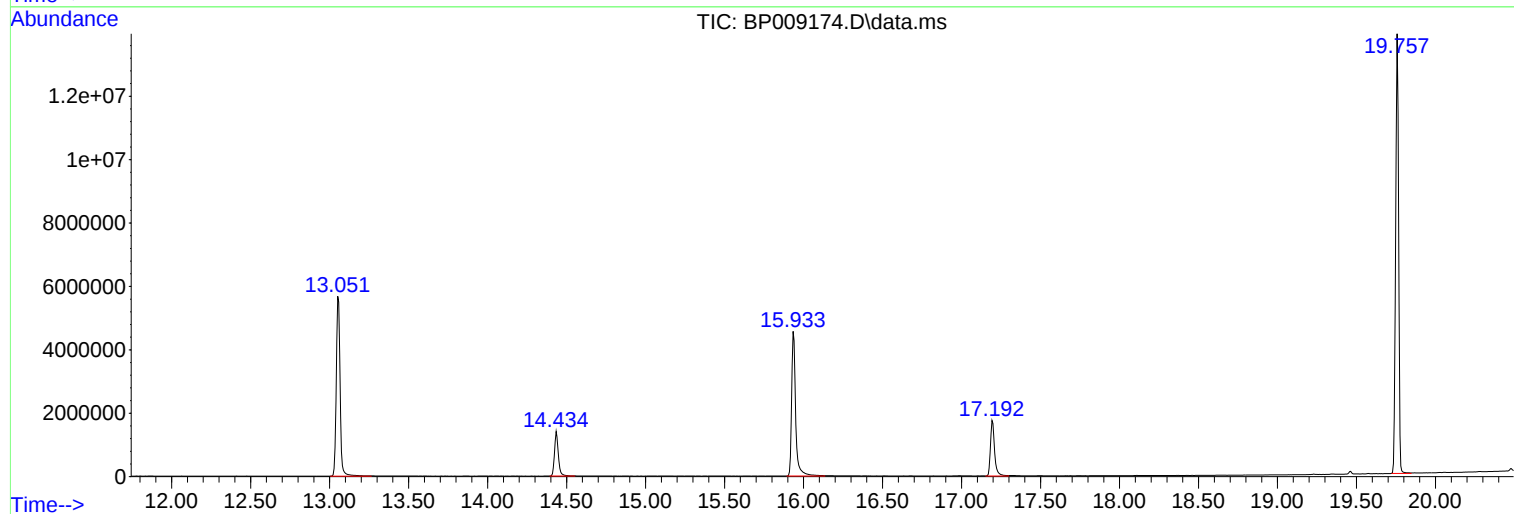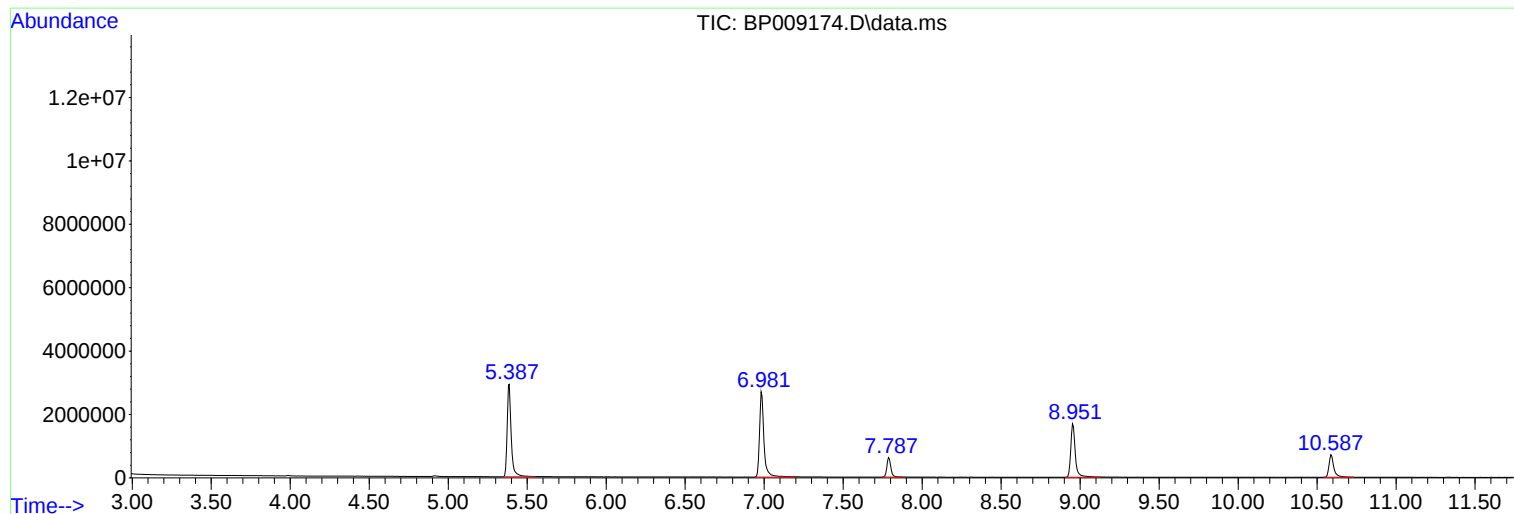

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021622\
Data File : BP009174.D
Acq On : 16 Feb 2022 12:28
Operator : CG/JU
Sample : PB142687BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142687BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021622\
Data File : BP009174.D
Acq On : 16 Feb 2022 12:28
Operator : CG/JU
Sample : PB142687BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142687BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------