
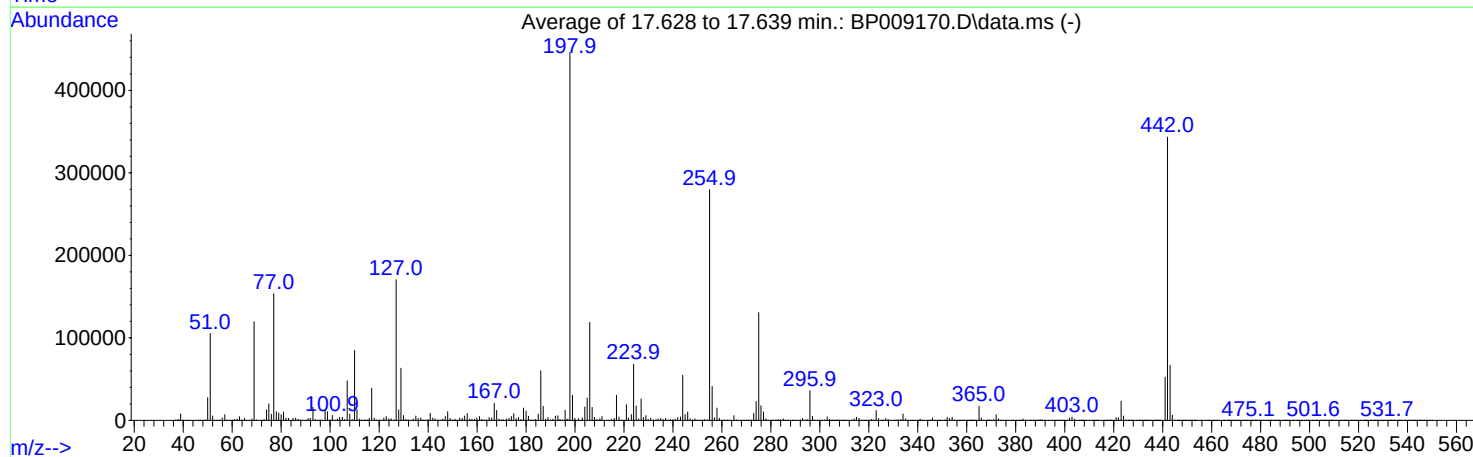


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021622\
 Data File : BP009170.D
 Acq On : 16 Feb 2022 09:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 16 14:30:24 2022

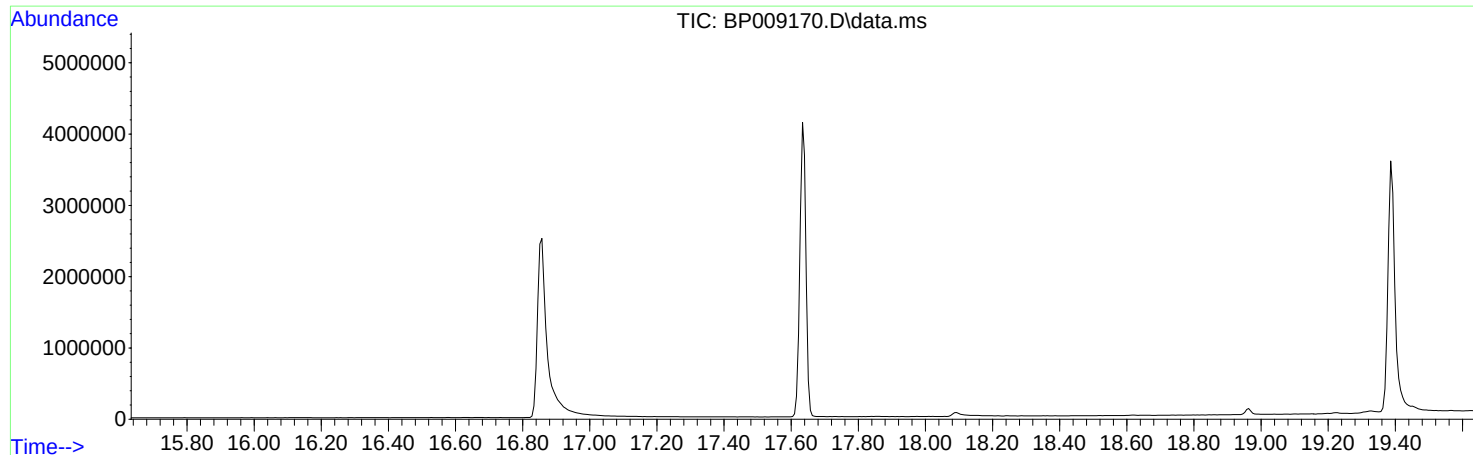




AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.6	105334	PASS
68	69	0.00	2	1.5	1807	PASS
69	198	0.00	100	26.8	119463	PASS
70	69	0.00	2	0.5	619	PASS
127	198	10	80	38.2	170556	PASS
197	198	0.00	2	0.4	1628	PASS
198	198	100	100	100.0	445918	PASS
199	198	5	9	6.8	30419	PASS
275	198	10	60	29.3	130719	PASS
365	198	1	100	3.8	17165	PASS
441	198	0.01	100	11.8	52429	PASS
442	442	100	100	100.0	343296	PASS
443	442	15	24	19.5	66788	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021622\
 Data File : BP009170.D
 Acq On : 16 Feb 2022 09:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Feb 16 14:26:29 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 16 01:29:44 2022
 Response via : Initial Calibration

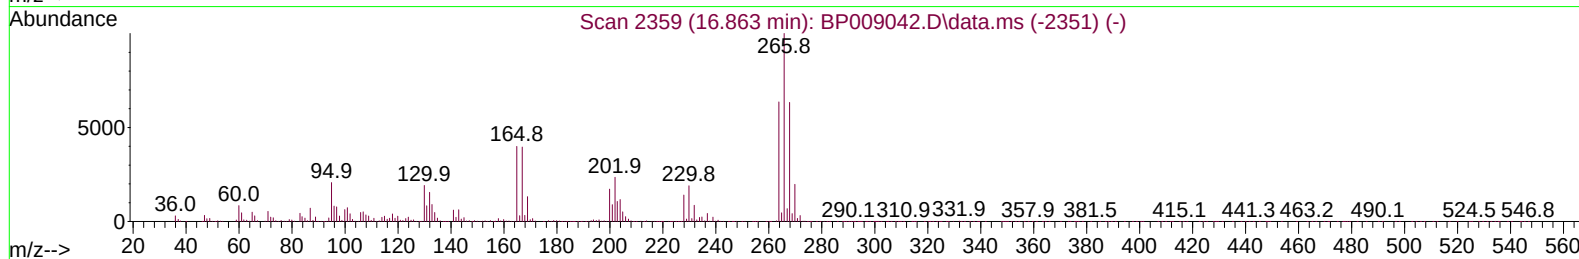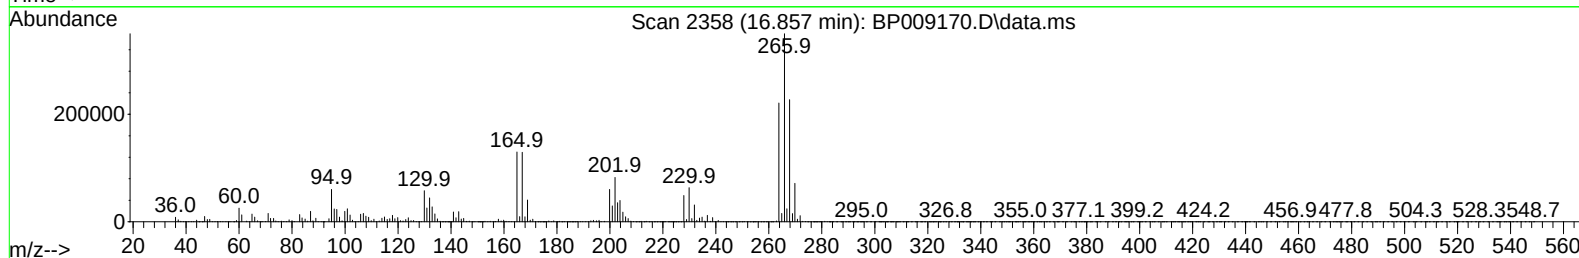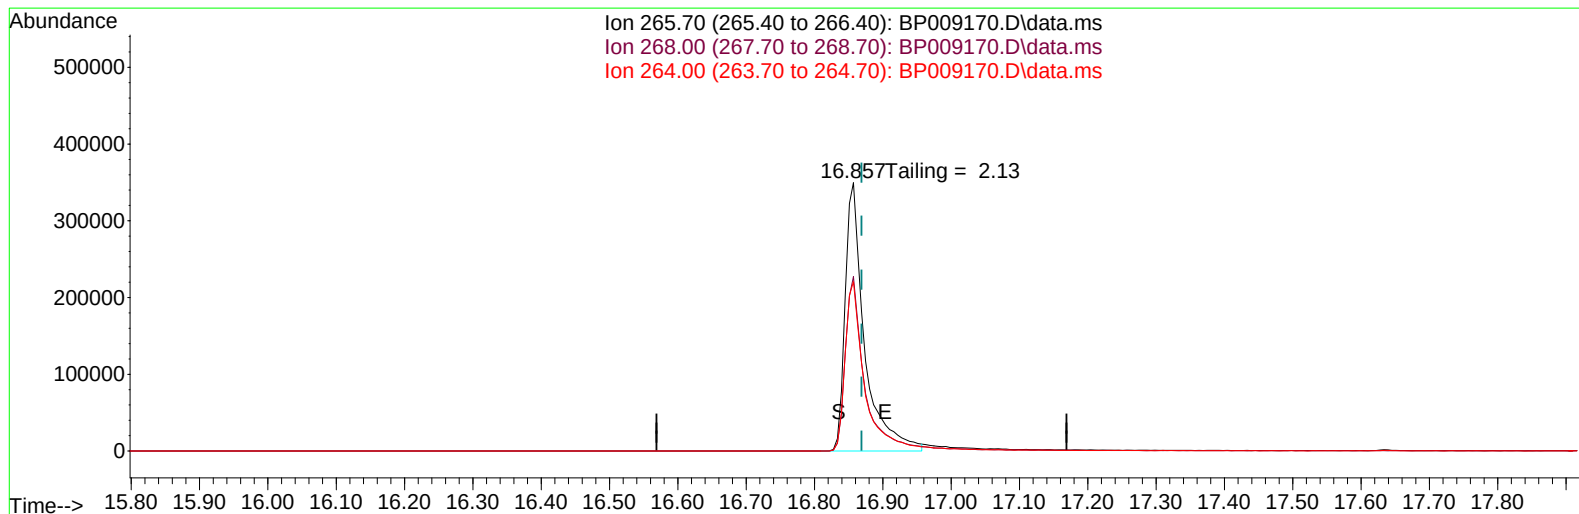

TIC: BP009170.D\data.ms

(70) Pentachlorophenol (C)

16.857min (-0.012) 2709870.60 ng




response 648259

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	64.98
264.00	62.90	63.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021622\
 Data File : BP009170.D
 Acq On : 16 Feb 2022 09:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Feb 16 14:26:29 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 16 01:29:44 2022
 Response via : Initial Calibration

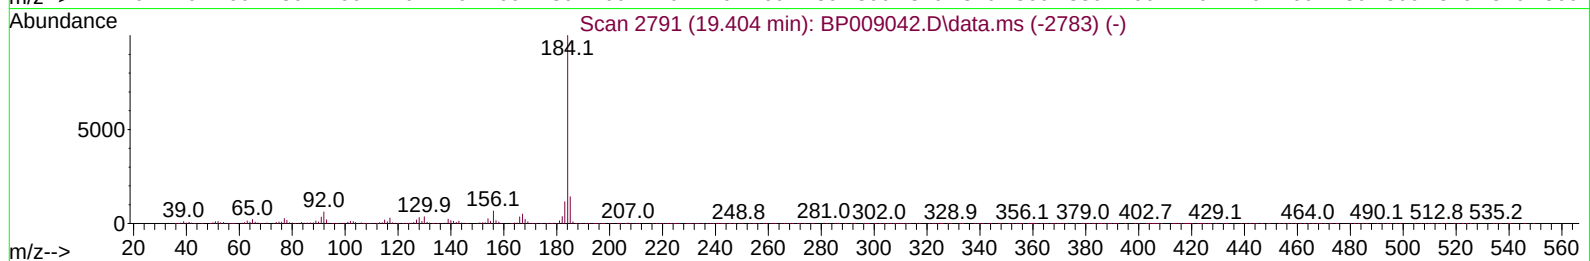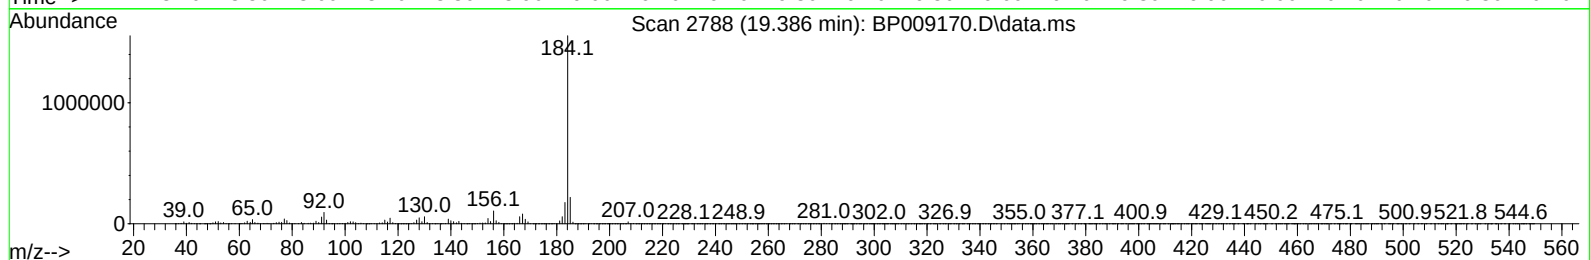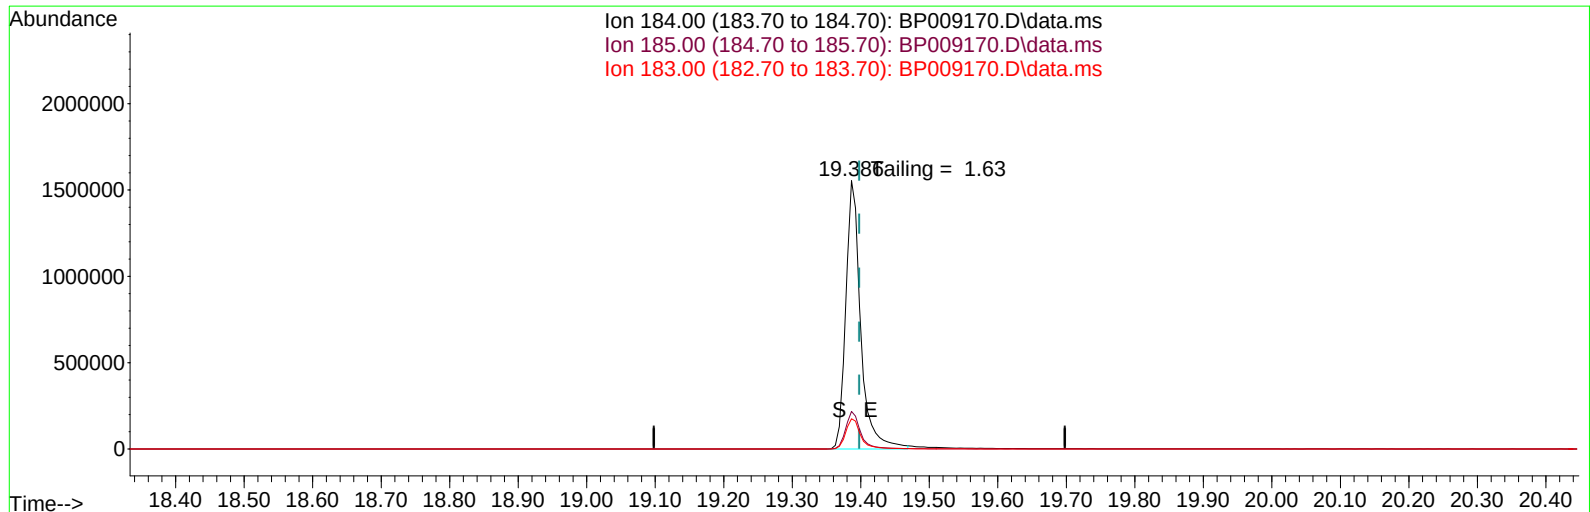

TIC: BP009170.D\data.ms

(77) Benzidine

19.386min (-0.012) 878172.77 ng

response 2165337

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.05
183.00	11.90	11.30
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/16/2022	BNA_P	<u>BP009170.D</u>
Compound Name	Response	Retention Time
DDT	1291846	20.58
DDD	16224	20.15
DDE	2189	19.66
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18413	1310259	1.41

Instrument :
BNA_P
ClientSampleId :
DFTPP