
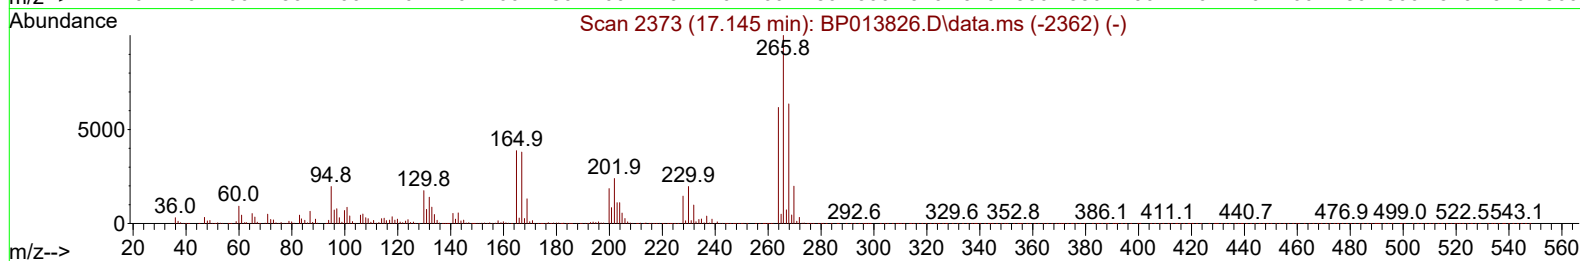
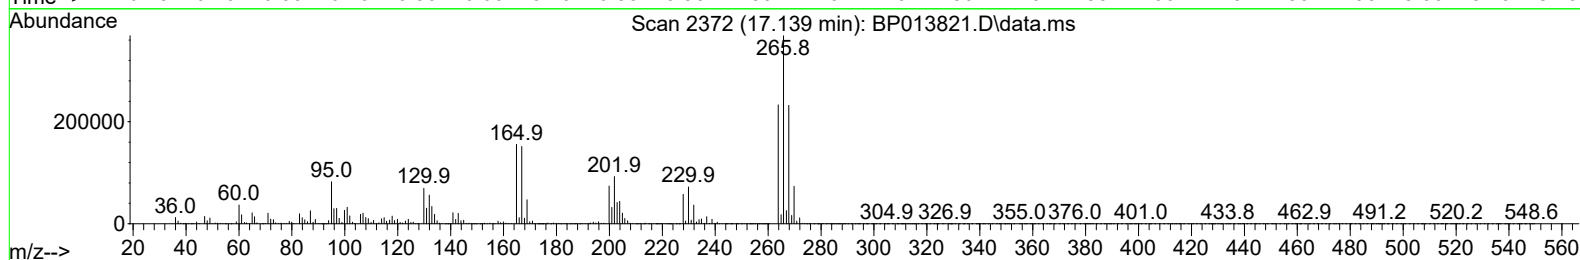


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021623\
Data File : BP013821.D
Acq On : 16 Feb 2023 11:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 17 07:27:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 01:08:52 2023
Response via : Initial Calibration

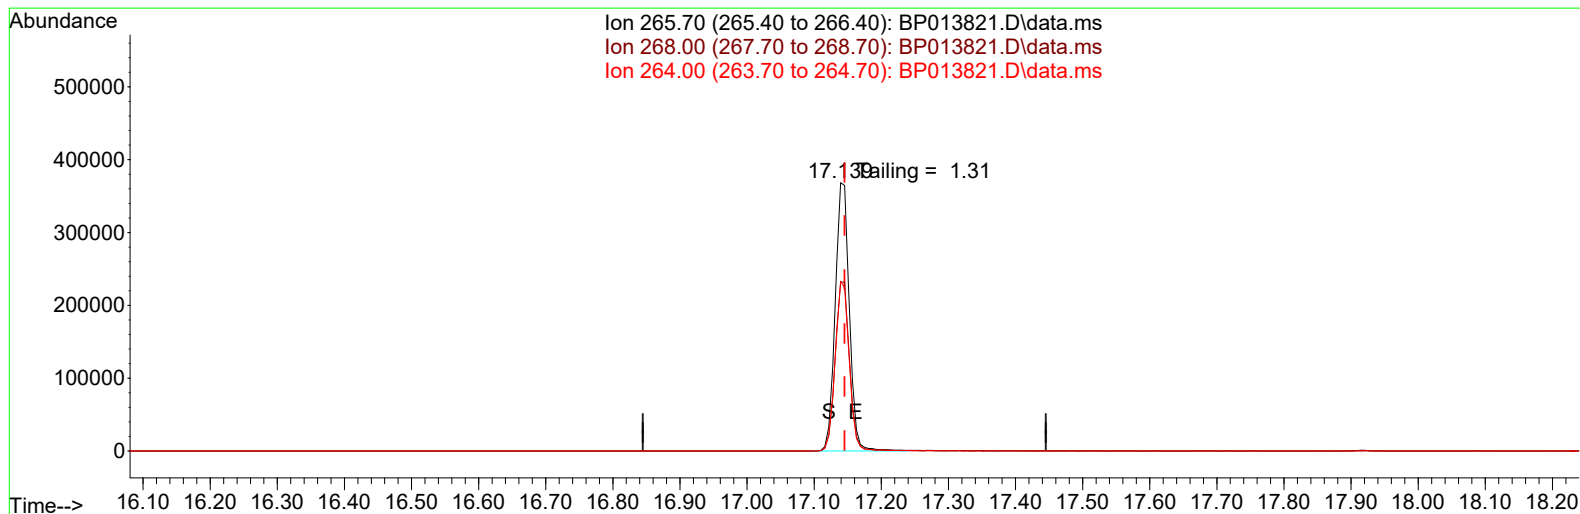

TIC: BP013821.D\data.ms

(70) Pentachlorophenol (C)




17.139min (-0.006) 4385192.38 ng

response 541522

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.01
264.00	61.70	63.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021623\
 Data File : BP013821.D
 Acq On : 16 Feb 2023 11:09
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 17 07:27:13 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 17 01:08:52 2023
 Response via : Initial Calibration

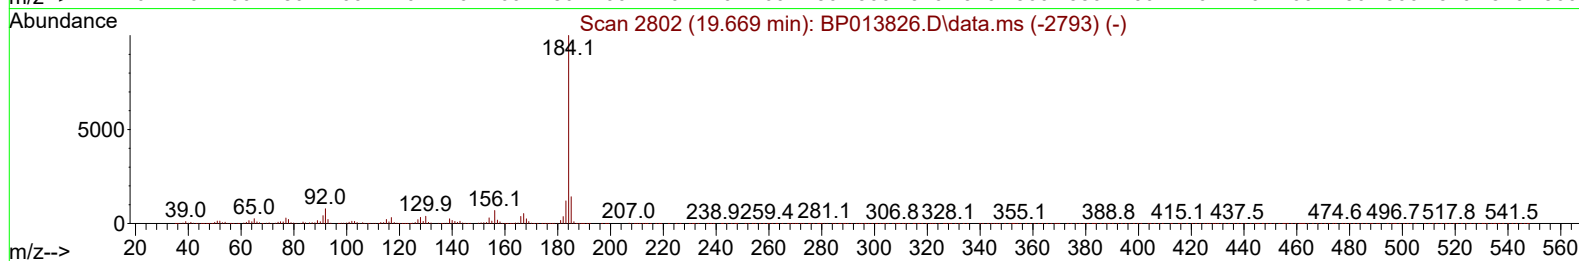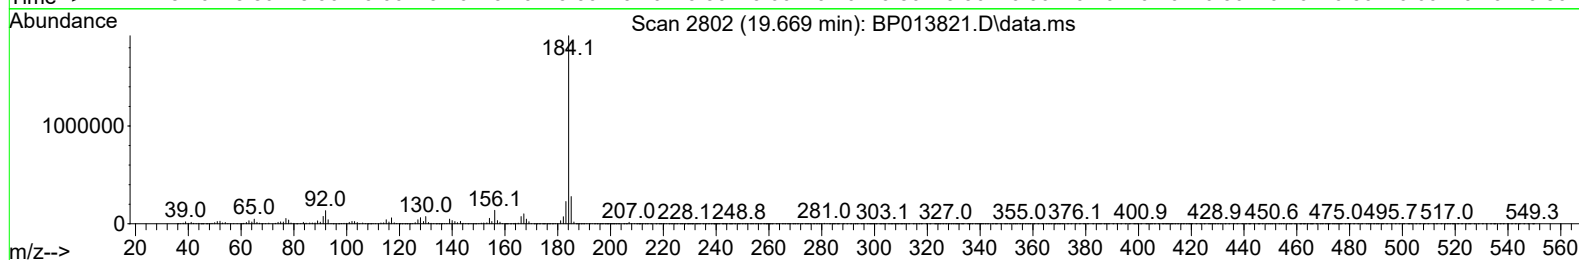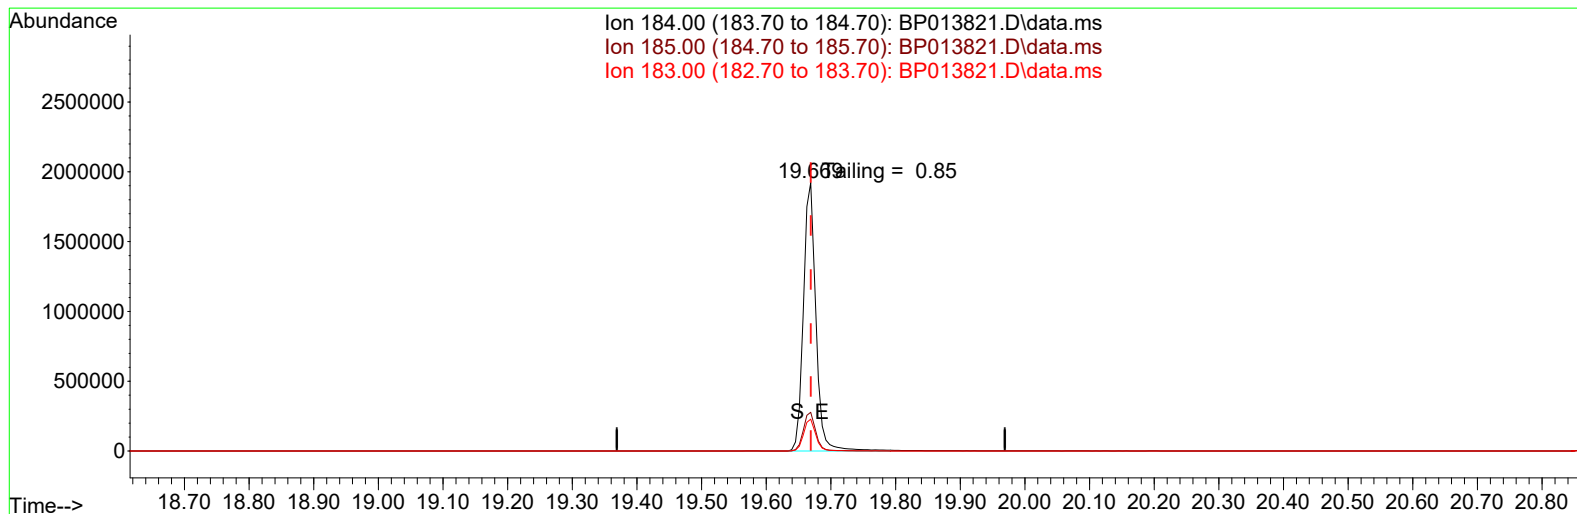

TIC: BP013821.D\data.ms

(77) Benzidine**19.669min (-0.000) 2614447.45 ng****response 2580467**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.44
183.00	12.00	11.87
0.00	0.00	0.00