
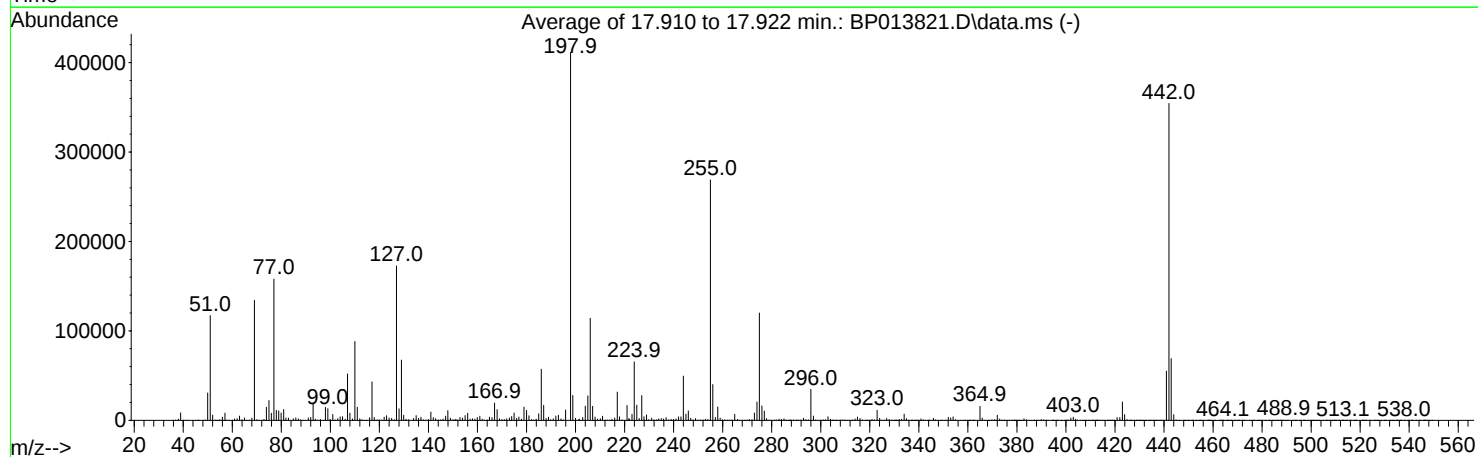


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021623\
 Data File : BP013821.D
 Acq On : 16 Feb 2023 11:09
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 17 01:08:52 2023

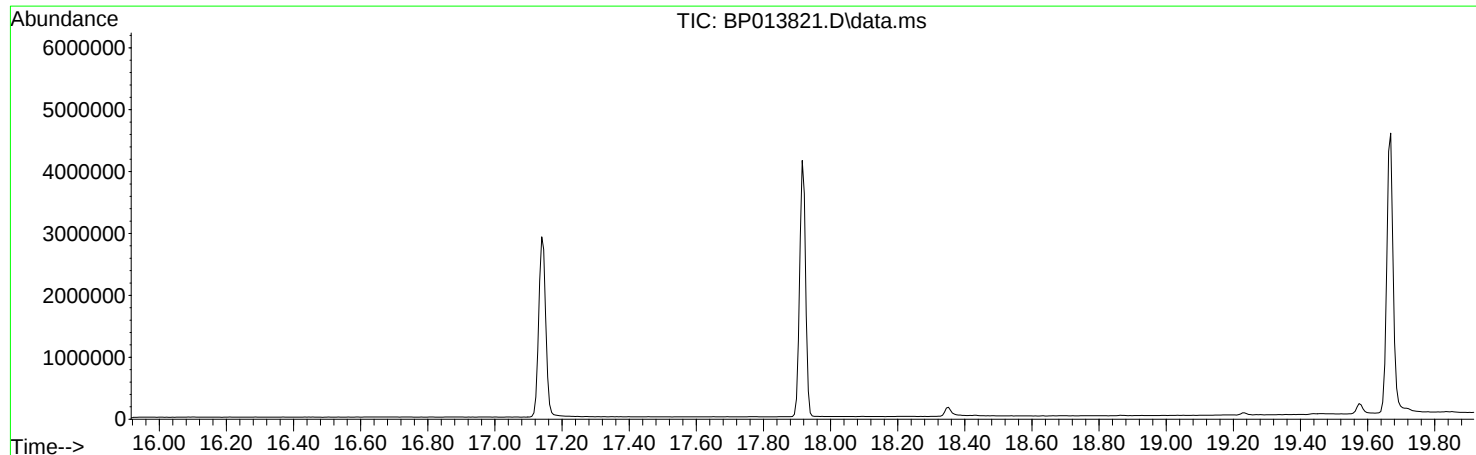




AutoFind: Scans 2503, 2504, 2505; Background Corrected with Scan 2494

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.5	117119	PASS
68	69	0.00	2	1.8	2349	PASS
69	198	0.00	100	32.6	134176	PASS
70	69	0.00	2	0.5	674	PASS
127	198	10	80	42.0	172595	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	411413	PASS
199	198	5	9	6.8	27825	PASS
275	198	10	60	29.1	119912	PASS
365	198	1	100	3.8	15646	PASS
441	198	0.01	100	13.4	55099	PASS
442	442	100	100	100.0	354453	PASS
443	442	15	24	19.4	68920	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021623\
Data File : BP013821.D
Acq On : 16 Feb 2023 11:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 17 07:27:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 01:08:52 2023
Response via : Initial Calibration

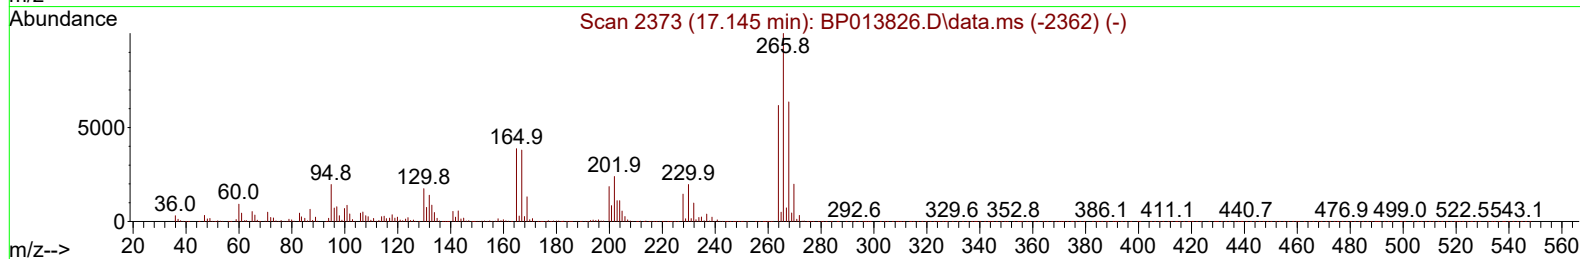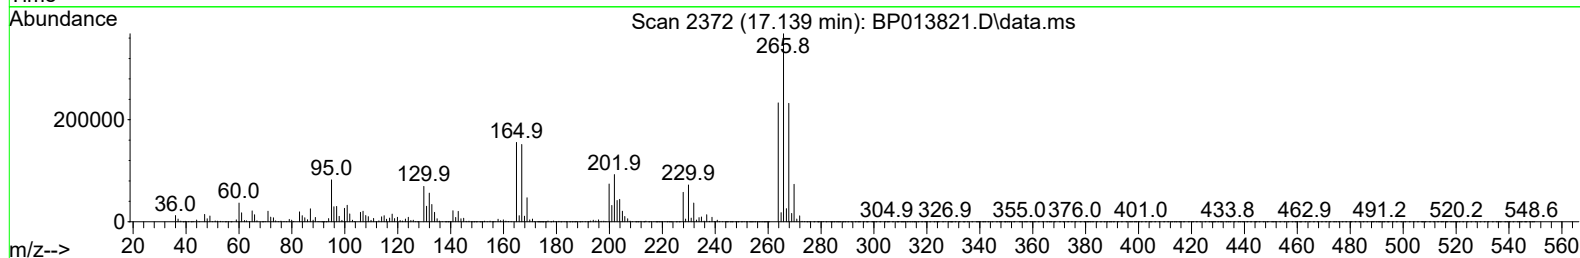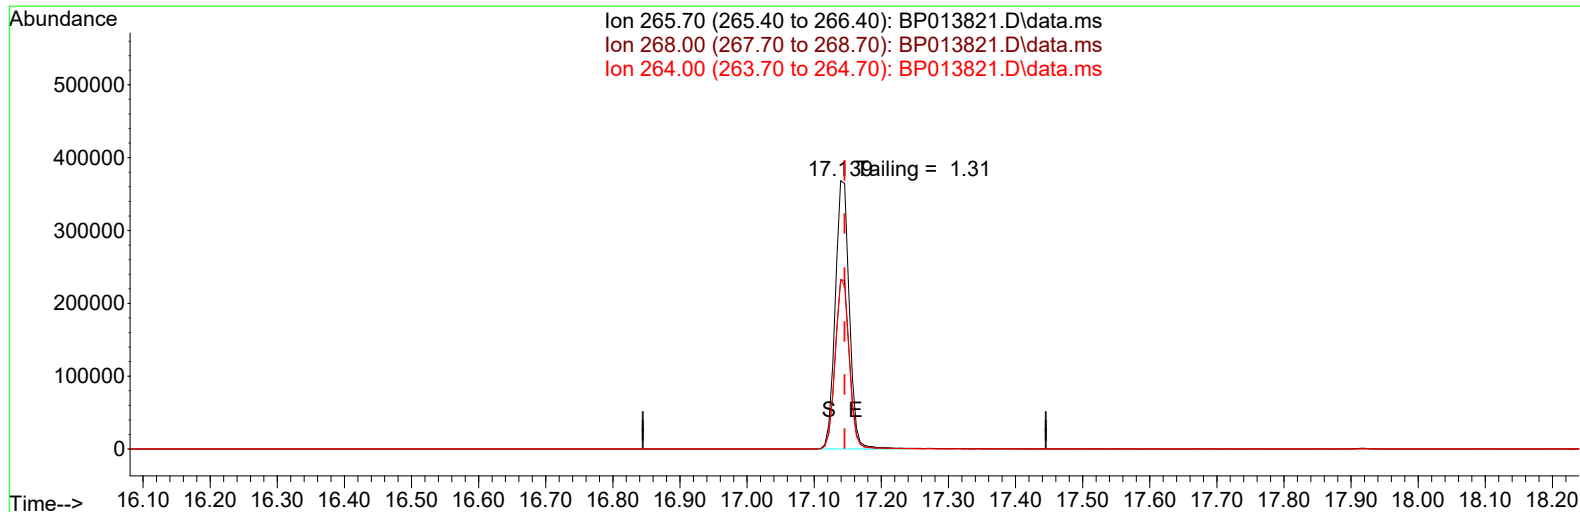

TIC: BP013821.D\data.ms

(70) Pentachlorophenol (C)

17.139min (-0.006) 4385192.38 ng




response 541522

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.01
264.00	61.70	63.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021623\
Data File : BP013821.D
Acq On : 16 Feb 2023 11:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 17 07:27:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 01:08:52 2023
Response via : Initial Calibration

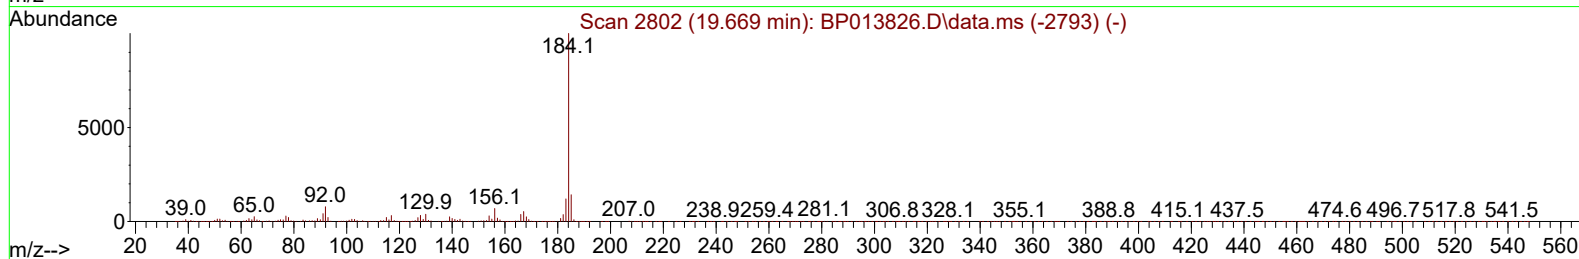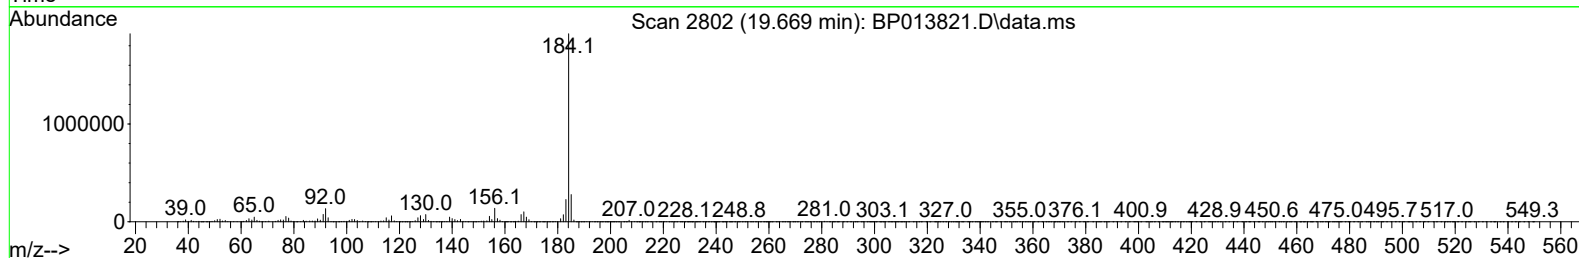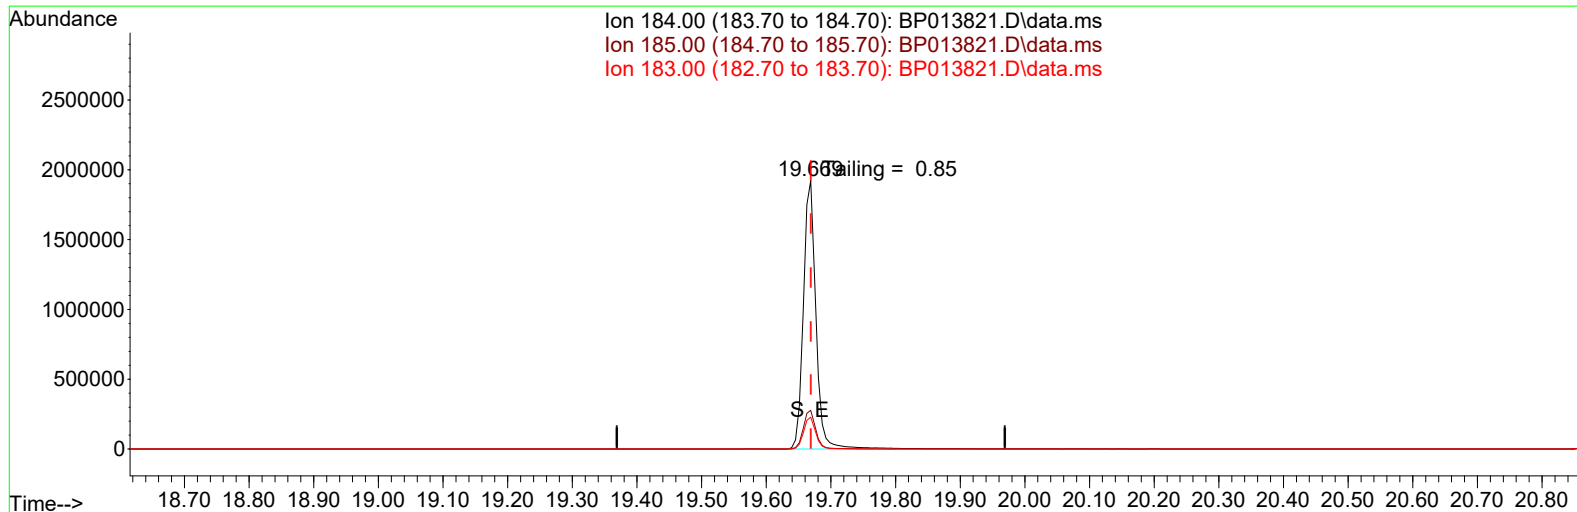

TIC: BP013821.D\data.ms

(77) Benzidine

19.669min (-0.000) 2614447.45 ng

response 2580467

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.44
183.00	12.00	11.87
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/16/2023	BNA_P	<u>BP013821.D</u>
Compound Name	Response	Retention Time
DDT	1393751	20.863
DDD	20323	20.486
DDE	885	19.945
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21208	1414959	1.50

Instrument :
BNA_P
ClientSampleId :
DFTPP