
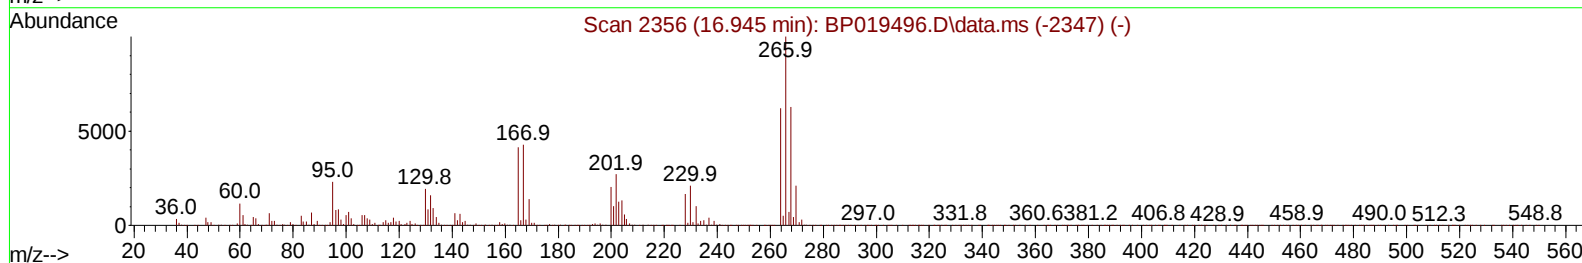
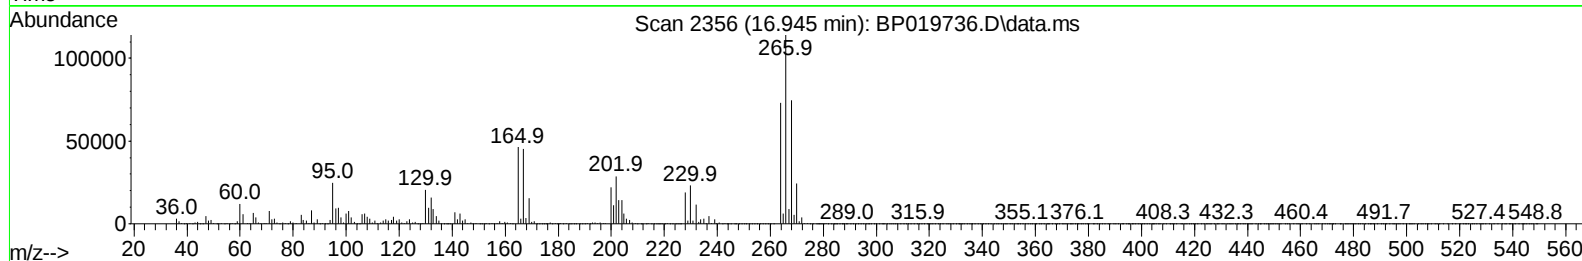


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021624\
Data File : BP019736.D
Acq On : 16 Feb 2024 09:53
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 19 01:04:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

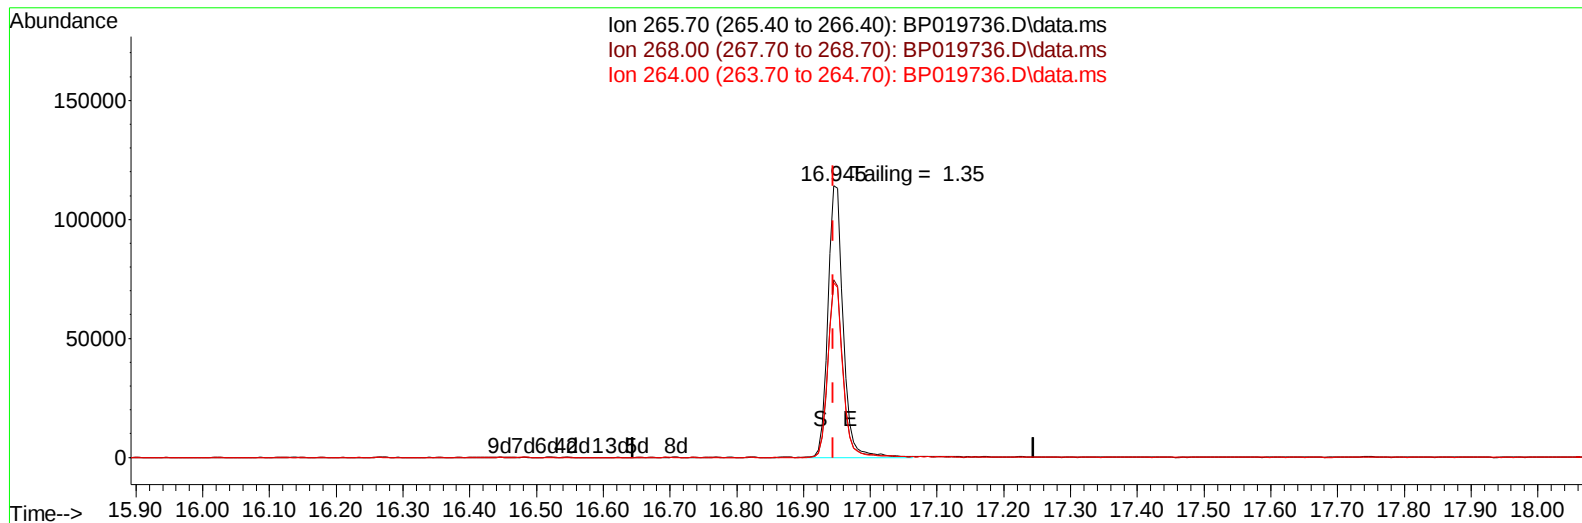

TIC: BP019736.D\data.ms

(70) Pentachlorophenol (C)




16.945min (+ 0.000) 130319.54 ng m

response 182453

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	65.44
264.00	62.10	64.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021624\
Data File : BP019736.D
Acq On : 16 Feb 2024 09:53
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 19 01:04:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

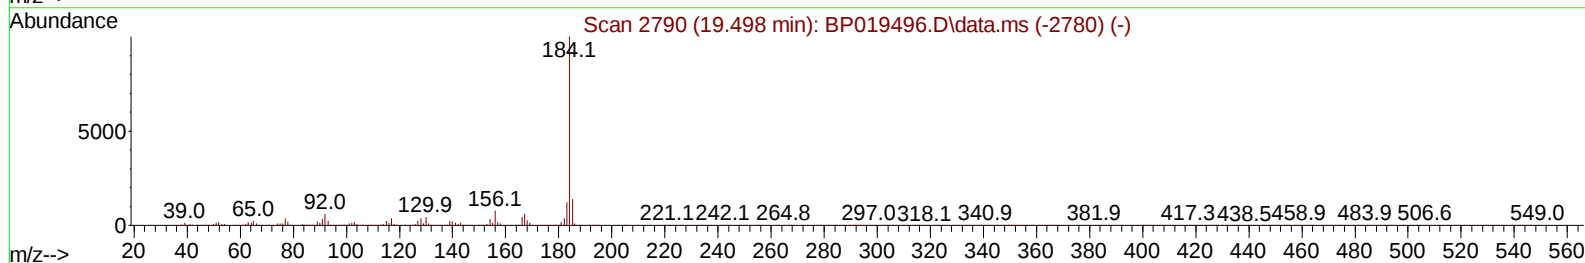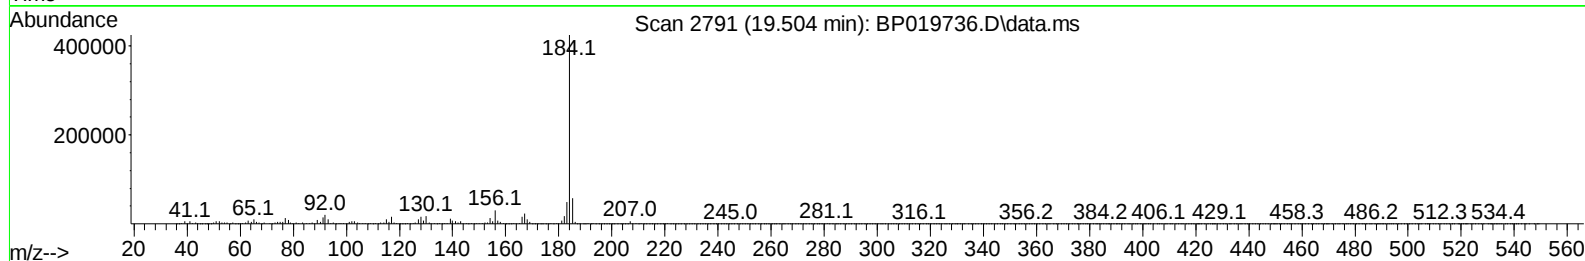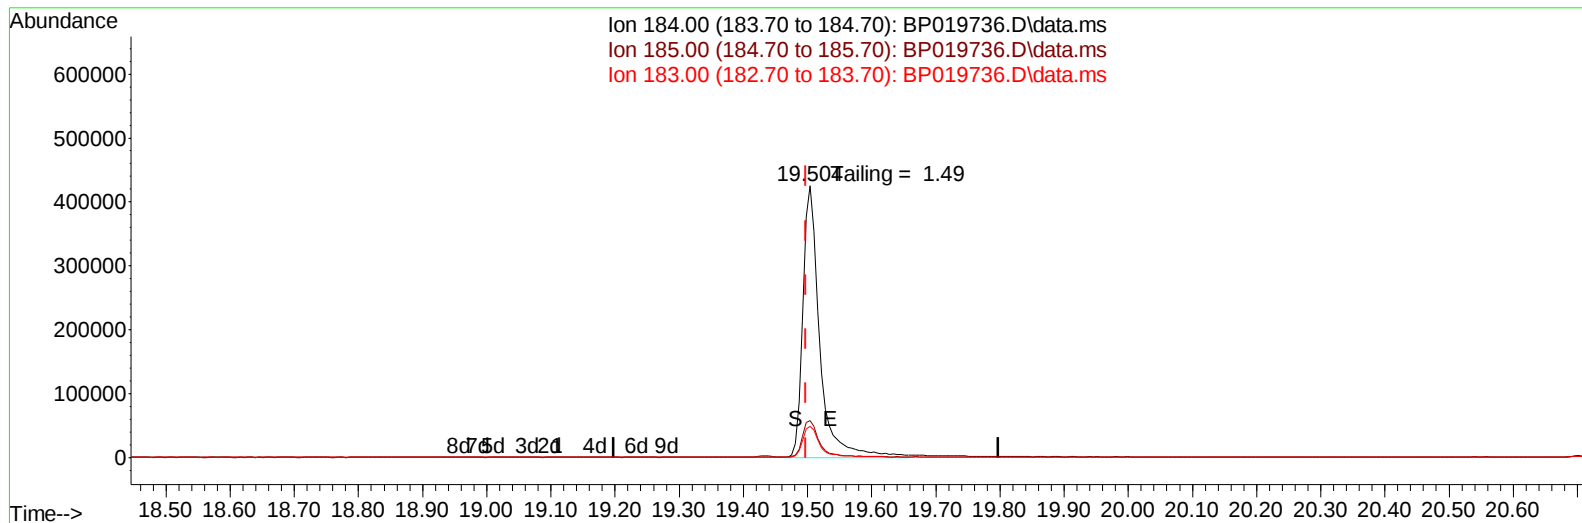

TIC: BP019736.D\data.ms

(77) Benzidine**19.504min (+ 0.006) 119449.31 ng m****response 789143**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.66
183.00	12.10	11.51
0.00	0.00	0.00