


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021624\
Data File : BP019736.D
Acq On : 16 Feb 2024 09:53
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 01 00:51:48 2024

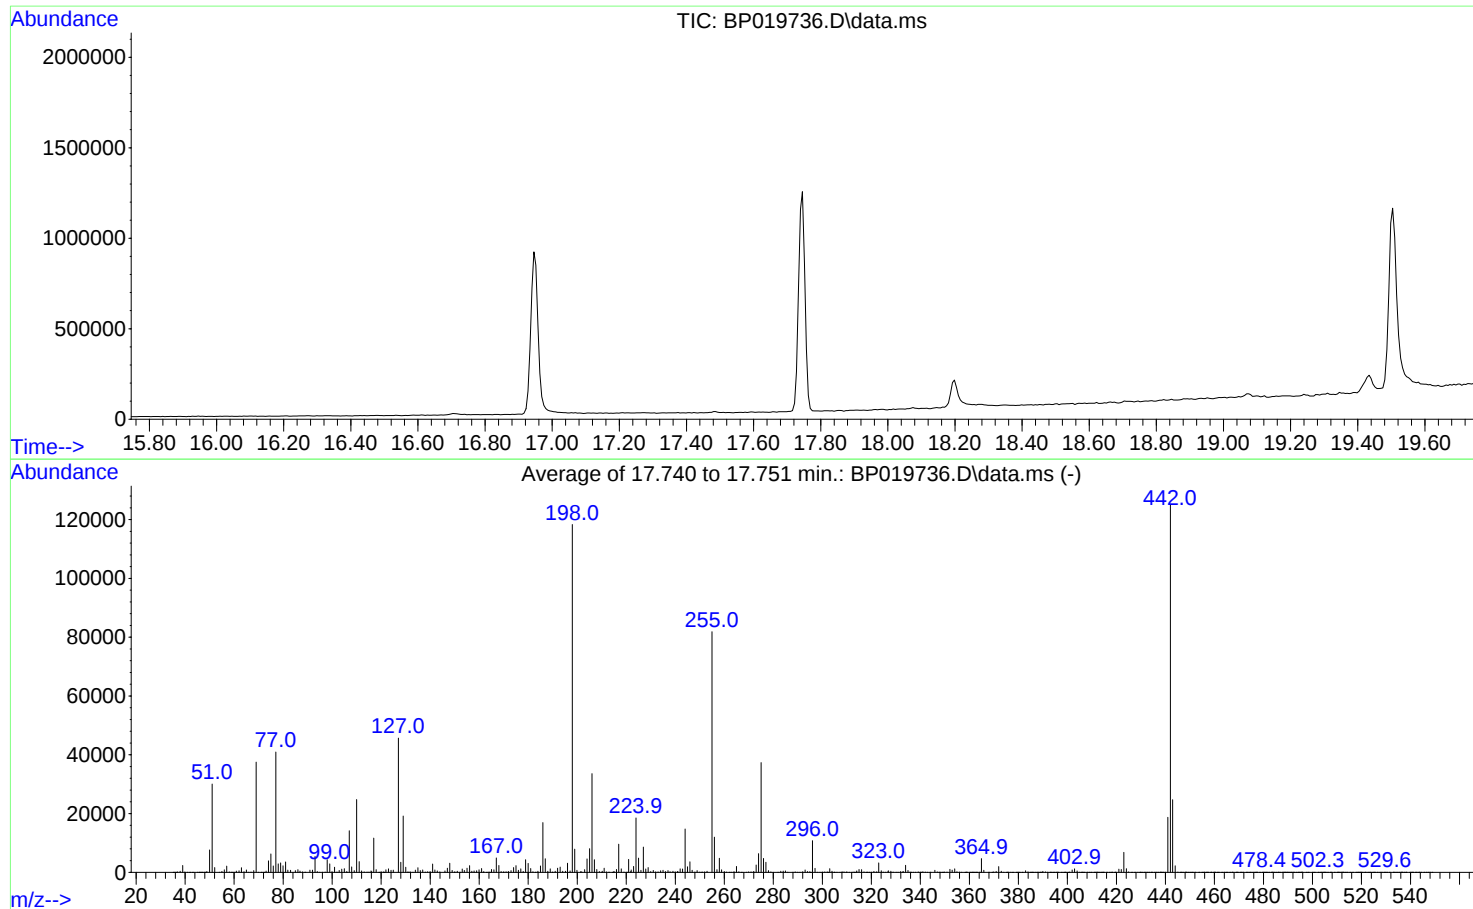




AutoFind: Scans 2491, 2492, 2493; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.4	30018	PASS
68	69	0.00	2	1.7	620	PASS
69	198	0.00	100	31.7	37488	PASS
70	69	0.00	2	0.1	56	PASS
127	198	10	80	38.6	45661	PASS
197	198	0.00	2	0.4	483	PASS
198	198	100	100	100.0	118316	PASS
199	198	5	9	6.7	7892	PASS
275	198	10	60	31.5	37320	PASS
365	198	1	100	4.0	4704	PASS
441	198	0.01	100	15.8	18707	PASS
442	442	100	100	100.0	125125	PASS
443	442	15	24	19.8	24738	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021624\
Data File : BP019736.D
Acq On : 16 Feb 2024 09:53
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 19 01:04:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

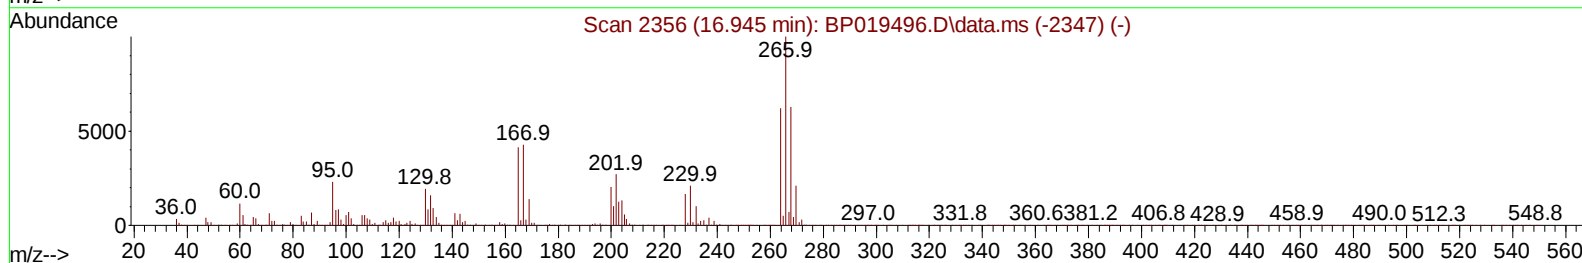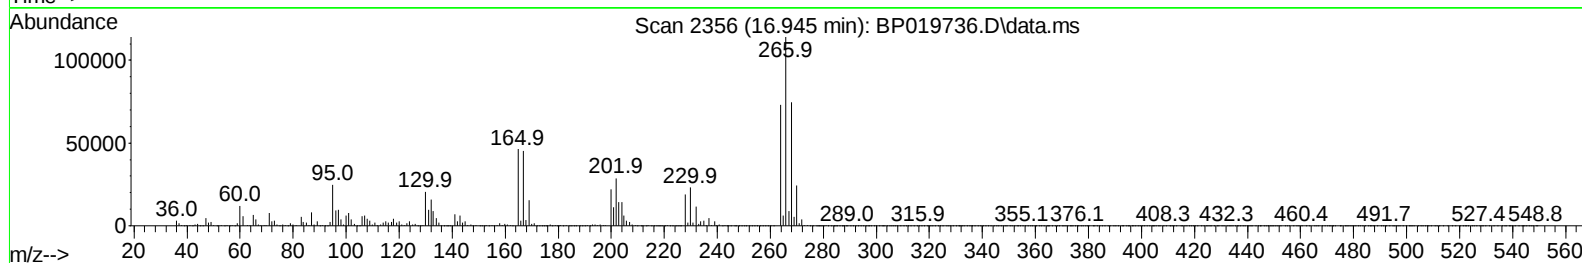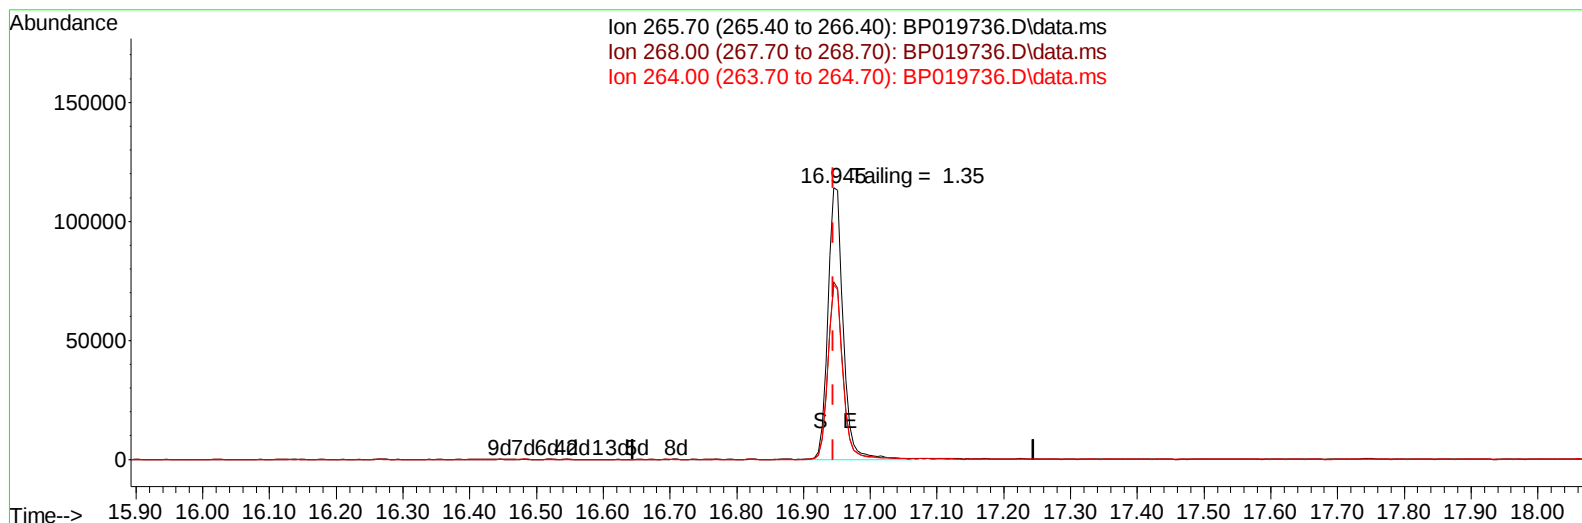

TIC: BP019736.D\data.ms

(70) Pentachlorophenol (C)

16.945min (+ 0.000) 130319.54 ng m




response 182453

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	65.44
264.00	62.10	64.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021624\
Data File : BP019736.D
Acq On : 16 Feb 2024 09:53
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 19 01:04:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 00:51:48 2024
Response via : Initial Calibration

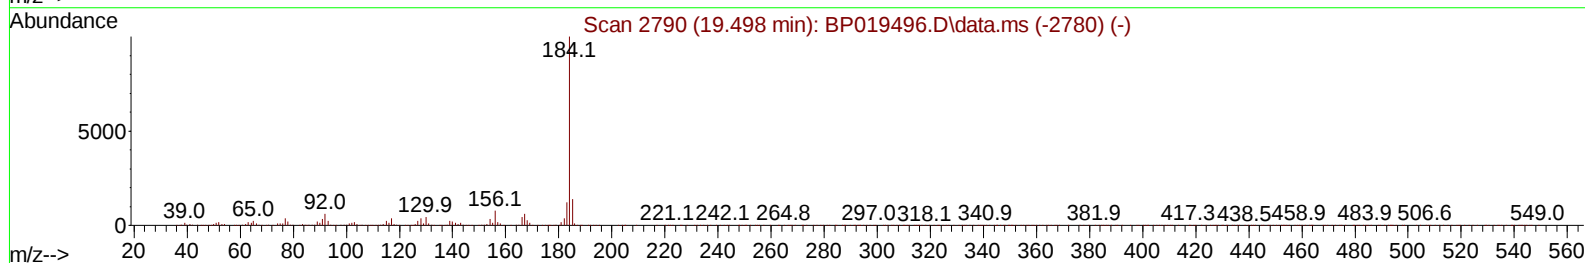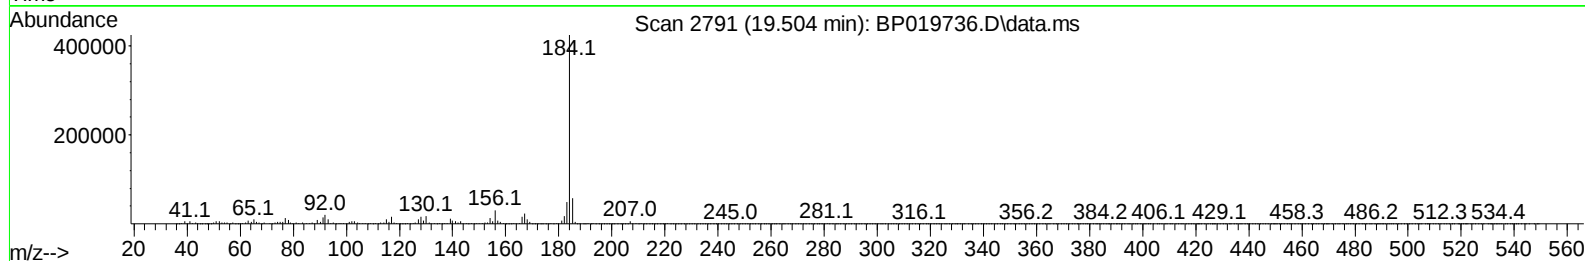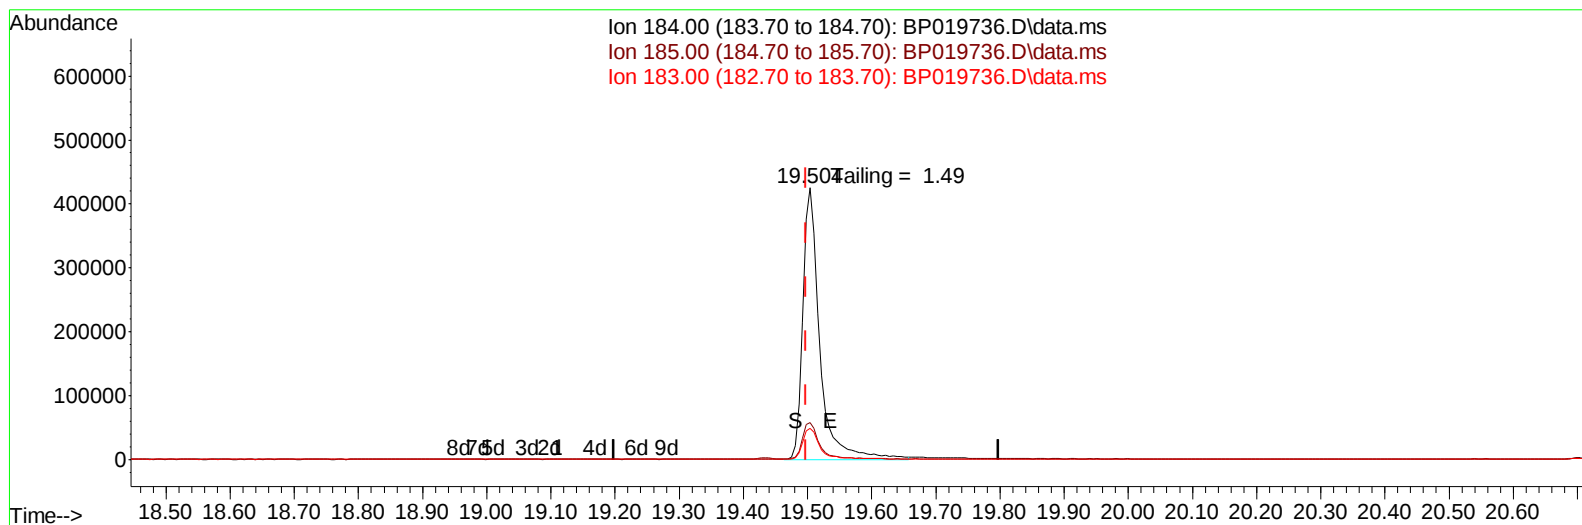

TIC: BP019736.D\data.ms

(77) Benzidine

19.504min (+ 0.006) 119449.31 ng m

response 789143

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.66
183.00	12.10	11.51
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/16/2024	BNA_P	<u>BP019736.D</u>
Compound Name	Response	Retention Time
DDT	456620	20.698
DDD	14062	20.268
DDE	2454	19.768
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16516	473136	3.49

Instrument :
BNA_P
ClientSampleId :
DFTPP