


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP021721\
Data File : BP004773.D
Acq On : 17 Feb 2021 15:12
Operator : CG/JU
Sample : M1407-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBGK0

Manual Integrations
APPROVED

mohammad
2/18/2021 1:40:05 PM

Quant Time: Feb 17 16:37:09 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 15 12:16:19 2021
Response via : Initial Calibration

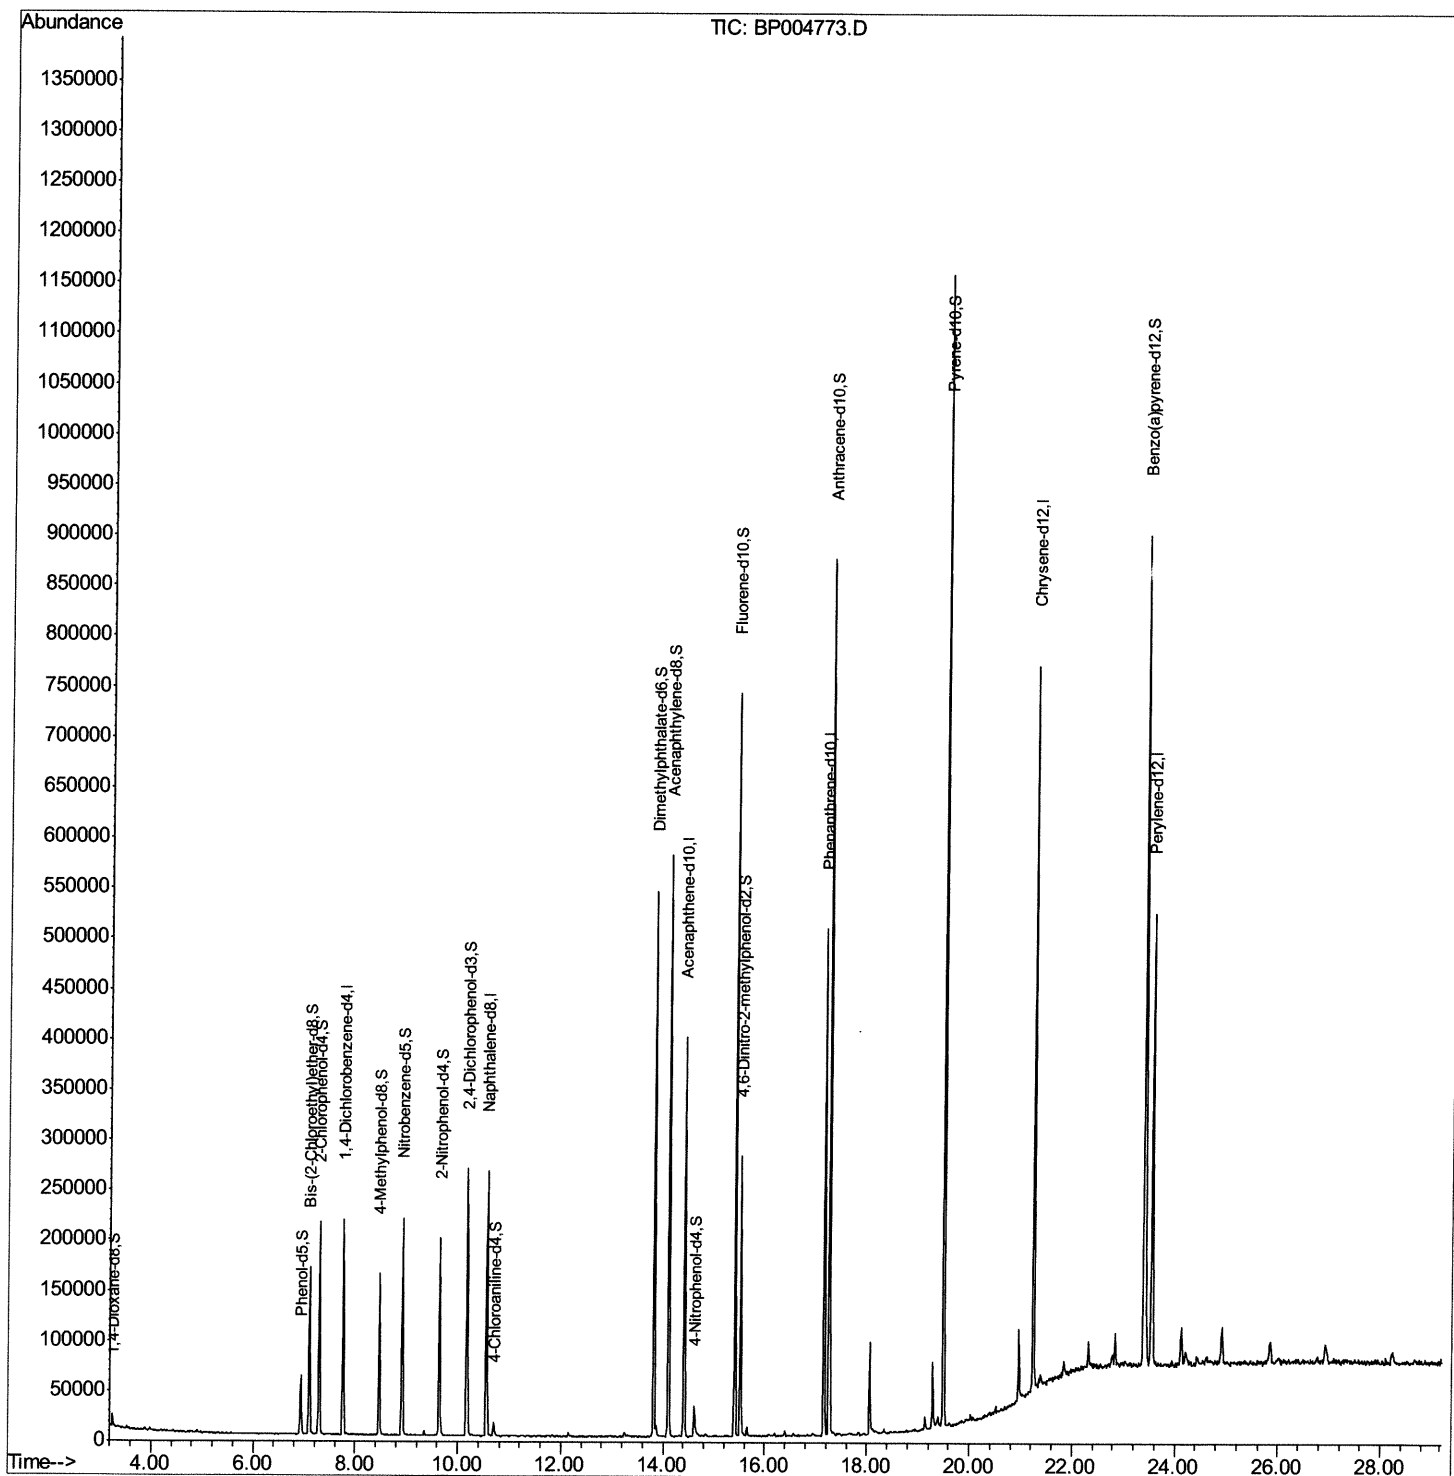

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP021721\
 Data File : BP004773.D
 Acq On : 17 Feb 2021 15:12
 Operator : CG/JU
 Sample : M1407-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
ClientSampleId :
 DBGK0

Manual Integrations
APPROVED

mohammad
 2/18/2021 1:40:05 PM

Quant Time: Feb 17 16:35:58 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Feb 15 12:16:19 2021
 Response via : Initial Calibration

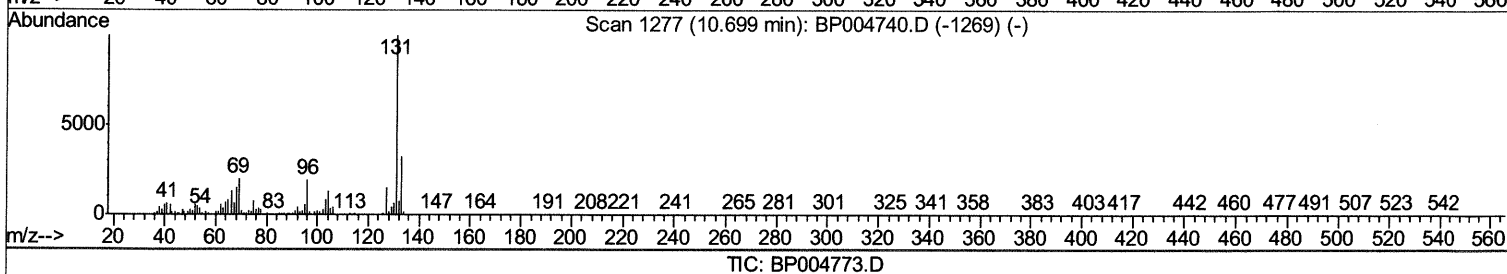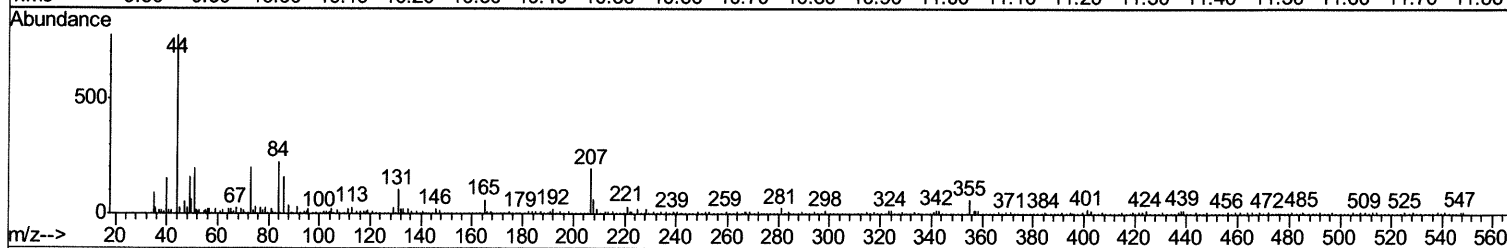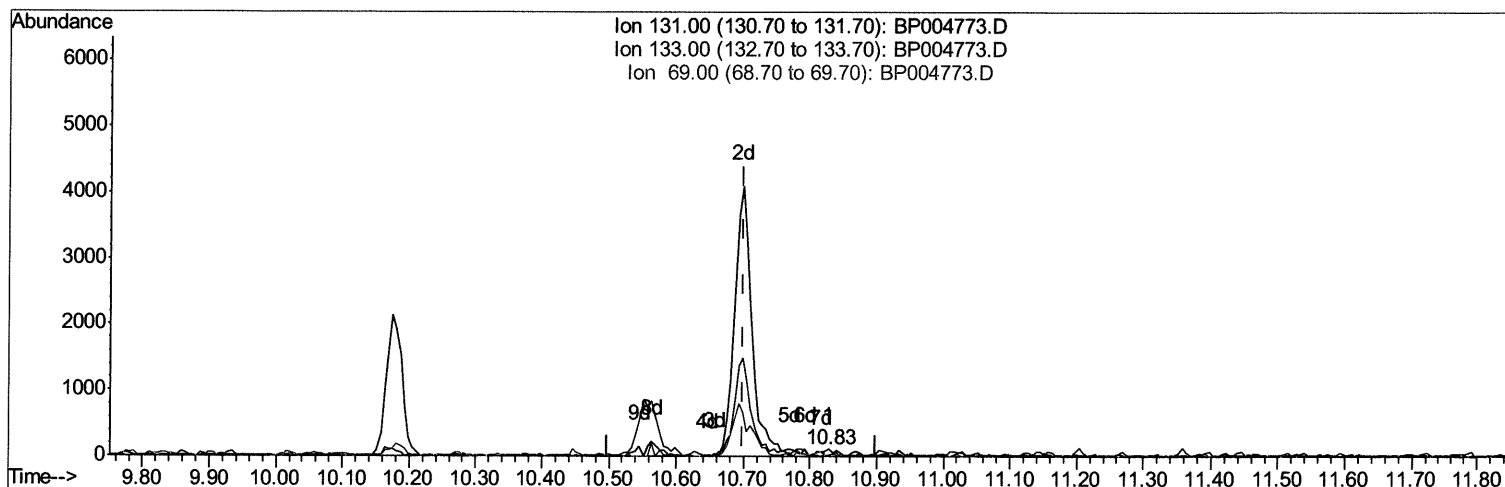

TIC: BP004773.D

(29) 4-Chloroaniline-d4 (S)

10.828min (+0.129) 0.02ng/ul

response 74

Ion	Exp%	Act%
131.00	100	100
133.00	31.20	26.42
69.00	20.50	19.81
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP021721\
 Data File : BP004773.D
 Acq On : 17 Feb 2021 15:12
 Operator : CG/JU
 Sample : M1407-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBGK0

Manual Integrations
 APPROVED

mohammad
 2/18/2021 1:40:05 PM

Quant Time: Feb 17 16:35:58 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Feb 15 12:16:19 2021
 Response via : Initial Calibration

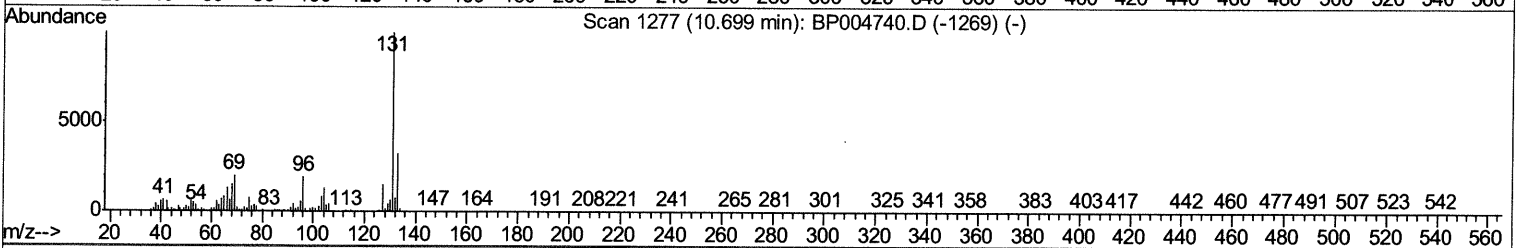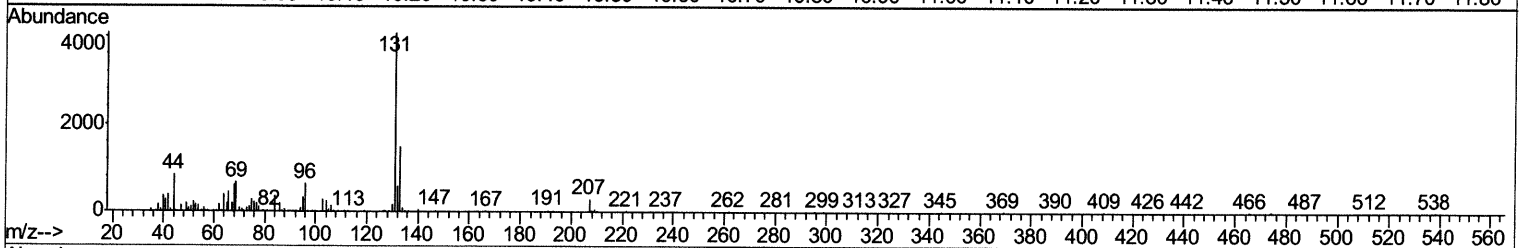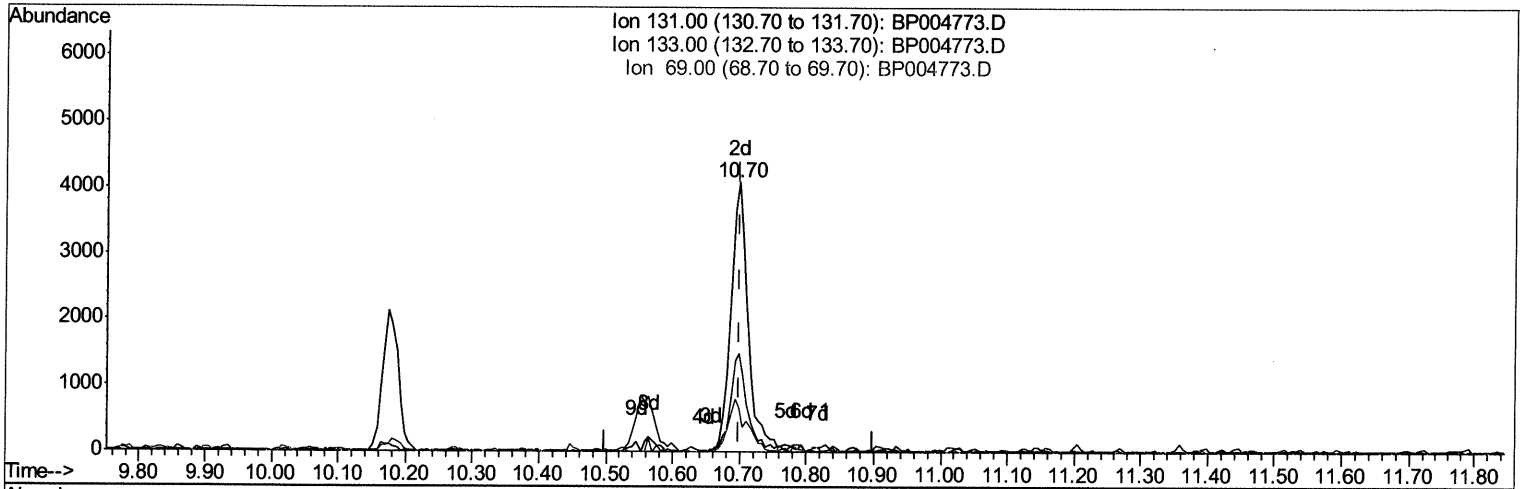

TIC: BP004773.D

(29) 4-Chloroaniline-d4 (S)

10.699min (-0.000) 2.17ng/ul m 02/22/21 JU

response 7380

Ion	Exp%	Act%
131.00	100	100
133.00	31.20	36.31
69.00	20.50	16.17#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021721\
 Data File : BP004773.D
 Acq On : 17 Feb 2021 15:12
 Operator : CG/JU
 Sample : M1407-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBGK0

Manual Integrations
 APPROVED

mohammad
 2/18/2021 1:40:05 PM

Quant Time: Feb 17 16:37:09 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Feb 15 12:16:19 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.76	152	52846	20.00	ng/ul	0.00
18) Naphthalene-d8	10.56	136	200173	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.41	164	126979	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.16	188	280398	20.00	ng/ul	0.00
78) Chrysene-d12	21.25	240	313121	20.00	ng/ul	-0.01
86) Perylene-d12	23.54	264	321870	20.00	ng/ul	-0.02

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.25	96	6633	4.85	ng/uL	0.00
5) Phenol-d5	6.93	99	31350	7.39	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.10	67	65560	29.76	ng/ul	0.00
9) 2-Chlorophenol-d4	7.30	132	85445	26.58	ng/ul	0.00
13) 4-Methylphenol-d8	8.47	113	54354	16.29	ng/ul	0.00
19) Nitrobenzene-d5	8.92	128	47295	34.22	ng/ul	0.00
22) 2-Nitrophenol-d4	9.64	143	54402	35.87	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.18	165	89630	29.36	ng/ul	0.00
29) 4-Chloroaniline-d4	10.70	131	7380m>	2.17	ng/ul>	0.00
44) Dimethylphthalate-d6	13.82	166	321274	34.85	ng/ul	0.00
47) Acenaphthylene-d8	14.10	160	381187	33.99	ng/ul	0.00
52) 4-Nitrophenol-d4	14.61	143	8087	5.02	ng/ul	0.00
58) Fluorene-d10	15.40	176	278701	35.29	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.52	200	55260	32.60	ng/ul	0.00
71) Anthracene-d10	17.26	188	465682	37.66	ng/ul	0.00
79) Pyrene-d10	19.50	212	554126	37.80	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.40	264	617630	37.93	ng/ul	-0.02

02/22/21JU

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed