

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP021721\
 Data File : BP004768.D
 Acq On : 17 Feb 2021 12:23
 Operator : CG/JU
 Sample : M1349-18DL 100X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBGQ5DL

Quant Time: Feb 18 06:39:09 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Feb 15 12:16:19 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.76	152	44929	20.00	ng/ul	0.00
18) Naphthalene-d8	10.56	136	169051	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.41	164	100816	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.16	188	202699	20.00	ng/ul	0.00
78) Chrysene-d12	21.25	240	243962	20.00	ng/ul	-0.01
86) Perylene-d12	23.55	264	254149	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	0.00	96	0d	0.00	ng/uL	
5) Phenol-d5	0.00	99	0d	0.00	ng/ul	
7) Bis-(2-Chloroethyl)ether-d	7.11	67	482	0.26	ng/ul	0.01
9) 2-Chlorophenol-d4	7.30	132	778	0.28	ng/ul	0.00
13) 4-Methylphenol-d8	8.48	113	346	0.12	ng/ul	0.01
19) Nitrobenzene-d5	8.93	128	312	0.27	ng/ul	0.00
22) 2-Nitrophenol-d4	0.00	143	0d	0.00	ng/ul	
26) 2,4-Dichlorophenol-d3	0.00	165	0d	0.00	ng/ul	
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul	
44) Dimethylphthalate-d6	13.83	166	2628	0.36	ng/ul	0.00
47) Acenaphthylene-d8	14.10	160	2728	0.31	ng/ul	0.00
52) 4-Nitrophenol-d4	0.00	143	0d	0.00	ng/ul	
58) Fluorene-d10	15.40	176	2060	0.33	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	0.00	200	0d	0.00	ng/ul	
71) Anthracene-d10	17.26	188	4815	0.54	ng/ul	0.00
79) Pyrene-d10	19.50	212	3992	0.35	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.40	264	4611	0.36	ng/ul	-0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
41) 1,1'-Biphenyl	13.24	154	183284	24.661	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP021721\
Data File : BP004768.D
Acq On : 17 Feb 2021 12:23
Operator : CG/JU
Sample : M1349-18DL 100X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBGQ5DL

Quant Time: Feb 18 06:39:09 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 15 12:16:19 2021
Response via : Initial Calibration

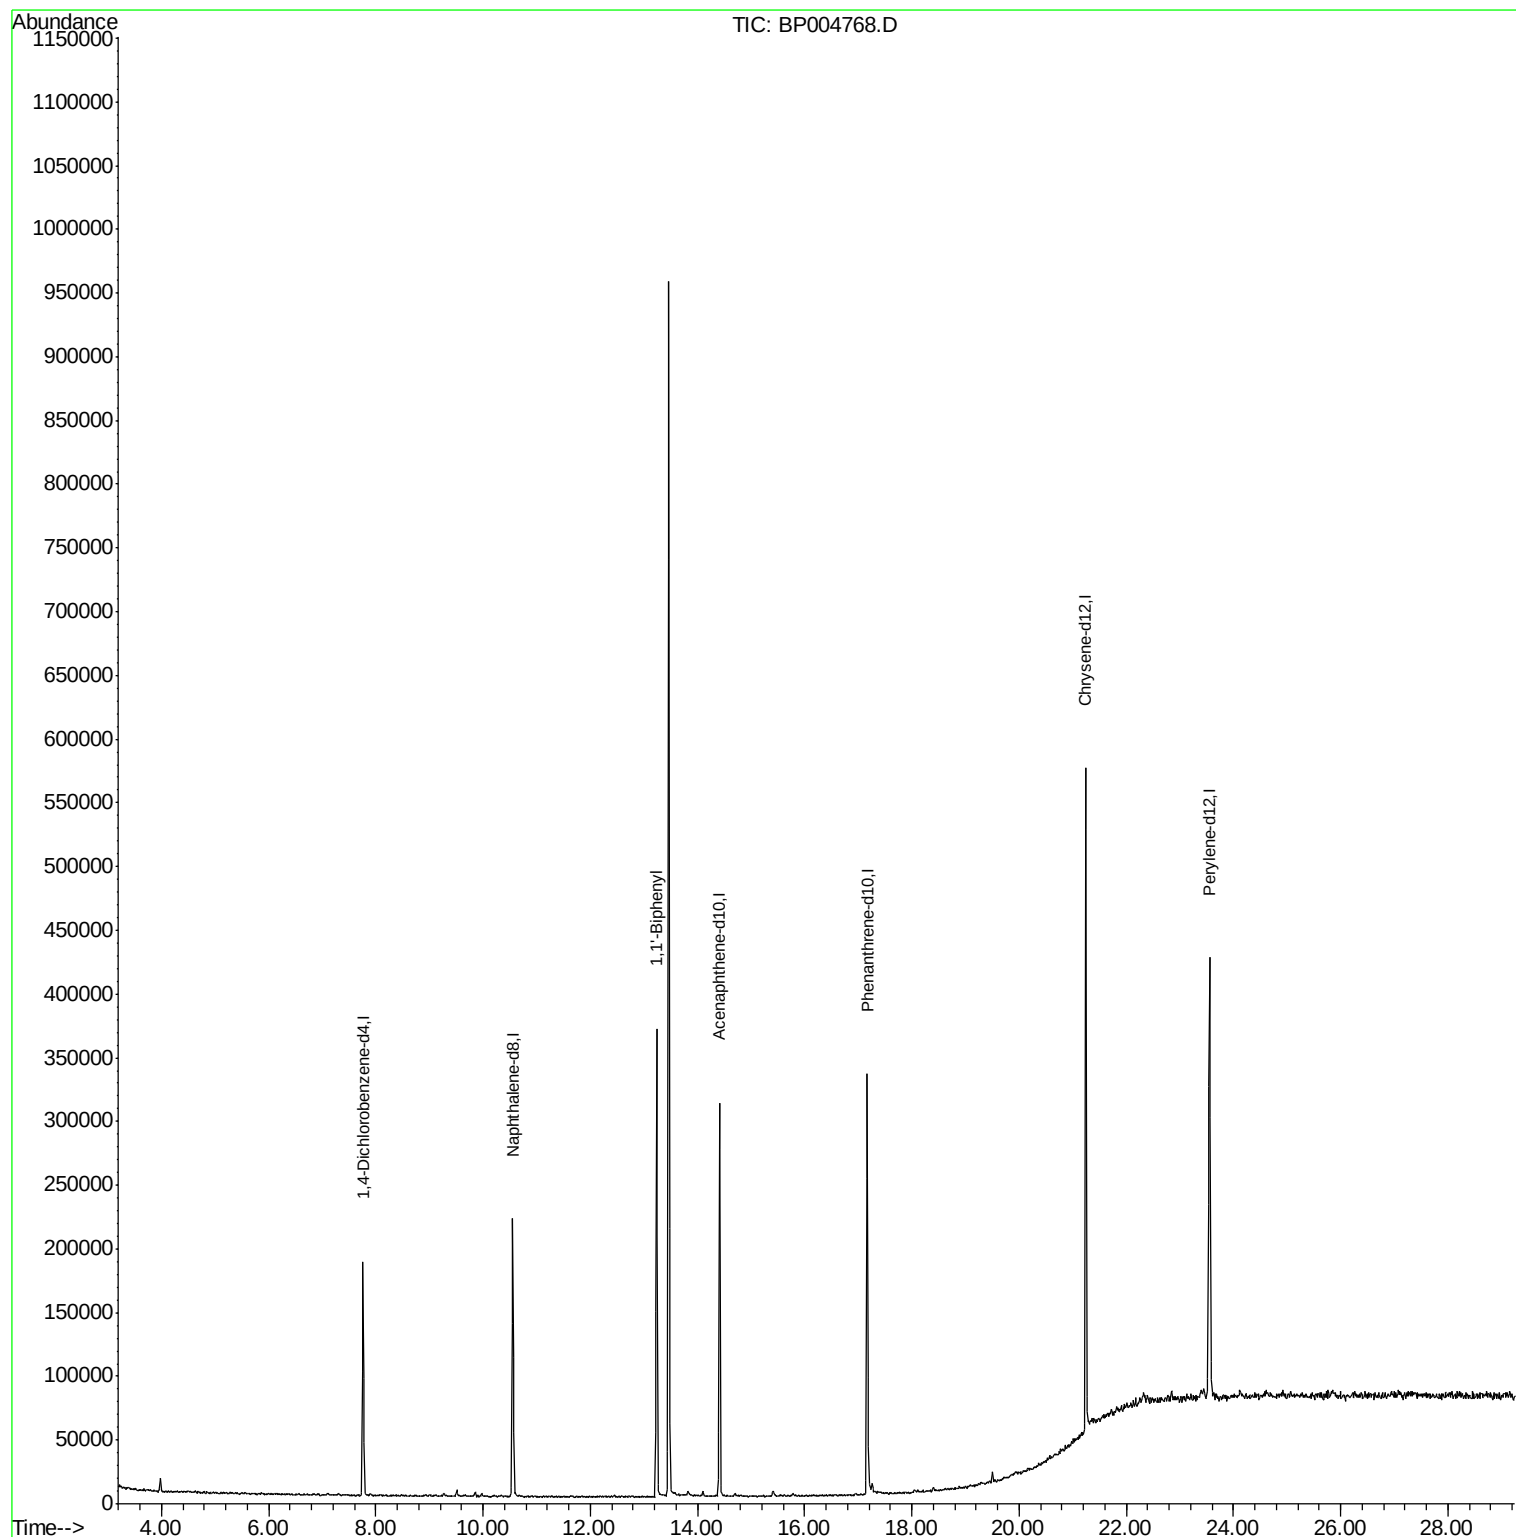

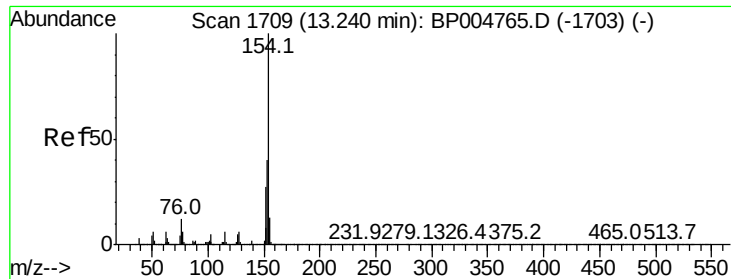

#41
 1,1'-Biphenyl
 Concen: 24.661 ng/ul
 RT: 13.24 min Scan# 1709
 Delta R.T. -0.01 min
 Lab File: BP004768.D
 Acq: 17 Feb 2021 12:23

Instrument :
 BNA_P
 ClientSampleId :
 DBGQ5DL

Tot Ion	Ratio	Lower	Upper
154	100		
153	40.5	32.3	48.5
76	11.6	8.8	13.2

