

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP021721\
 Data File : BP004781.D
 Acq On : 17 Feb 2021 19:42
 Operator : CG/JU
 Sample : M1379-06
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBGY6

Quant Time: Feb 17 23:29:05 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 17 23:17:49 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.76	152	49665	20.00	ng/ul	0.00
18) Naphthalene-d8	10.56	136	188053	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.41	164	107700	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.17	188	228786	20.00	ng/ul	0.00
78) Chrysene-d12	21.25	240	251239	20.00	ng/ul	0.00
86) Perylene-d12	23.56	264	263492	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.25	96	2758	2.15	ng/uL	0.00
5) Phenol-d5	6.95	99	45615	11.44	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	7.10	67	24857	12.01	ng/ul	0.00
9) 2-Chlorophenol-d4	7.30	132	39410	13.05	ng/ul	0.00
13) 4-Methylphenol-d8	8.48	113	35134	11.20	ng/ul	0.01
19) Nitrobenzene-d5	8.92	128	17344	13.36	ng/ul	0.00
22) 2-Nitrophenol-d4	9.64	143	20400	14.32	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.19	165	35462	12.36	ng/ul	0.00
29) 4-Chloroaniline-d4	10.70	131	39171	12.23	ng/ul	0.00
44) Dimethylphthalate-d6	13.82	166	114104	14.59	ng/ul	0.00
47) Acenaphthylene-d8	14.10	160	134519	14.14	ng/ul	0.00
52) 4-Nitrophenol-d4	14.63	143	14859	10.88	ng/ul	0.02
58) Fluorene-d10	15.41	176	93623	13.98	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.53	200	16263	11.76	ng/ul	0.00
71) Anthracene-d10	17.26	188	163488	16.20	ng/ul	0.00
79) Pyrene-d10	19.50	212	208994	17.77	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.41	264	238218	17.87	ng/ul	0.00

Target Compounds


				Ovalue	
14) Acetophenone	8.59	105	5705	1.106	ng/ul 94
84) Bis(2-ethylhexyl)phthalate	21.16	149	10507	1.290	ng/ul# 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP021721\
Data File : BP004781.D
Acq On : 17 Feb 2021 19:42
Operator : CG/JU
Sample : M1379-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBGY6

Quant Time: Feb 17 23:29:05 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 17 23:17:49 2021
Response via : Initial Calibration




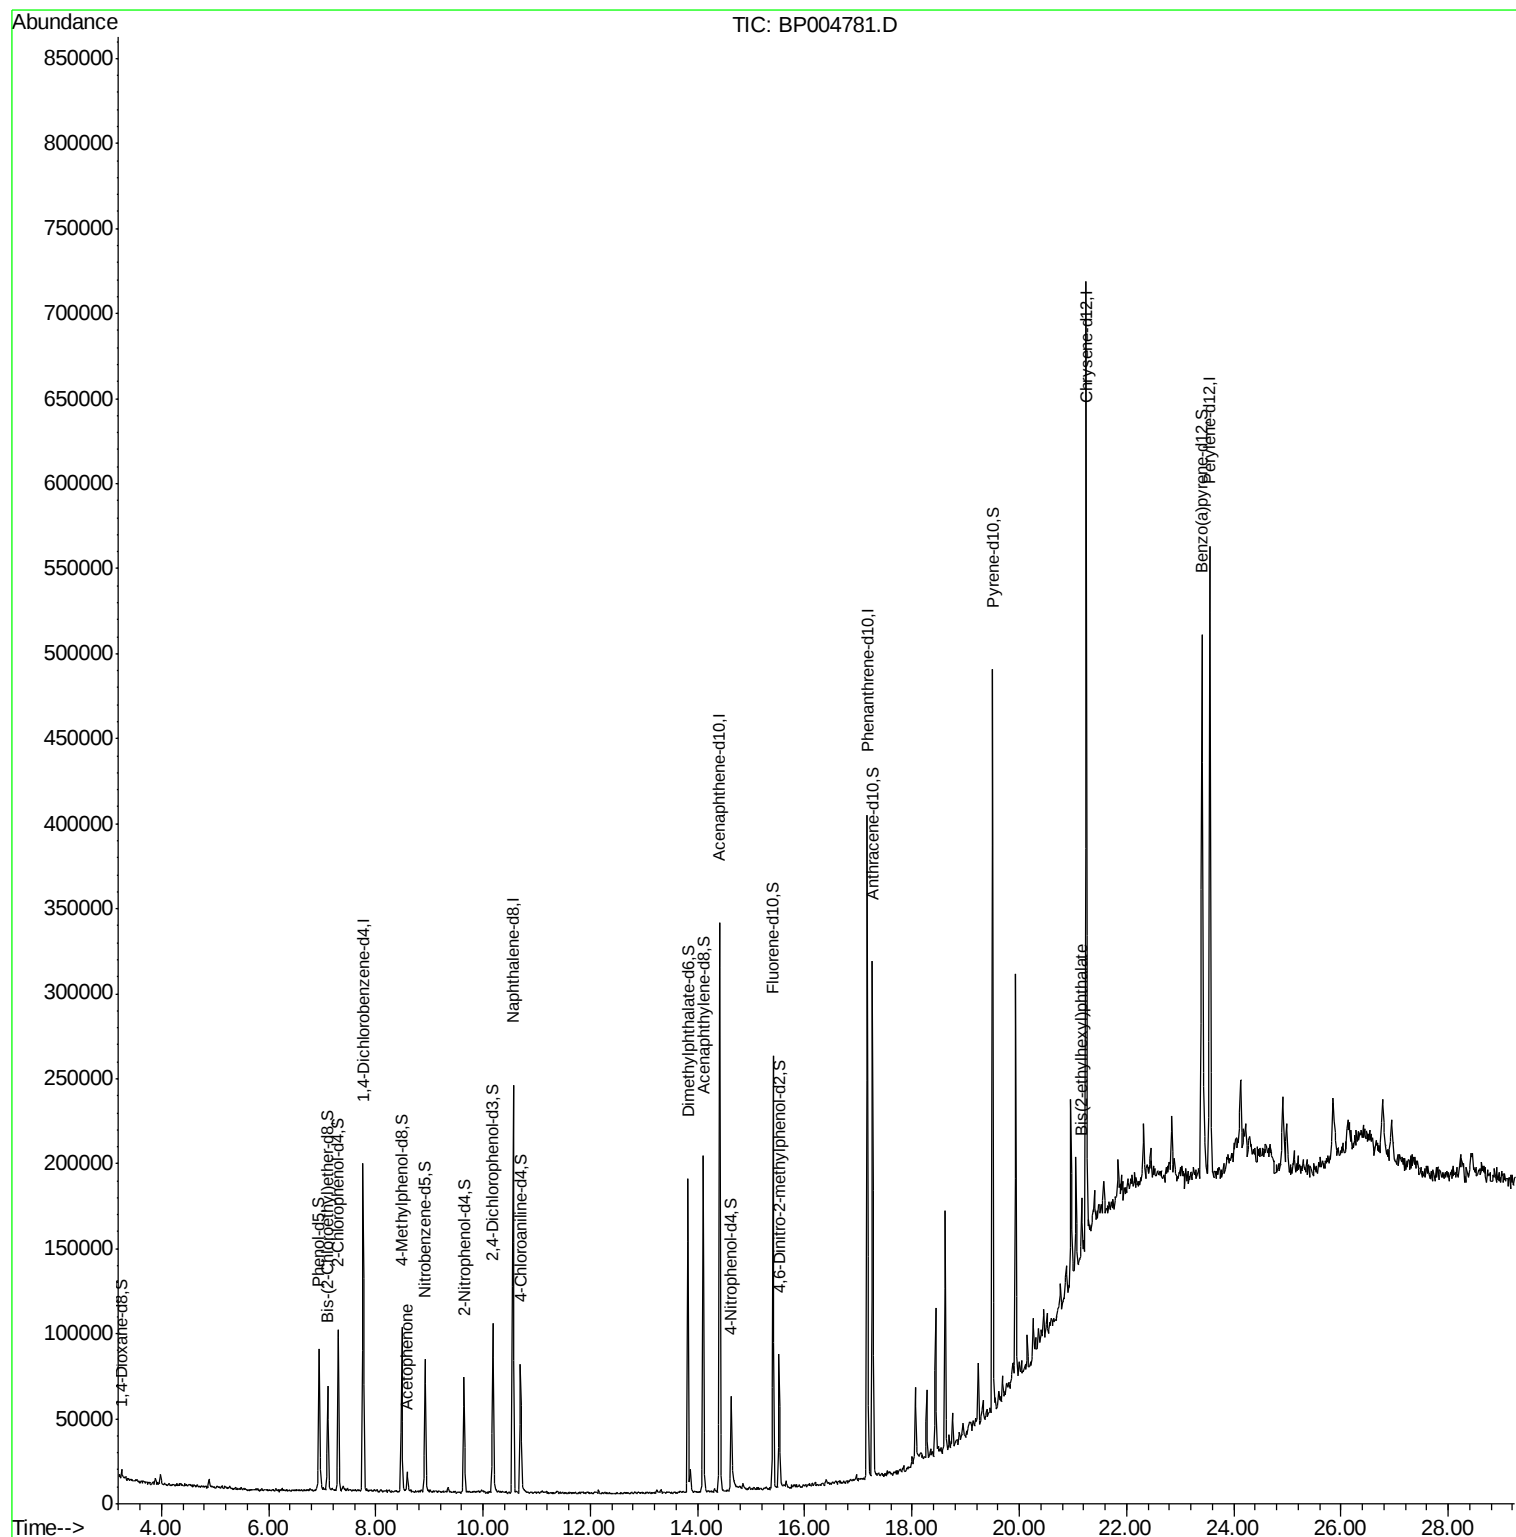


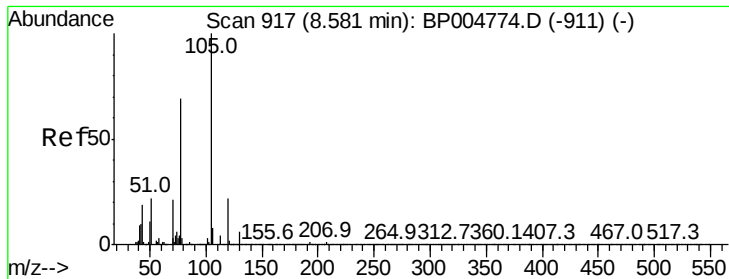

#14
Acetophenone
Concen: 1.106 ng/ul
RT: 8.59 min Scan# 918
Delta R.T. -0.00 min
Lab File: BP004781.D
Acq: 17 Feb 2021 19:42

Instrument :
BNA_P
ClientSampleId :
DBGY6

Tot Ion:	105	Resp:	5705
Ion	Ratio	Lower	Upper
105	100		
77	89.7	66.5	99.7
51	26.9	20.2	30.2

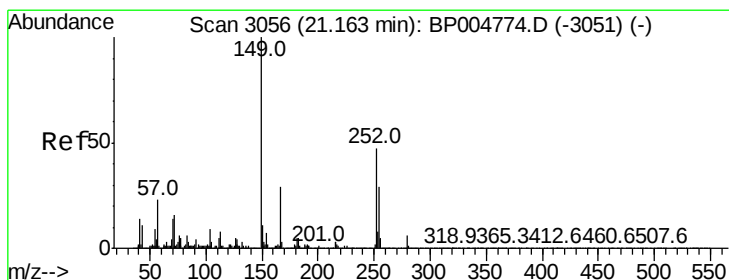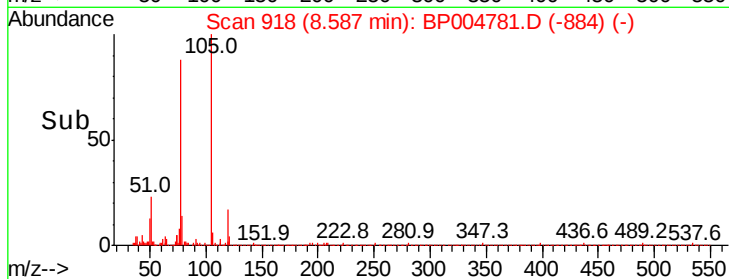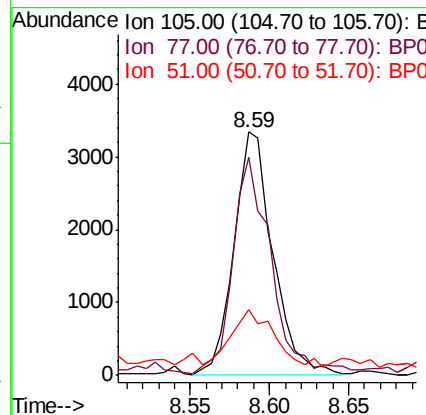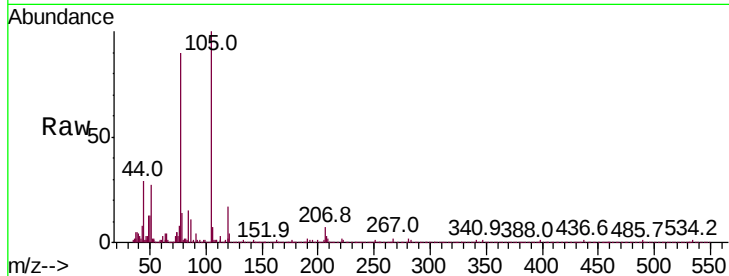

#84
Bis(2-ethylhexyl)phthalate
Concen: 1.290 ng/ul
RT: 21.16 min Scan# 3056
Delta R.T. -0.01 min
Lab File: BP004781.D
Acq: 17 Feb 2021 19:42

Tgt Ion:	149	Resp:	10507
Ion	Ratio	Lower	Upper
149	100		
167	30.9	22.6	33.8
279	6.6	4.1	6.1#

