

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP021721\
 Data File : BP004798.D
 Acq On : 18 Feb 2021 05:48
 Operator : CG/JU
 Sample : M1407-17
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBG2

Manual Integrations
 APPROVED

mohammad
 2/23/2021 3:42:03 PM

Quant Time: Feb 18 07:05:00 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 18 03:00:36 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	52180	20.00	ng/ul	0.00
18) Naphthalene-d8	10.56	136	195468	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.42	164	107241	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.17	188	201105	20.00	ng/ul	0.00
78) Chrysene-d12	21.26	240	195248	20.00	ng/ul	0.00
86) Perylene-d12	23.56	264	215464	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.25	96	7192	5.33	ng/uL	0.00
5) Phenol-d5	6.96	99	33944	8.11	ng/ul	0.02
7) Bis-(2-Chloroethyl)ether-d	7.10	67	72671	33.41	ng/ul	0.00
9) 2-Chlorophenol-d4	7.31	132	99405	31.32	ng/ul	0.01
13) 4-Methylphenol-d8	8.49	113	59556	18.08	ng/ul	0.02
19) Nitrobenzene-d5	8.93	128	54513	40.39	ng/ul	0.00
22) 2-Nitrophenol-d4	9.65	143	60419	40.79	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.19	165	100897	33.85	ng/ul	0.01
29) 4-Chloroaniline-d4	10.71	131	7679m	2.31	ng/ul	0.01
44) Dimethylphthalate-d6	13.83	166	308005	39.57	ng/ul	0.00
47) Acenaphthylene-d8	14.11	160	383520	40.50	ng/ul	0.00
52) 4-Nitrophenol-d4	14.65	143	8681	6.38	ng/ul	0.04
58) Fluorene-d10	15.42	176	252834	37.90	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.53	200	42619	35.06	ng/ul	0.00
71) Anthracene-d10	17.27	188	390782	44.06	ng/ul	0.00
79) Pyrene-d10	19.51	212	418576	45.80	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.42	264	483818	44.39	ng/ul	0.00

Target Compounds					Ovalue
45) Dimethylphthalate	13.87	163	10476m	1.305	ng/ul

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP021721\
Data File : BP004798.D
Acq On : 18 Feb 2021 05:48
Operator : CG/JU
Sample : M1407-17
Misc :
ALS Vial : 34 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
DBGM2

Quant Time: Feb 18 07:05:00 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 18 03:00:36 2021
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
2/23/2021 3:42:03 PM

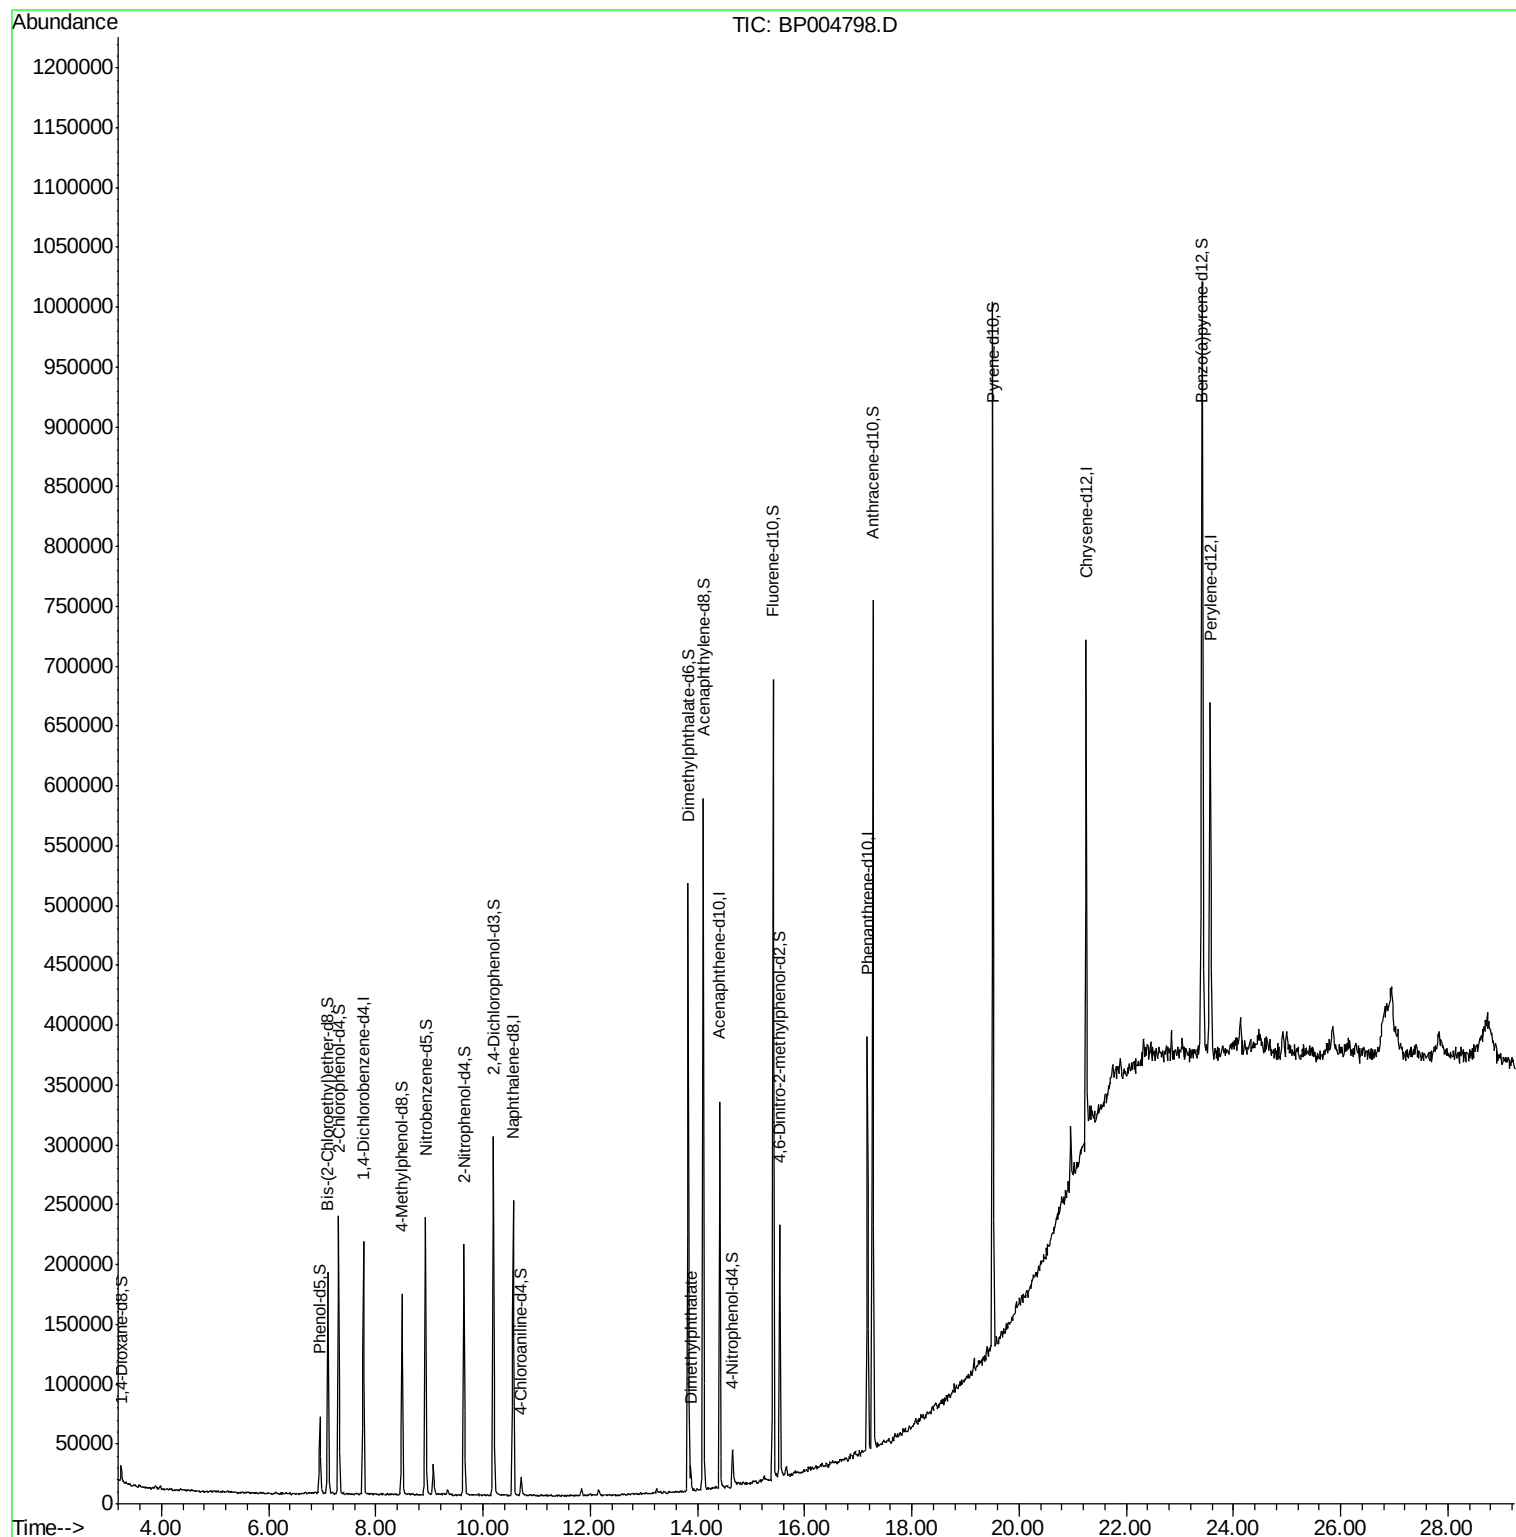

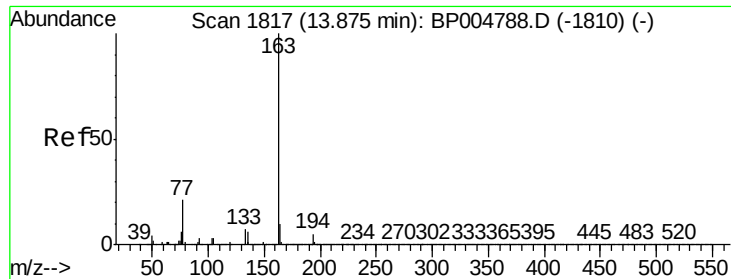

#45
 Dimethylphthalate
 Concen: 1.305 ng/ul m
 RT: 13.87 min Scan# 1817
 Delta R.T. -0.00 min
 Lab File: BP004798.D
 Acq: 18 Feb 2021 05:48

Instrument :
 BNA_P
 ClientSampleId :
 DBGM2

Tot Ion	Ratio	Resp	Lower	Upper
163	100			
194	6.7	3.8	5.6#	
164	8.3	8.0	12.0	

Manual Integrations
 APPROVED

mohammad
 2/23/2021 3:42:03 PM

