

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP021721\
 Data File : BP004775.D
 Acq On : 17 Feb 2021 16:19
 Operator : CG/JU
 Sample : PB134658BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK58

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.246	7	10	16	rVB	18106	25275	2.02%	0.203%
2	3.834	108	110	112	rVB3	1826	1379	0.11%	0.011%
3	3.858	112	114	116	rBV4	1436	1763	0.14%	0.014%
4	3.981	131	135	139	rBV6	2206	3920	0.31%	0.031%
5	4.134	157	161	164	rBV5	1182	1857	0.15%	0.015%
6	4.852	281	283	286	rBV3	1334	1494	0.12%	0.012%
7	4.970	301	303	304	rVV2	1590	1519	0.12%	0.012%
8	5.005	307	309	312	rVV3	1517	1655	0.13%	0.013%
9	5.040	312	315	317	rVB4	1378	1415	0.11%	0.011%
10	5.075	317	321	326	rVB8	1338	2429	0.19%	0.019%
11	6.587	577	578	582	rVB3	1053	1309	0.10%	0.010%
12	6.934	628	637	647	rBV	278564	438599	35.14%	3.517%
13	7.099	655	665	673	rBV	207402	322930	25.87%	2.590%
14	7.181	677	679	683	rVB5	1348	1487	0.12%	0.012%
15	7.299	691	699	708	rBV	303959	489246	39.20%	3.924%
16	7.764	771	778	785	rVV	166305	262352	21.02%	2.104%
17	8.187	849	850	853	rBV3	1195	1260	0.10%	0.010%
18	8.469	890	898	913	rBV	338671	533467	42.74%	4.278%
19	8.922	967	975	985	rBV	255048	417445	33.44%	3.348%
20	9.640	1088	1097	1105	rBV	230707	375331	30.07%	3.010%
21	10.175	1180	1188	1198	rBV	331601	553535	44.35%	4.439%
22	10.557	1244	1253	1260	rBV	196077	327402	26.23%	2.626%
23	10.693	1269	1276	1287	rBV	284500	495285	39.68%	3.972%
24	11.110	1343	1347	1350	rBV5	1021	1484	0.12%	0.012%
25	11.205	1362	1363	1368	rBV4	883	1388	0.11%	0.011%
26	12.152	1520	1524	1532	rVB2	4868	7687	0.62%	0.062%
27	13.375	1729	1732	1735	rBV4	1072	1308	0.10%	0.010%
28	13.822	1800	1808	1818	rBV	515544	677879	54.31%	5.436%
29	13.928	1822	1826	1830	rVB7	851	1314	0.11%	0.011%
30	14.098	1848	1855	1869	rBV	570258	838022	67.14%	6.721%
31	14.328	1888	1894	1895	rVB5	924	1510	0.12%	0.012%
32	14.410	1901	1908	1917	rBV	264374	382054	30.61%	3.064%
33	14.610	1935	1942	1960	rBV	150803	281470	22.55%	2.257%
34	14.834	1977	1980	1983	rVB5	1314	1399	0.11%	0.011%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP021721\
 Data File : BP004775.D
 Acq On : 17 Feb 2021 16:19
 Operator : CG/JU
 Sample : PB134658BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK58

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
 Title : SVOA CALIBRATION

35	15.404	2070	2077	2087	rBV	661318	952101	76.28%	7.636%
36	15.522	2090	2097	2109	rVV	211648	297463	23.83%	2.386%
37	15.651	2112	2119	2124	rVB3	7566	12187	0.98%	0.098%
38	15.975	2172	2174	2177	rBV4	1200	1323	0.11%	0.011%
39	16.081	2187	2192	2194	rBV5	1081	1746	0.14%	0.014%
40	16.192	2207	2211	2215	rVB4	2881	4347	0.35%	0.035%
41	16.781	2309	2311	2314	rBV3	1060	1257	0.10%	0.010%
42	16.845	2317	2322	2325	rVB6	1789	2106	0.17%	0.017%
43	16.951	2335	2340	2348	rBV9	2052	4742	0.38%	0.038%
44	17.163	2368	2376	2385	rBV	292961	407870	32.68%	3.271%
45	17.263	2385	2393	2403	rBV	696688	991977	79.47%	7.955%
46	17.363	2409	2410	2414	rVB3	1635	1809	0.14%	0.015%
47	18.069	2526	2530	2533	rBV6	1438	1917	0.15%	0.015%
48	18.663	2628	2631	2634	rBV5	1104	1263	0.10%	0.010%
49	19.145	2709	2713	2721	rBV	7293	10479	0.84%	0.084%
50	19.292	2736	2738	2740	rVB3	1742	1546	0.12%	0.012%
51	19.316	2740	2742	2743	rBV2	1787	1298	0.10%	0.010%
52	19.398	2751	2756	2758	rVB3	5084	6802	0.54%	0.055%
53	19.504	2767	2774	2782	rBV	836323	1135154	90.94%	9.104%
54	20.328	2912	2914	2915	rBV3	3021	2313	0.19%	0.019%
55	21.245	3065	3070	3080	rBV	355167	461841	37.00%	3.704%
56	23.404	3429	3437	3450	rVB	630288	1248202	100.00%	10.010%
57	23.545	3455	3461	3469	rVV2	232575	461732	36.99%	3.703%


Sum of corrected areas: 12469344

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP021721\
Data File : BP004775.D
Acq On : 17 Feb 2021 16:19
Operator : CG/JU
Sample : PB134658BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK58

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

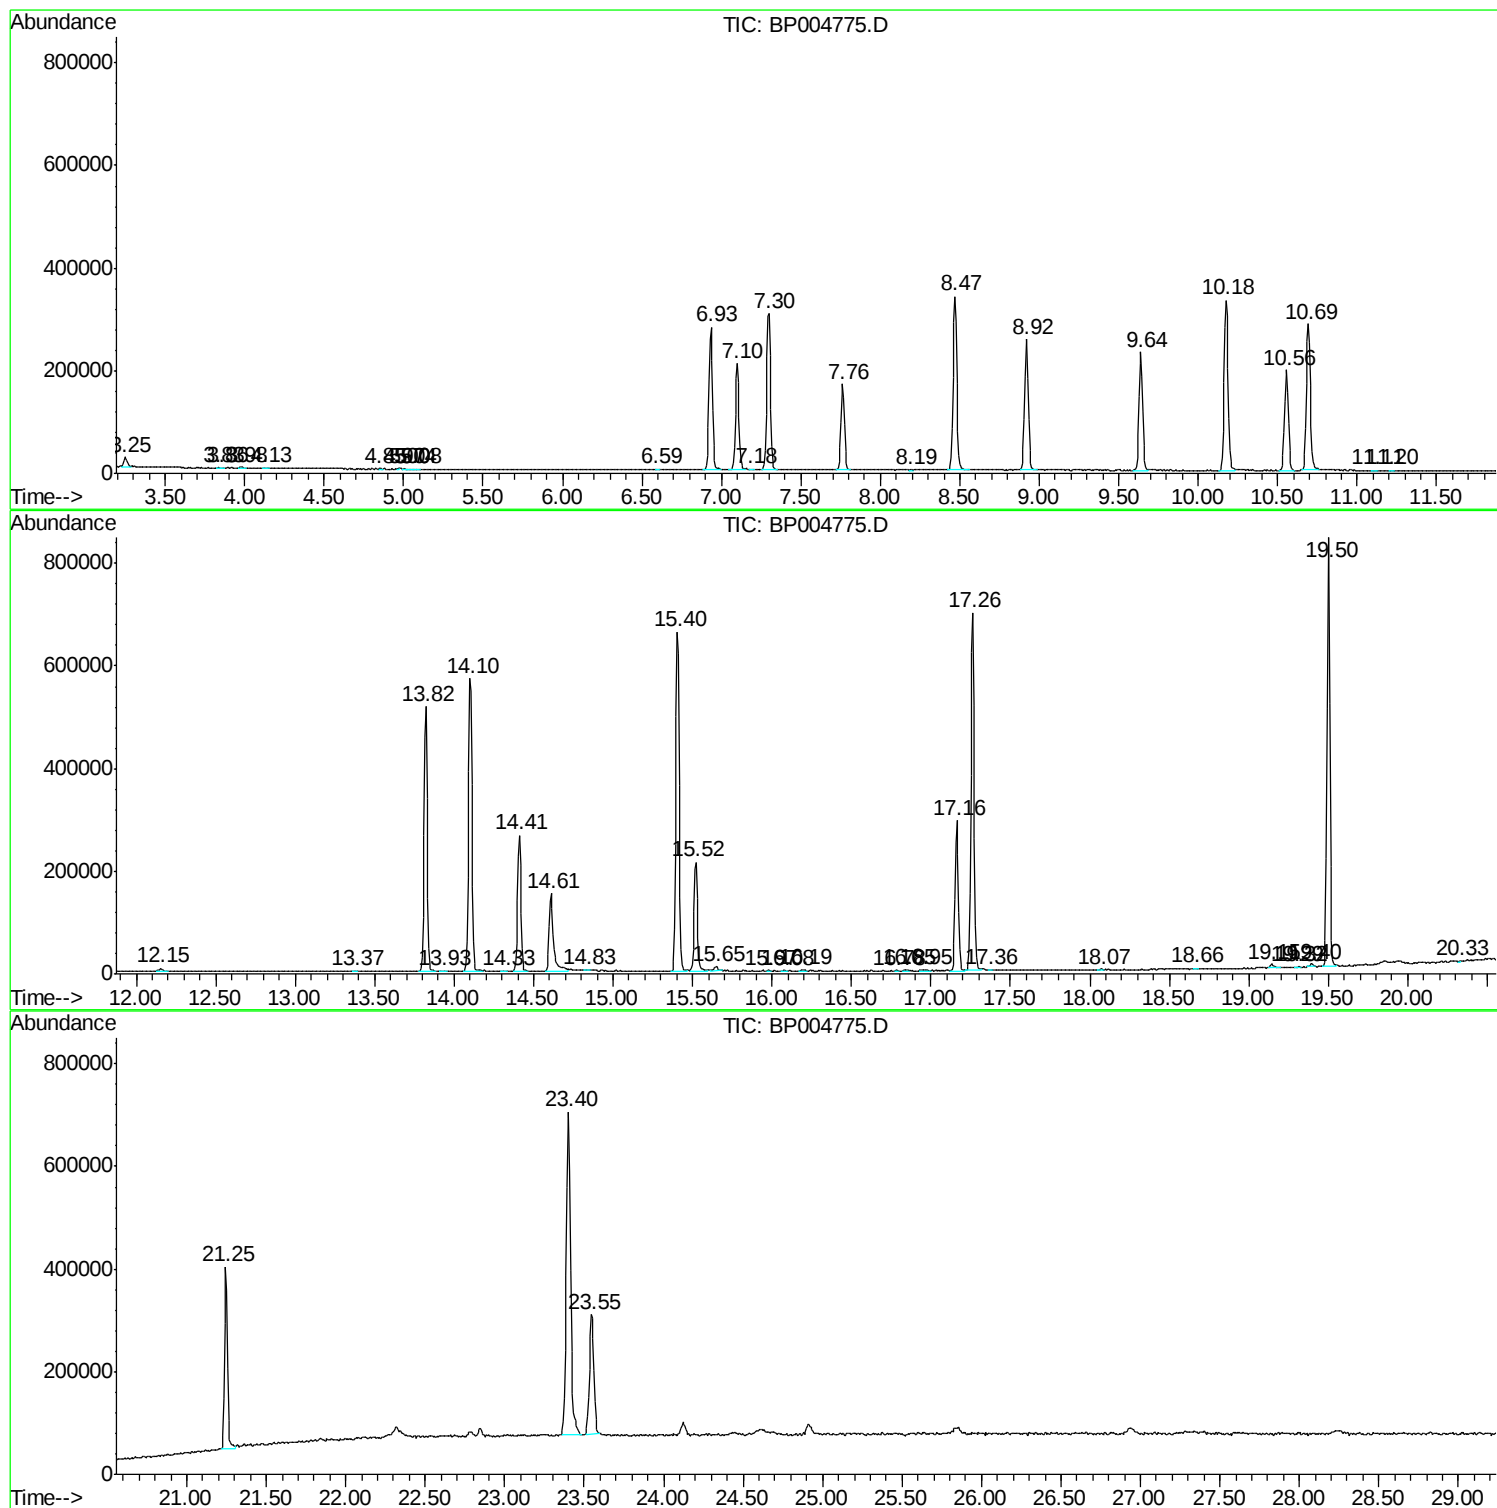

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP021721\
Data File : BP004775.D
Acq On : 17 Feb 2021 16:19
Operator : CG/JU
Sample : PB134658BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK58

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP021721\
Data File : BP004775.D
Acq On : 17 Feb 2021 16:19
Operator : CG/JU
Sample : PB134658BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK58

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc