

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP021721\
 Data File : BP004798.D
 Acq On : 18 Feb 2021 05:48
 Operator : CG/JU
 Sample : M1407-17
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBG2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	8	11	17	rVB	13600	18752	1.49%	0.161%
2	3.887	116	119	123	rVB5	2783	3717	0.30%	0.032%
3	3.981	132	135	139	rVB4	3781	5519	0.44%	0.048%
4	4.217	174	175	178	rBV2	1389	1749	0.14%	0.015%
5	4.358	195	199	201	rBV5	1942	3131	0.25%	0.027%
6	4.687	252	255	259	rVB6	1268	2235	0.18%	0.019%
7	5.846	448	452	453	rBV4	1395	1397	0.11%	0.012%
8	6.075	490	491	496	rBV5	1299	1782	0.14%	0.015%
9	6.258	519	522	524	rBV4	1483	1633	0.13%	0.014%
10	6.405	544	547	549	rVB4	1915	1700	0.14%	0.015%
11	6.916	630	634	635	rBV3	1487	1766	0.14%	0.015%
12	6.958	635	641	649	rVB	63875	103538	8.24%	0.891%
13	7.105	659	666	676	rBV	184931	285515	22.72%	2.458%
14	7.310	691	701	712	rBV	232870	375769	29.90%	3.235%
15	7.387	712	714	717	rVV4	1593	1812	0.14%	0.016%
16	7.452	721	725	728	rBV6	966	1532	0.12%	0.013%
17	7.522	733	737	740	rVB5	1091	1632	0.13%	0.014%
18	7.769	772	779	789	rBV	211179	326119	25.95%	2.808%
19	7.916	802	804	809	rVB5	1280	1788	0.14%	0.015%
20	8.216	850	855	858	rVV7	759	1278	0.10%	0.011%
21	8.252	858	861	865	rVB6	1222	1427	0.11%	0.012%
22	8.305	867	870	874	rVB5	1303	1574	0.13%	0.014%
23	8.493	895	902	912	rVB	167175	266827	21.23%	2.297%
24	8.687	931	935	938	rVB5	1098	1619	0.13%	0.014%
25	8.928	967	976	989	rBV	232479	388086	30.88%	3.341%
26	9.075	992	1001	1006	rBV2	25474	44354	3.53%	0.382%
27	9.340	1042	1046	1052	rVB6	4590	8195	0.65%	0.071%
28	9.646	1088	1098	1107	rBV	210042	350618	27.90%	3.019%
29	9.846	1127	1132	1134	rBV5	959	1304	0.10%	0.011%
30	10.193	1184	1191	1208	rBV	299678	493888	39.30%	4.252%
31	10.563	1245	1254	1262	rBV	246661	415773	33.08%	3.580%
32	10.710	1272	1279	1289	rBV2	15789	31703	2.52%	0.273%
33	11.063	1335	1339	1343	rBV7	959	1909	0.15%	0.016%
34	11.263	1370	1373	1377	rBV6	769	1347	0.11%	0.012%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP021721\
 Data File : BP004798.D
 Acq On : 18 Feb 2021 05:48
 Operator : CG/JU
 Sample : M1407-17
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBG2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
 Title : SVOA CALIBRATION

35	11.840	1463	1471	1477	rBV2	5992	12010	0.96%	0.103%
36	12.040	1502	1505	1510	rBV6	813	1554	0.12%	0.013%
37	12.157	1519	1525	1530	rBV3	4813	8687	0.69%	0.075%
38	12.328	1551	1554	1557	rBV5	930	1504	0.12%	0.013%
39	12.369	1559	1561	1566	rVB6	1087	1528	0.12%	0.013%
40	12.634	1603	1606	1610	rBV6	853	1289	0.10%	0.011%
41	12.728	1618	1622	1625	rVB5	989	1440	0.11%	0.012%
42	12.763	1625	1628	1631	rBV4	851	1350	0.11%	0.012%
43	12.810	1633	1636	1638	rVB4	1032	1273	0.10%	0.011%
44	13.034	1670	1674	1677	rBV6	1002	1707	0.14%	0.015%
45	13.240	1705	1709	1713	rBV6	4075	5588	0.44%	0.048%
46	13.316	1720	1722	1726	rVB5	1680	1772	0.14%	0.015%
47	13.375	1729	1732	1736	rVB6	1429	2007	0.16%	0.017%
48	13.469	1744	1748	1749	rBV4	1323	1462	0.12%	0.013%
49	13.581	1765	1767	1771	rBV5	833	1272	0.10%	0.011%
50	13.828	1803	1809	1814	rBV	507801	688458	54.78%	5.928%
51	13.875	1814	1817	1822	rVV	20958	28324	2.25%	0.244%
52	13.934	1825	1827	1831	rVB5	1666	2150	0.17%	0.019%
53	14.110	1847	1857	1870	rBV	578585	836517	66.56%	7.203%
54	14.210	1872	1874	1877	rBV4	1277	1468	0.12%	0.013%
55	14.263	1880	1883	1884	rBV3	1164	1365	0.11%	0.012%
56	14.416	1903	1909	1916	rBV2	322928	484653	38.56%	4.173%
57	14.469	1916	1918	1920	rVB3	1920	1307	0.10%	0.011%
58	14.616	1941	1943	1944	rBV2	1643	1484	0.12%	0.013%
59	14.651	1944	1949	1956	rBV2	30610	59911	4.77%	0.516%
60	14.892	1989	1990	1993	rVB3	2296	1563	0.12%	0.013%
61	14.922	1993	1995	1996	rBV2	2153	1564	0.12%	0.013%
62	14.998	2006	2008	2009	rBV2	2062	1422	0.11%	0.012%
63	15.416	2072	2079	2086	rBV	669503	965581	76.83%	8.314%
64	15.534	2094	2099	2107	rBV	209419	295259	23.49%	2.542%
65	15.651	2116	2119	2126	rVB5	7702	14494	1.15%	0.125%
66	16.069	2188	2190	2191	rBV2	4029	2737	0.22%	0.024%
67	17.169	2372	2377	2388	rBV	344269	498789	39.69%	4.295%
68	17.269	2388	2394	2403	rBV	709269	1038501	82.63%	8.942%
69	19.510	2770	2775	2782	rVB	873447	1112271	88.50%	9.577%
70	21.257	3067	3072	3077	rBV	423939	574966	45.75%	4.951%
71	23.416	3433	3439	3448	rVB	639372	1256760	100.00%	10.821%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP021721\
Data File : BP004798.D
Acq On : 18 Feb 2021 05:48
Operator : CG/JU
Sample : M1407-17
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBGM2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
Title : SVOA CALIBRATION

72	23.563	3460	3464	3472	rVB2	289881	549266	43.70%	4.729%
----	--------	------	------	------	------	--------	--------	--------	--------


Sum of corrected areas: 11614241

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP021721\
Data File : BP004798.D
Acq On : 18 Feb 2021 05:48
Operator : CG/JU
Sample : M1407-17
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBGM2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

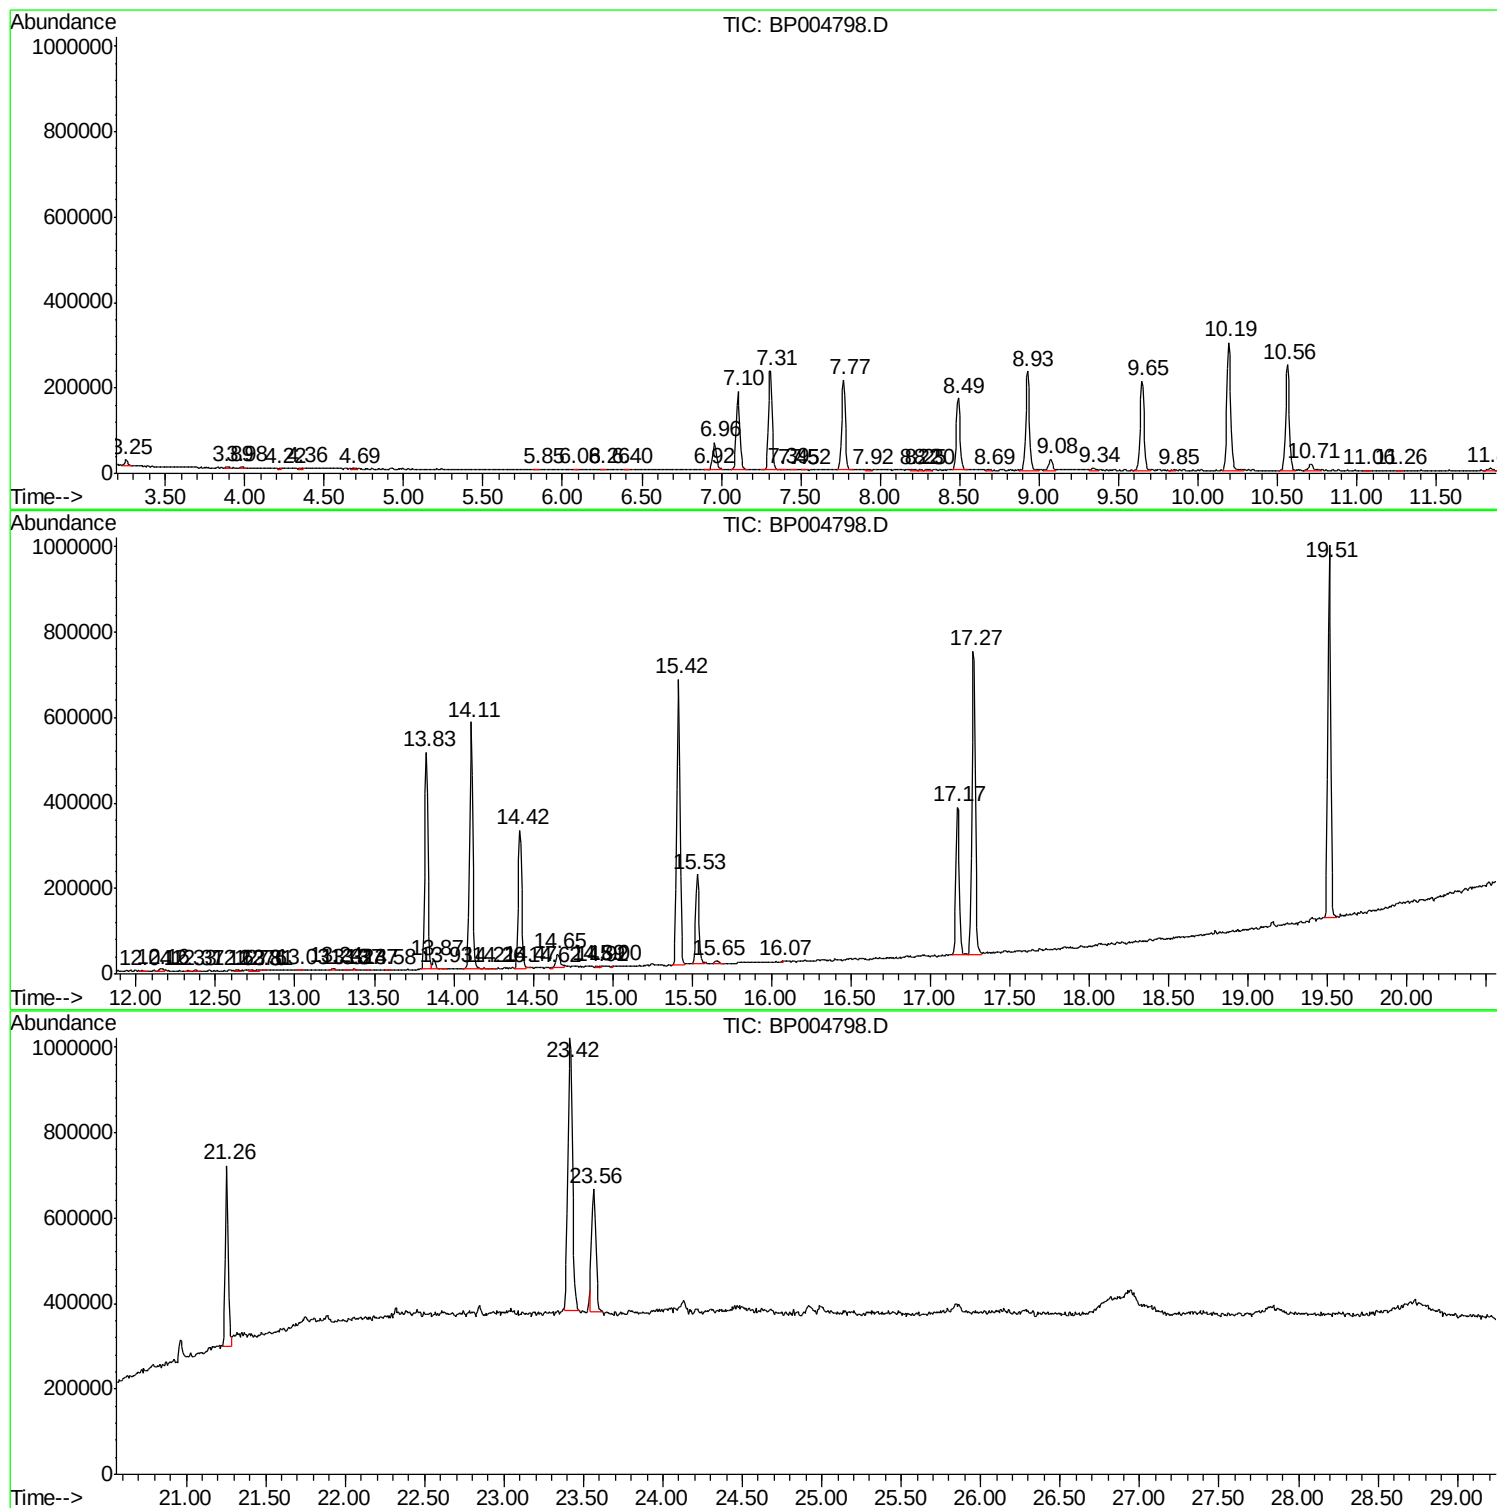

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP021721\
Data File : BP004798.D
Acq On : 18 Feb 2021 05:48
Operator : CG/JU
Sample : M1407-17
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBGM2










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Hexanoic acid, 2-ethyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
9.08	2.72 ng/ul	44354	1,4-Dichlorobenzene-d4	7.77

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Hexanoic acid, 2-ethyl-	144	C8H16O2	000149-57-5	80
2		Hexanoic acid, 2-ethyl-	144	C8H16O2	000149-57-5	59
3		L(-)-Fucose, tetramethyl ether	220	C10H20O5	1000332-75-0	47
4		Pentanoic acid, 2-methyl-, methyl...	130	C7H14O2	002177-77-7	38
5		Octanoic acid, 2-methyl-, methyl...	172	C10H20O2	002177-86-8	38

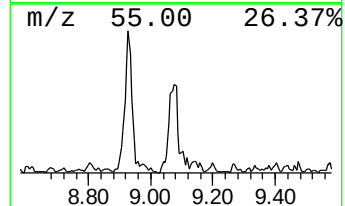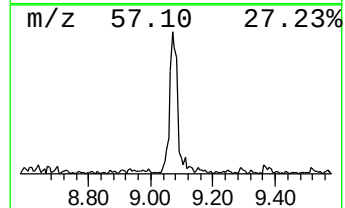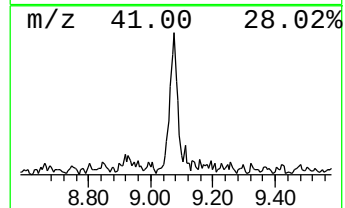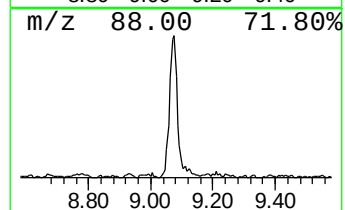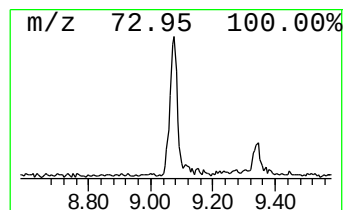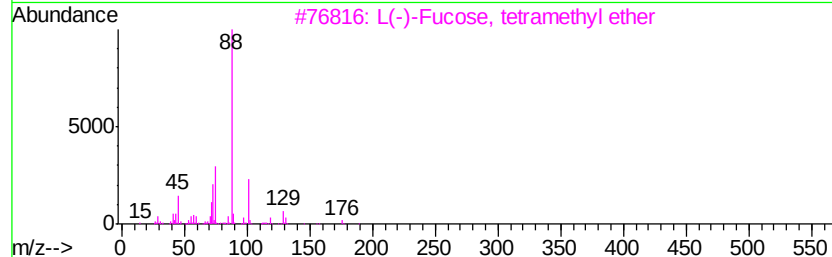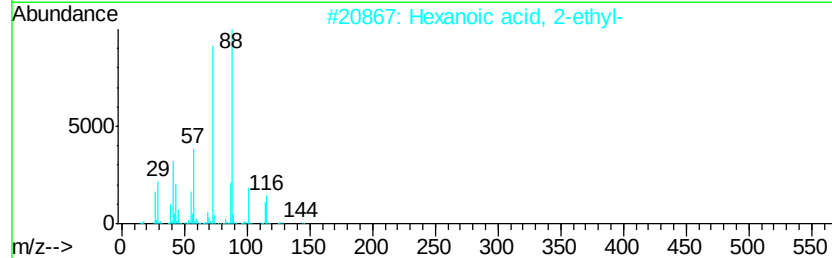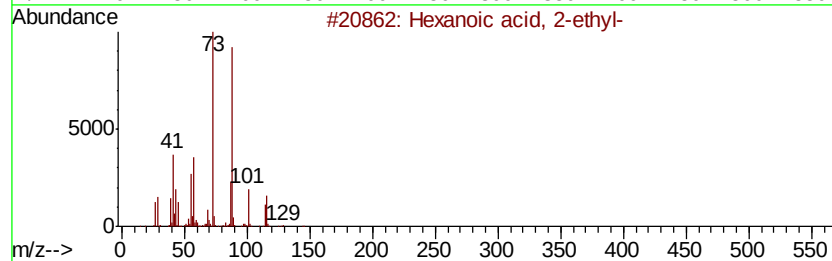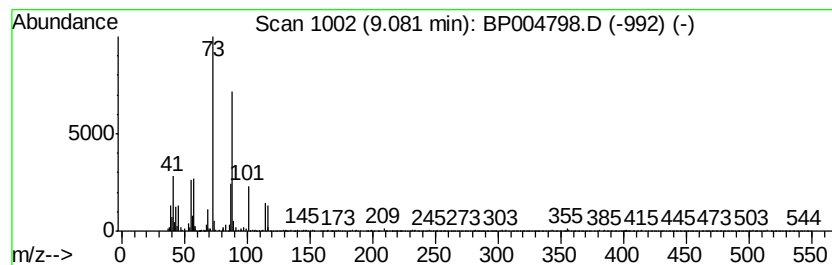

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP021721\
Data File : BP004798.D
Acq On : 18 Feb 2021 05:48
Operator : CG/JU
Sample : M1407-17
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBGM2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Hexanoic acid, 2-...	9.08	2.7	ng/ul	44354	1	7.77	326119	20.0