

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP021721\
 Data File : BP004800.D
 Acq On : 18 Feb 2021 06:55
 Operator : CG/JU
 Sample : M1407-19
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBG7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	8	11	21	rVB	11275	17247	1.11%	0.143%
2	3.558	61	63	67	rBV4	1557	1928	0.12%	0.016%
3	3.987	132	136	140	rVB4	4955	5653	0.36%	0.047%
4	5.369	369	371	377	rVB6	1632	2222	0.14%	0.018%
5	6.234	515	518	520	rBV3	1232	1628	0.11%	0.013%
6	6.499	558	563	564	rVB5	1222	1634	0.11%	0.014%
7	6.869	623	626	630	rVV6	1314	2167	0.14%	0.018%
8	6.910	630	633	634	rVV2	1859	1710	0.11%	0.014%
9	6.952	634	640	650	rVB2	54131	103724	6.70%	0.858%
10	7.105	660	666	678	rVB	165418	261609	16.89%	2.164%
11	7.305	692	700	710	rVB	215067	339324	21.91%	2.807%
12	7.399	714	716	719	rBV4	1314	1571	0.10%	0.013%
13	7.769	773	779	788	rVV	213218	333269	21.52%	2.757%
14	7.834	788	790	797	rVB8	1975	3638	0.23%	0.030%
15	8.487	894	901	909	rBV	147984	233461	15.07%	1.932%
16	8.928	968	976	985	rVV	216697	354372	22.88%	2.932%
17	9.110	1005	1007	1014	rVB7	970	1615	0.10%	0.013%
18	9.340	1039	1046	1051	rVB3	4828	8225	0.53%	0.068%
19	9.646	1090	1098	1106	rBV	189072	315864	20.39%	2.613%
20	10.193	1179	1191	1203	rBV	261168	448098	28.93%	3.707%
21	10.563	1247	1254	1263	rBV	249185	410718	26.52%	3.398%
22	10.710	1272	1279	1287	rBV2	12469	25193	1.63%	0.208%
23	11.081	1336	1342	1347	rVB9	1180	2360	0.15%	0.020%
24	11.404	1387	1397	1400	rBV8	3303	8664	0.56%	0.072%
25	11.722	1445	1451	1453	rBV7	1619	2165	0.14%	0.018%
26	11.840	1466	1471	1476	rVB4	3949	6349	0.41%	0.053%
27	12.157	1519	1525	1532	rBV4	4251	8301	0.54%	0.069%
28	12.816	1636	1637	1645	rVB8	1344	1564	0.10%	0.013%
29	13.028	1666	1673	1674	rBV7	1080	1784	0.12%	0.015%
30	13.239	1705	1709	1711	rBV5	2820	4499	0.29%	0.037%
31	13.263	1711	1713	1717	rVV3	3331	4105	0.27%	0.034%
32	13.316	1720	1722	1728	rVV7	1667	2348	0.15%	0.019%
33	13.387	1732	1734	1739	rVB6	1290	1830	0.12%	0.015%
34	13.739	1788	1794	1796	rBV6	1602	2436	0.16%	0.020%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP021721\
 Data File : BP004800.D
 Acq On : 18 Feb 2021 06:55
 Operator : CG/JU
 Sample : M1407-19
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBG7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
 Title : SVOA CALIBRATION

35	13.828	1800	1809	1814	rBV	466694	648580	41.88%	5.366%
36	13.875	1814	1817	1823	rVV	34864	45713	2.95%	0.378%
37	14.057	1846	1848	1850	rBV3	1736	1758	0.11%	0.015%
38	14.110	1850	1857	1866	rVV	537625	773303	49.93%	6.398%
39	14.228	1875	1877	1881	rBV5	1167	1714	0.11%	0.014%
40	14.322	1889	1893	1894	rBV4	1418	1768	0.11%	0.015%
41	14.416	1902	1909	1917	rBV	331290	492506	31.80%	4.075%
42	14.651	1943	1949	1961	rBV	29621	64613	4.17%	0.535%
43	14.845	1976	1982	1986	rBV9	3699	7624	0.49%	0.063%
44	15.169	2034	2037	2043	rBV7	2619	3850	0.25%	0.032%
45	15.216	2043	2045	2046	rBV2	2440	2444	0.16%	0.020%
46	15.239	2047	2049	2053	rVB4	5000	5763	0.37%	0.048%
47	15.351	2066	2068	2071	rBV4	2108	2869	0.19%	0.024%
48	15.410	2072	2078	2085	rVV	665228	945702	61.06%	7.824%
49	15.533	2093	2099	2108	rBV	218645	318721	20.58%	2.637%
50	15.651	2116	2119	2124	rVB2	8136	11452	0.74%	0.095%
51	15.781	2137	2141	2142	rBV4	1951	2071	0.13%	0.017%
52	16.198	2210	2212	2216	rVB5	4024	4775	0.31%	0.040%
53	17.169	2371	2377	2383	rBV	374961	537542	34.71%	4.447%
54	17.269	2388	2394	2406	rVB2	785212	1099368	70.98%	9.096%
55	19.510	2770	2775	2782	rVB	1007416	1262751	81.53%	10.448%
56	20.963	3020	3022	3028	rBV5	44488	48332	3.12%	0.400%
57	21.257	3067	3072	3078	rBV	489420	651666	42.08%	5.392%
58	23.415	3432	3439	3449	rBV	807275	1548794	100.00%	12.814%
59	23.562	3458	3464	3472	rVB2	358723	681502	44.00%	5.639%


Sum of corrected areas: 12086456

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP021721\
Data File : BP004800.D
Acq On : 18 Feb 2021 06:55
Operator : CG/JU
Sample : M1407-19
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBGM7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

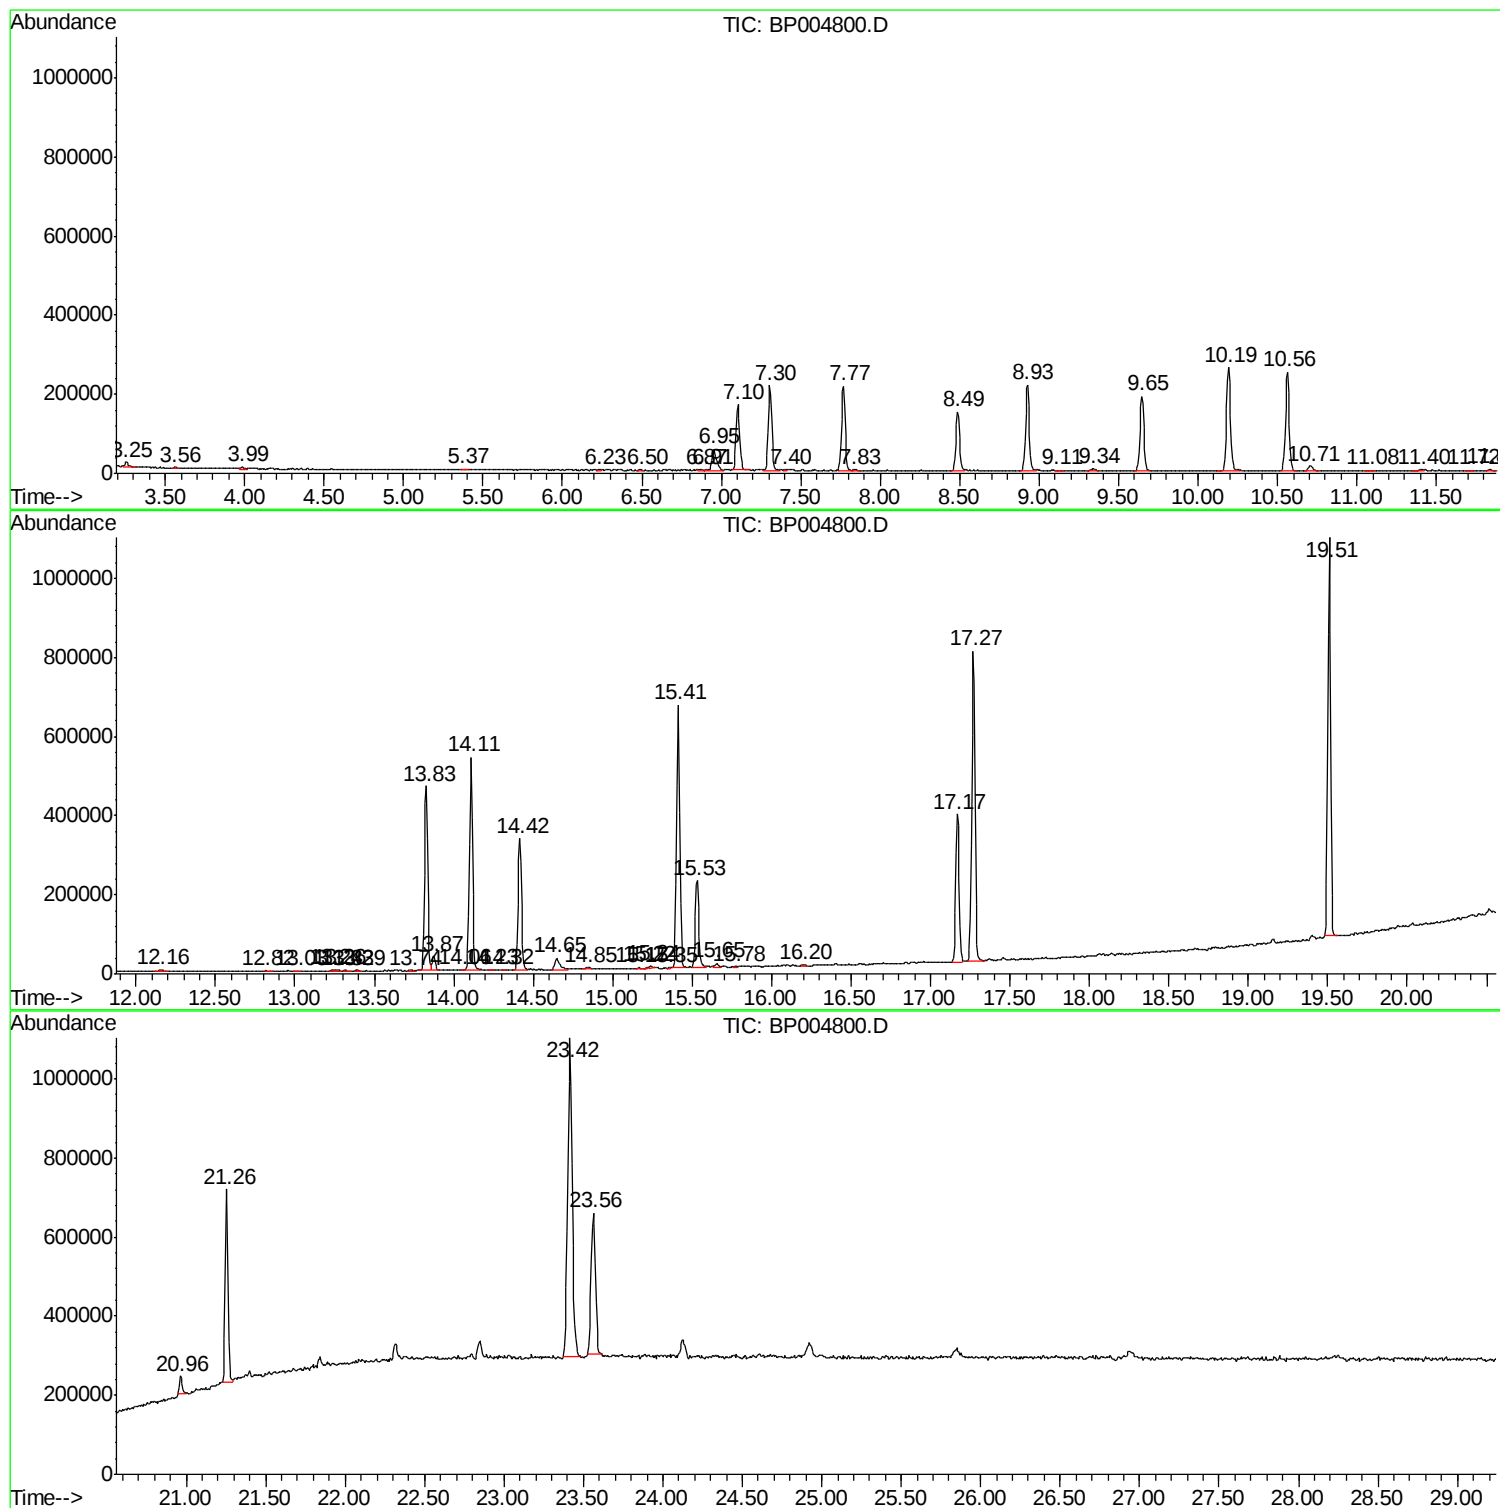

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP021721\
Data File : BP004800.D
Acq On : 18 Feb 2021 06:55
Operator : CG/JU
Sample : M1407-19
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBGM7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP021721\
Data File : BP004800.D
Acq On : 18 Feb 2021 06:55
Operator : CG/JU
Sample : M1407-19
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBGM7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc