

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP021721\
 Data File : BP004801.D
 Acq On : 18 Feb 2021 07:29
 Operator : CG/JU
 Sample : M1407-20
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBGN2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	7	11	17	rVB	10814	15902	1.01%	0.128%
2	3.628	73	75	79	rVB5	2664	2397	0.15%	0.019%
3	3.981	133	135	139	rVB3	3683	4297	0.27%	0.035%
4	4.540	226	230	236	rVB8	1337	2091	0.13%	0.017%
5	5.899	457	461	463	rBV4	1279	1608	0.10%	0.013%
6	6.893	624	630	632	rBV7	1489	2227	0.14%	0.018%
7	6.952	634	640	650	rVB	50303	85179	5.42%	0.685%
8	7.105	658	666	676	rBV	143916	232358	14.79%	1.867%
9	7.305	691	700	708	rBV	193875	307365	19.57%	2.470%
10	7.769	770	779	786	rBV	183900	293230	18.67%	2.356%
11	8.111	835	837	841	rVB4	1675	1846	0.12%	0.015%
12	8.487	894	901	912	rBV	142612	228563	14.55%	1.837%
13	8.616	917	923	928	rVB6	4113	7927	0.50%	0.064%
14	8.822	954	958	963	rBV8	1079	1809	0.12%	0.015%
15	8.922	965	975	986	rBV	195497	322478	20.53%	2.592%
16	8.999	986	988	993	rVB6	1433	1837	0.12%	0.015%
17	9.340	1039	1046	1051	rVV2	8848	14210	0.90%	0.114%
18	9.646	1091	1098	1107	rBV	175931	292298	18.61%	2.349%
19	10.193	1182	1191	1201	rBV	260766	449230	28.60%	3.610%
20	10.434	1229	1232	1235	rBV5	1477	1634	0.10%	0.013%
21	10.563	1245	1254	1261	rBV	228207	385462	24.54%	3.098%
22	10.710	1273	1279	1289	rVV2	12154	25787	1.64%	0.207%
23	10.775	1289	1290	1296	rVB7	1159	1681	0.11%	0.014%
24	10.922	1310	1315	1320	rBV9	1501	2291	0.15%	0.018%
25	11.840	1466	1471	1477	rVB2	11562	17187	1.09%	0.138%
26	12.128	1515	1520	1521	rBV5	1699	2291	0.15%	0.018%
27	12.152	1521	1524	1531	rVB4	4453	7703	0.49%	0.062%
28	12.716	1616	1620	1623	rBV5	922	1777	0.11%	0.014%
29	13.022	1667	1672	1673	rBV5	1749	2046	0.13%	0.016%
30	13.128	1684	1690	1692	rBV7	1269	1972	0.13%	0.016%
31	13.169	1692	1697	1700	rVV7	972	1677	0.11%	0.013%
32	13.246	1704	1710	1711	rVV6	2979	4903	0.31%	0.039%
33	13.263	1711	1713	1717	rVB5	2272	2902	0.18%	0.023%
34	13.828	1802	1809	1814	rVV	522241	721590	45.94%	5.799%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP021721\
 Data File : BP004801.D
 Acq On : 18 Feb 2021 07:29
 Operator : CG/JU
 Sample : M1407-20
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBGN2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
 Title : SVOA CALIBRATION

35	13.869	1814	1816	1822	rVB	29449	37643	2.40%	0.303%
36	14.104	1846	1856	1868	rVV	540915	819282	52.16%	6.584%
37	14.316	1890	1892	1896	rVB5	2439	2540	0.16%	0.020%
38	14.416	1902	1909	1918	rVB	336563	502269	31.98%	4.036%
39	14.481	1918	1920	1924	rBV5	1142	1914	0.12%	0.015%
40	14.646	1943	1948	1958	rBV	38365	71746	4.57%	0.577%
41	14.757	1963	1967	1971	rVB6	2925	4315	0.27%	0.035%
42	14.840	1978	1981	1985	rBV6	3966	5604	0.36%	0.045%
43	14.963	1999	2002	2006	rVB6	3972	4451	0.28%	0.036%
44	15.051	2014	2017	2020	rBV4	3196	3352	0.21%	0.027%
45	15.163	2034	2036	2040	rBV6	2530	2186	0.14%	0.018%
46	15.410	2072	2078	2085	rBV	699913	990174	63.04%	7.957%
47	15.534	2093	2099	2104	rBV	238907	340388	21.67%	2.735%
48	15.616	2111	2113	2115	rBV3	3137	3558	0.23%	0.029%
49	15.651	2115	2119	2125	rVB8	9008	15573	0.99%	0.125%
50	16.098	2191	2195	2198	rBV6	3312	5426	0.35%	0.044%
51	16.192	2209	2211	2215	rVB5	5635	7457	0.47%	0.060%
52	17.169	2371	2377	2385	rBV	412289	578792	36.85%	4.651%
53	17.269	2388	2394	2402	rVV	829672	1158619	73.76%	9.311%
54	18.063	2526	2529	2535	rBV7	22196	28137	1.79%	0.226%
55	19.510	2769	2775	2782	rBV	1098486	1415578	90.12%	11.376%
56	20.963	3020	3022	3027	rVB3	53635	61640	3.92%	0.495%
57	21.251	3067	3071	3077	rBV	531568	691249	44.01%	5.555%
58	23.416	3433	3439	3450	rVB	775931	1570713	100.00%	12.623%
59	23.563	3459	3464	3471	rVB2	369779	673186	42.86%	5.410%


Sum of corrected areas: 12443547

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP021721\
Data File : BP004801.D
Acq On : 18 Feb 2021 07:29
Operator : CG/JU
Sample : M1407-20
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampled :
DBGN2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

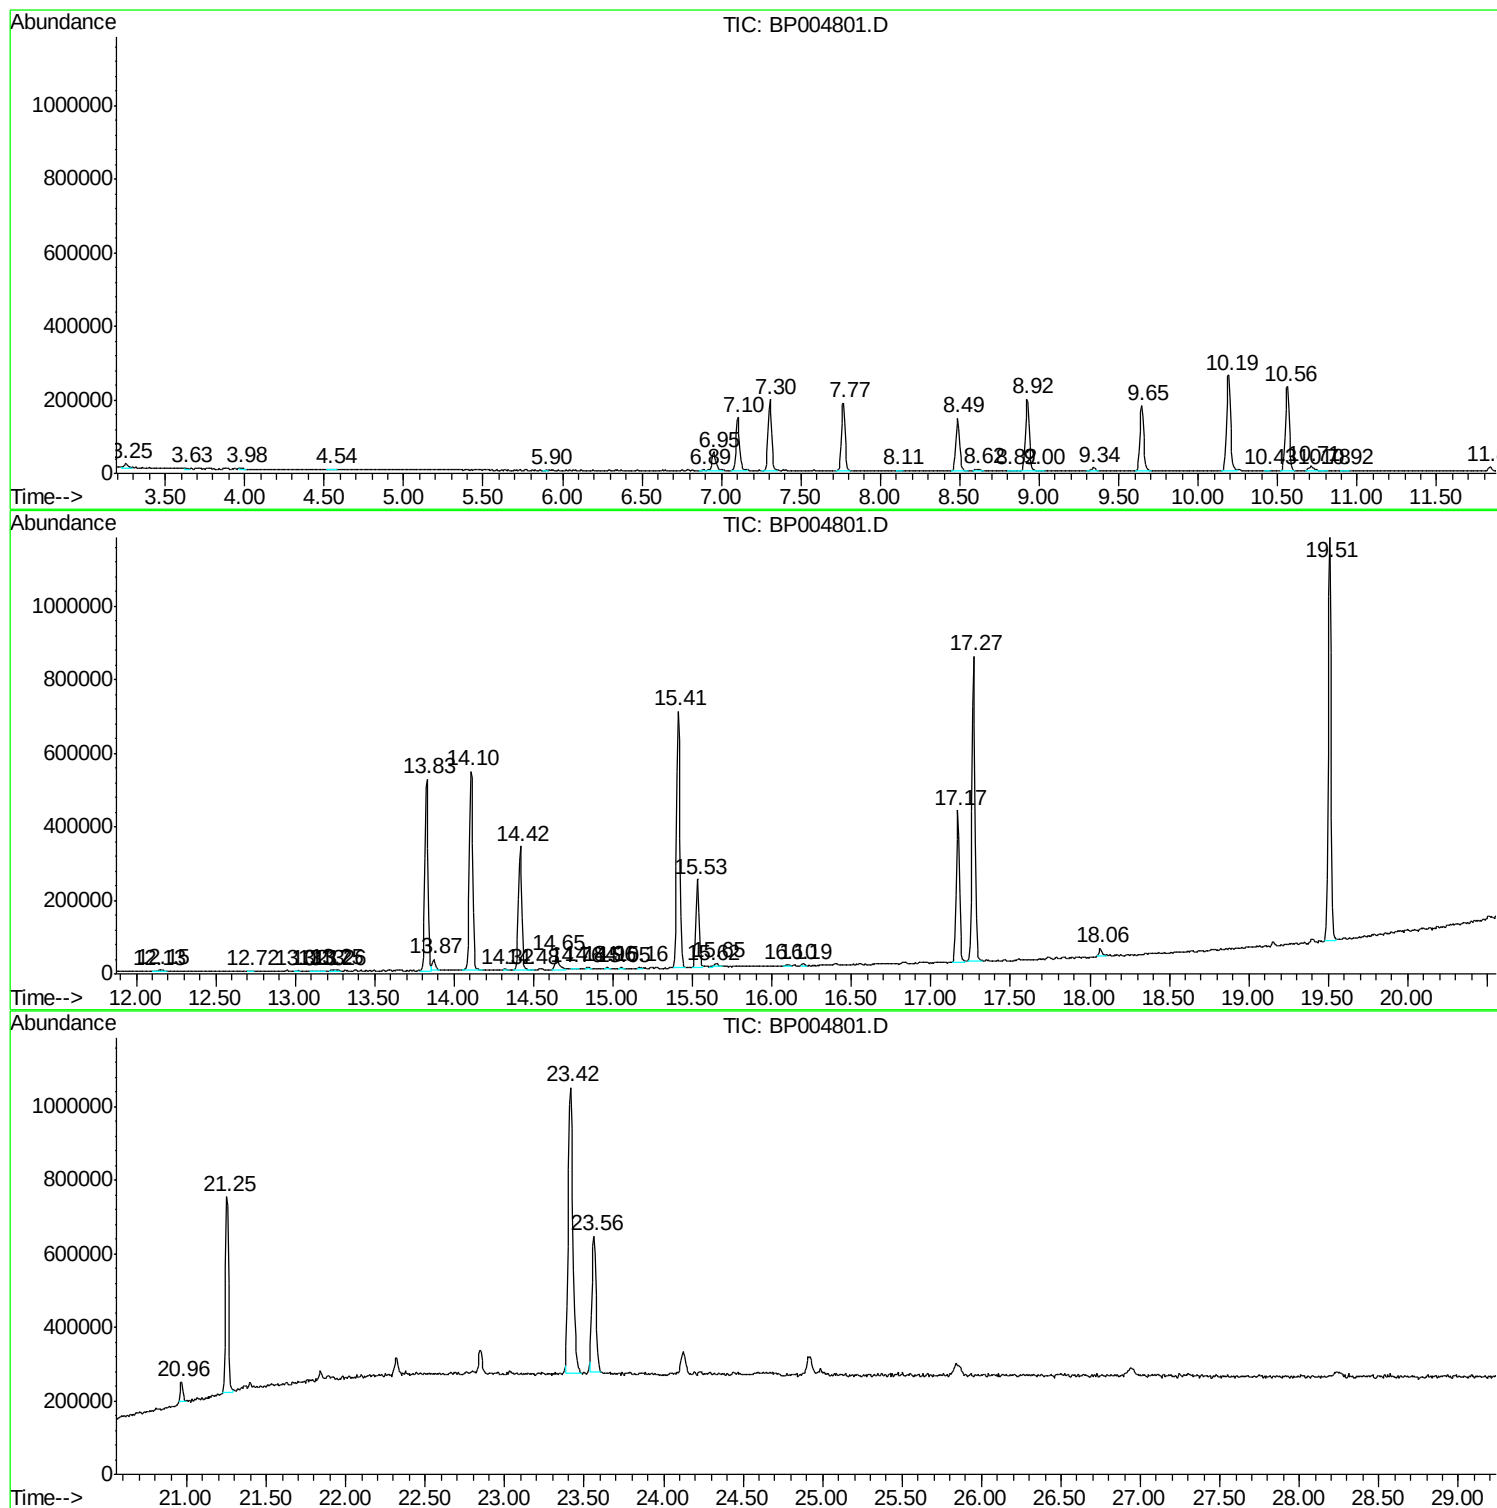

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP021721\
Data File : BP004801.D
Acq On : 18 Feb 2021 07:29
Operator : CG/JU
Sample : M1407-20
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBGN2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP021721\
Data File : BP004801.D
Acq On : 18 Feb 2021 07:29
Operator : CG/JU
Sample : M1407-20
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBGN2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc