

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP021721\
 Data File : BP004804.D
 Acq On : 18 Feb 2021 11:14
 Operator : CG/JU
 Sample : M1407-07DL2 50X
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBGK7DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.528	56	58	60	rVB3	1933	1517	0.20%	0.034%
2	3.552	60	62	64	rBV3	1083	1298	0.17%	0.029%
3	3.858	113	114	117	rBV3	1027	1021	0.13%	0.023%
4	3.981	132	135	141	rVB4	3642	5848	0.76%	0.132%
5	4.775	269	270	275	rBV4	935	1059	0.14%	0.024%
6	4.952	299	300	303	rBV2	999	1087	0.14%	0.025%
7	5.034	312	314	317	rVV4	766	1148	0.15%	0.026%
8	5.058	317	318	324	rVV6	1172	1448	0.19%	0.033%
9	5.105	324	326	331	rVB5	1403	1084	0.14%	0.024%
10	5.434	378	382	385	rBV6	1334	2322	0.30%	0.052%
11	5.505	393	394	396	rBV2	1185	938	0.12%	0.021%
12	5.658	417	420	422	rVB4	828	939	0.12%	0.021%
13	6.416	547	549	551	rVB3	1264	1046	0.14%	0.024%
14	6.863	622	625	626	rBV3	1004	1023	0.13%	0.023%
15	7.110	662	667	672	rVB4	3274	5087	0.66%	0.115%
16	7.240	687	689	692	rBV3	939	924	0.12%	0.021%
17	7.310	696	701	705	rBV6	3594	5814	0.76%	0.131%
18	7.422	716	720	724	rBV7	1795	2804	0.37%	0.063%
19	7.499	727	733	740	rBV4	3691	6397	0.83%	0.144%
20	7.775	773	780	788	rBV	192892	306377	39.96%	6.911%
21	7.875	794	797	800	rBV5	921	1594	0.21%	0.036%
22	8.087	831	833	837	rBV4	776	1175	0.15%	0.027%
23	8.234	855	858	862	rVB5	779	1115	0.15%	0.025%
24	8.310	865	871	876	rBV8	2672	5499	0.72%	0.124%
25	8.499	898	903	907	rBV6	2197	3385	0.44%	0.076%
26	8.622	921	924	928	rVB6	1862	2404	0.31%	0.054%
27	8.746	943	945	947	rBV3	1026	1083	0.14%	0.024%
28	8.928	972	976	986	rVB7	3275	7781	1.01%	0.176%
29	9.110	1003	1007	1008	rBV4	668	939	0.12%	0.021%
30	9.128	1008	1010	1014	rVB5	715	929	0.12%	0.021%
31	9.240	1026	1029	1036	rVB7	2505	5376	0.70%	0.121%
32	9.304	1036	1040	1042	rBV5	954	1369	0.18%	0.031%
33	9.657	1095	1100	1105	rBV8	2849	4988	0.65%	0.113%
34	9.963	1150	1152	1155	rBV4	777	954	0.12%	0.022%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP021721\
 Data File : BP004804.D
 Acq On : 18 Feb 2021 11:14
 Operator : CG/JU
 Sample : M1407-07DL2 50X
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBGK7DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
 Title : SVOA CALIBRATION

35	10.146	1181	1183	1186	rVB4	1071	940	0.12%	0.021%
36	10.204	1186	1193	1200	rBV4	3447	8185	1.07%	0.185%
37	10.310	1208	1211	1214	rBV5	1008	1393	0.18%	0.031%
38	10.410	1227	1228	1233	rVV5	819	982	0.13%	0.022%
39	10.469	1235	1238	1242	rVB6	774	1038	0.14%	0.023%
40	10.569	1247	1255	1259	rVV	247141	418596	54.60%	9.442%
41	10.616	1259	1263	1273	rVV	271987	437063	57.01%	9.859%
42	10.681	1273	1274	1277	rVV3	1318	1660	0.22%	0.037%
43	10.734	1277	1283	1292	rVV	17878	33217	4.33%	0.749%
44	10.946	1314	1319	1322	rVB6	643	1129	0.15%	0.025%
45	11.457	1402	1406	1407	rBV4	864	1122	0.15%	0.025%
46	11.516	1413	1416	1421	rVB6	851	1428	0.19%	0.032%
47	11.669	1439	1442	1447	rBV7	1330	1850	0.24%	0.042%
48	12.128	1518	1520	1525	rVB4	1194	1792	0.23%	0.040%
49	12.234	1532	1538	1546	rBV	26203	43467	5.67%	0.980%
50	12.316	1550	1552	1555	rVB3	1142	1279	0.17%	0.029%
51	12.363	1555	1560	1563	rBV6	1686	3224	0.42%	0.073%
52	12.398	1563	1566	1567	rBV3	1164	984	0.13%	0.022%
53	12.457	1567	1576	1582	rBV2	15329	27031	3.53%	0.610%
54	12.734	1619	1623	1626	rVV5	899	1793	0.23%	0.040%
55	12.763	1626	1628	1632	rVB5	919	1190	0.16%	0.027%
56	12.940	1655	1658	1661	rBV5	761	929	0.12%	0.021%
57	13.104	1683	1686	1689	rVB5	726	980	0.13%	0.022%
58	13.175	1696	1698	1703	rVV6	1173	1842	0.24%	0.042%
59	13.251	1706	1711	1718	rVB2	7840	14030	1.83%	0.316%
60	13.392	1732	1735	1739	rVB6	948	1300	0.17%	0.029%
61	13.445	1742	1744	1747	rBV4	941	1100	0.14%	0.025%
62	13.592	1763	1769	1776	rVB4	3245	6701	0.87%	0.151%
63	13.734	1789	1793	1795	rBV4	1716	2525	0.33%	0.057%
64	13.798	1801	1804	1805	rBV3	1695	1889	0.25%	0.043%
65	13.834	1805	1810	1817	rVB3	11294	17777	2.32%	0.401%
66	14.116	1853	1858	1861	rBV2	9690	15328	2.00%	0.346%
67	14.181	1867	1869	1871	rVB3	1105	918	0.12%	0.021%
68	14.422	1902	1910	1916	rBV2	385344	563350	73.48%	12.708%
69	14.487	1916	1921	1927	rVV	26991	41668	5.43%	0.940%
70	14.557	1928	1933	1939	rVB2	6521	10209	1.33%	0.230%
71	14.775	1968	1970	1973	rBV4	803	1080	0.14%	0.024%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP021721\
 Data File : BP004804.D
 Acq On : 18 Feb 2021 11:14
 Operator : CG/JU
 Sample : M1407-07DL2 50X
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBGK7DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
 Title : SVOA CALIBRATION

72	14.822	1973	1978	1984	rVV	20201	30181	3.94%	0.681%
73	14.887	1987	1989	1995	rVB7	1047	1337	0.17%	0.030%
74	14.975	1998	2004	2007	rBV8	3798	6599	0.86%	0.149%
75	15.057	2014	2018	2022	rVV6	1690	2577	0.34%	0.058%
76	15.110	2025	2027	2029	rVB3	1332	946	0.12%	0.021%
77	15.198	2041	2042	2045	rVB3	1303	1102	0.14%	0.025%
78	15.251	2049	2051	2053	rBV3	1234	1075	0.14%	0.024%
79	15.416	2074	2079	2084	rBV3	15966	26187	3.42%	0.591%
80	15.475	2084	2089	2094	rVV	15196	22572	2.94%	0.509%
81	15.516	2094	2096	2099	rVB4	1395	1031	0.13%	0.023%
82	15.545	2099	2101	2103	rBV3	1072	1193	0.16%	0.027%
83	15.769	2137	2139	2142	rBV4	1583	1964	0.26%	0.044%
84	15.904	2160	2162	2164	rBV3	1653	1534	0.20%	0.035%
85	15.922	2164	2165	2168	rVB3	1564	1095	0.14%	0.025%
86	16.151	2202	2204	2208	rVB4	2833	2840	0.37%	0.064%
87	16.304	2226	2230	2233	rVB5	2055	2233	0.29%	0.050%
88	16.334	2233	2235	2236	rBV2	1338	975	0.13%	0.022%
89	16.369	2239	2241	2243	rBV3	1291	1225	0.16%	0.028%
90	16.445	2251	2254	2256	rBV4	2964	3571	0.47%	0.081%
91	16.657	2289	2290	2293	rBV3	2314	2082	0.27%	0.047%
92	16.792	2312	2313	2315	rBV2	1581	1016	0.13%	0.023%
93	16.833	2315	2320	2323	rVV7	5594	8968	1.17%	0.202%
94	16.886	2327	2329	2330	rVB2	1913	1140	0.15%	0.026%
95	17.175	2372	2378	2384	rBV	453711	666837	86.98%	15.042%
96	17.275	2390	2395	2399	rBV2	17153	23431	3.06%	0.529%
97	17.586	2444	2448	2453	rBV	26570	37621	4.91%	0.849%
98	19.516	2772	2776	2779	rBV	20941	28379	3.70%	0.640%
99	21.257	3068	3072	3079	rBV	590027	766680	100.00%	17.294%
100	23.568	3460	3465	3474	rVB	383395	728047	94.96%	16.423%


Sum of corrected areas: 4433199

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP021721\
Data File : BP004804.D
Acq On : 18 Feb 2021 11:14
Operator : CG/JU
Sample : M1407-07DL2 50X
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBGK7DL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

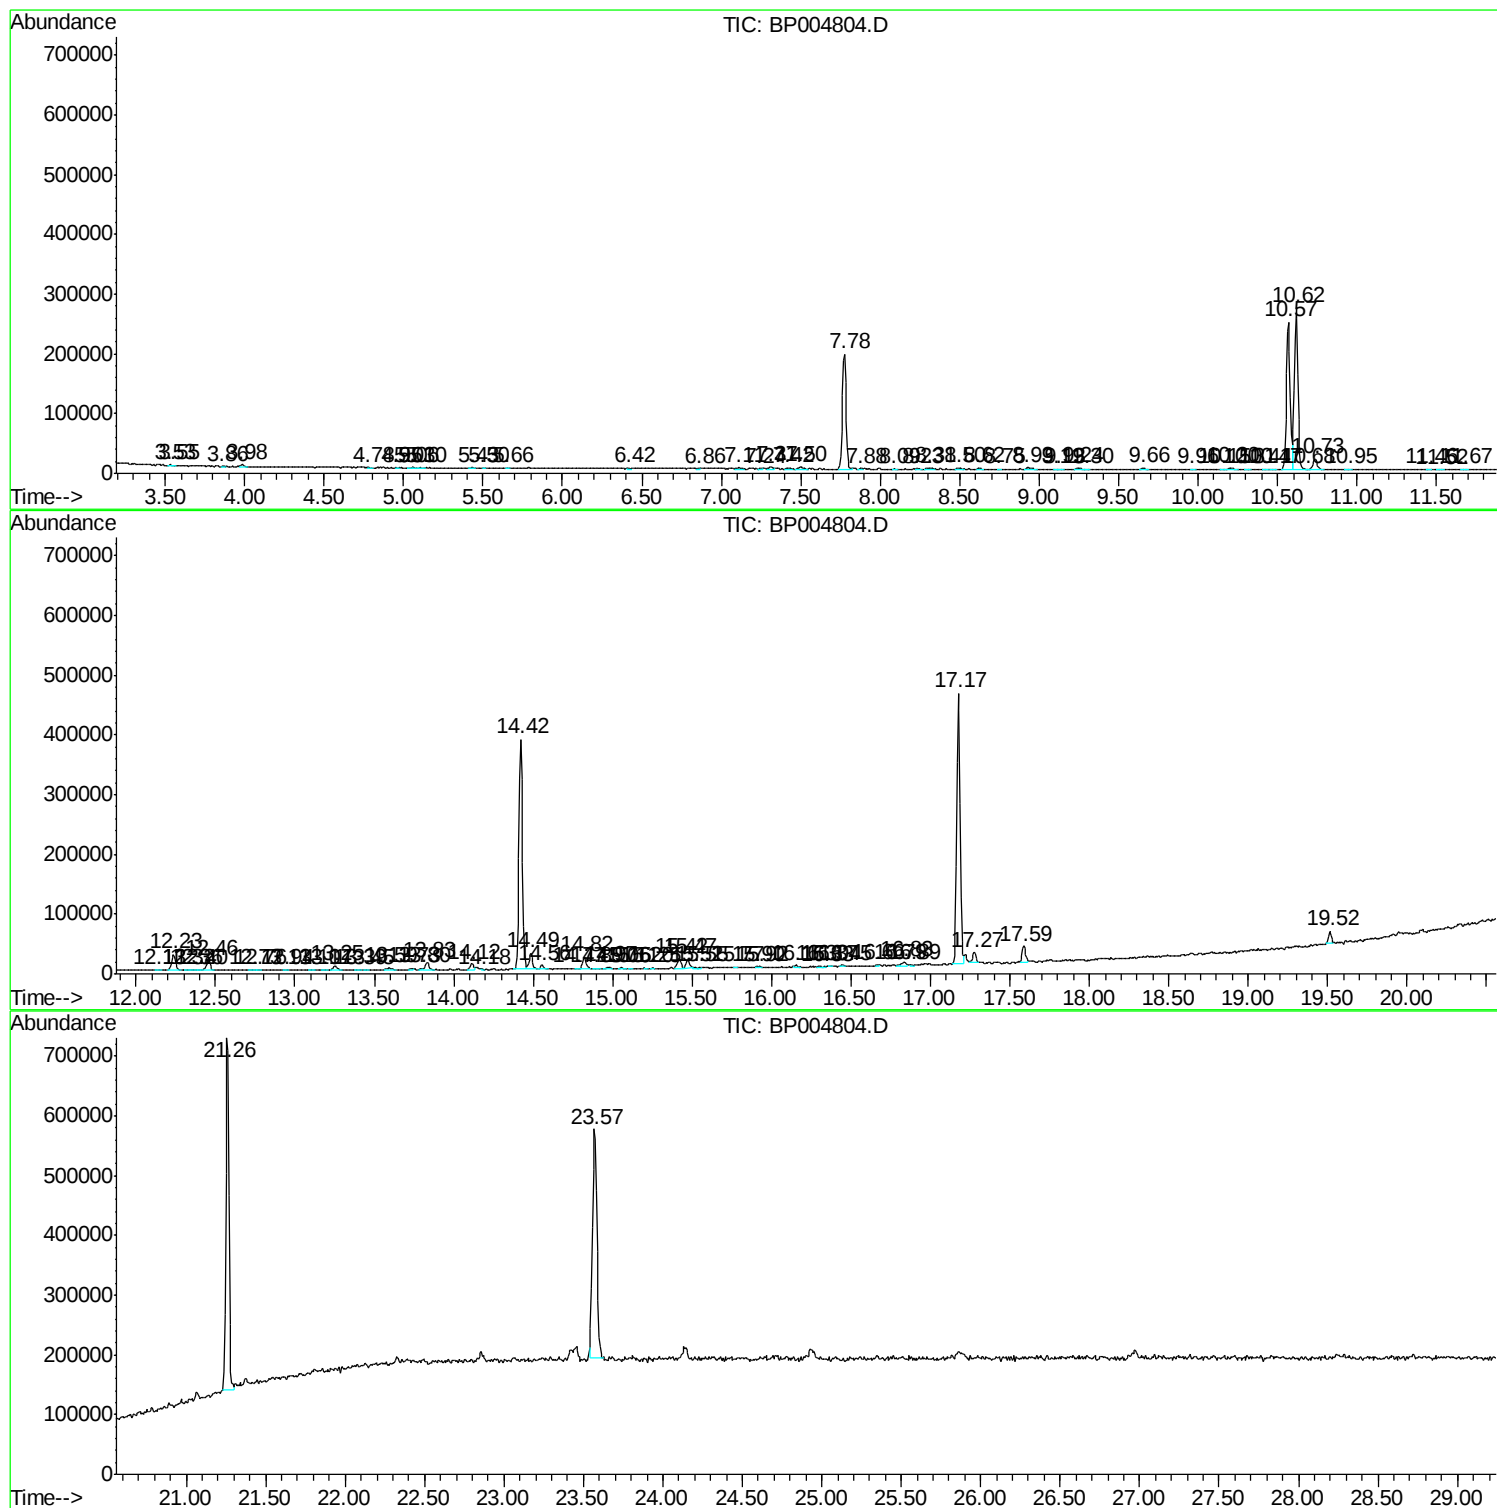

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP021721\
Data File : BP004804.D
Acq On : 18 Feb 2021 11:14
Operator : CG/JU
Sample : M1407-07DL2 50X
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBGK7DL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP021721\
Data File : BP004804.D
Acq On : 18 Feb 2021 11:14
Operator : CG/JU
Sample : M1407-07DL2 50X
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBGK7DL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc