

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP021721\
 Data File : BP004805.D
 Acq On : 18 Feb 2021 11:48
 Operator : CG/JU
 Sample : PB134658BL
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK58

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	7	11	15	rVB	11538	12936	1.30%	0.138%
2	3.563	62	64	68	rVB5	2248	2090	0.21%	0.022%
3	3.599	68	70	72	rBV3	2091	1778	0.18%	0.019%
4	3.710	87	89	92	rVB4	1662	1608	0.16%	0.017%
5	3.922	123	125	127	rBV2	1535	1178	0.12%	0.013%
6	3.975	132	134	139	rVV5	1806	2385	0.24%	0.025%
7	4.063	147	149	151	rVB3	1658	1147	0.12%	0.012%
8	4.087	151	153	155	rBV3	1215	1317	0.13%	0.014%
9	4.299	185	189	191	rBV5	1313	1753	0.18%	0.019%
10	4.363	198	200	205	rVB6	1266	1125	0.11%	0.012%
11	4.404	205	207	209	rBV3	1297	1211	0.12%	0.013%
12	5.969	472	473	477	rBV3	1001	1076	0.11%	0.011%
13	6.181	507	509	512	rBV3	1165	1159	0.12%	0.012%
14	6.946	633	639	648	rVV	195295	300149	30.26%	3.204%
15	7.098	659	665	674	rVB	142599	216203	21.79%	2.308%
16	7.298	692	699	710	rVB	209352	341100	34.39%	3.641%
17	7.463	724	727	730	rVV5	1001	1000	0.10%	0.011%
18	7.763	771	778	786	rBV	132365	211398	21.31%	2.257%
19	8.134	835	841	843	rBV7	839	1623	0.16%	0.017%
20	8.198	849	852	854	rVB4	1143	1106	0.11%	0.012%
21	8.281	865	866	869	rBV3	1240	1112	0.11%	0.012%
22	8.481	890	900	912	rBV	232746	371259	37.43%	3.963%
23	8.922	968	975	986	rBV2	173275	283370	28.57%	3.025%
24	8.998	986	988	991	rVB4	911	1043	0.11%	0.011%
25	9.492	1068	1072	1075	rVB6	1327	1506	0.15%	0.016%
26	9.645	1090	1098	1106	rBV	146297	247287	24.93%	2.640%
27	10.187	1182	1190	1199	rBV	228120	382141	38.52%	4.079%
28	10.322	1211	1213	1217	rVB5	1175	1396	0.14%	0.015%
29	10.557	1246	1253	1263	rBV	161546	273252	27.55%	2.917%
30	10.698	1270	1277	1296	rBV	189485	342530	34.53%	3.657%
31	11.392	1391	1395	1396	rBV4	932	1376	0.14%	0.015%
32	12.157	1519	1525	1531	rBV5	3781	6481	0.65%	0.069%
33	12.363	1557	1560	1563	rBV5	991	1504	0.15%	0.016%
34	12.910	1650	1653	1657	rBV6	1177	1567	0.16%	0.017%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP021721\
 Data File : BP004805.D
 Acq On : 18 Feb 2021 11:48
 Operator : CG/JU
 Sample : PB134658BL
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK58

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
 Title : SVOA CALIBRATION

35	13.098	1683	1685	1688	rBV3	963	1284	0.13%	0.014%
36	13.822	1802	1808	1817	rBV	348852	497241	50.12%	5.308%
37	14.104	1849	1856	1868	rBV	413852	599240	60.41%	6.397%
38	14.275	1881	1885	1887	rBV5	1147	1340	0.14%	0.014%
39	14.416	1902	1909	1917	rVB	213538	329273	33.19%	3.515%
40	14.528	1925	1928	1930	rBV4	1415	1106	0.11%	0.012%
41	14.639	1940	1947	1962	rBV	101451	202922	20.46%	2.166%
42	14.933	1995	1997	2002	rVV6	1573	1647	0.17%	0.018%
43	15.045	2012	2016	2019	rBV6	1283	1610	0.16%	0.017%
44	15.198	2040	2042	2045	rBV4	1096	1639	0.17%	0.017%
45	15.322	2060	2063	2065	rBV4	1204	1253	0.13%	0.013%
46	15.410	2071	2078	2084	rBV	489298	692966	69.86%	7.397%
47	15.527	2092	2098	2107	rBV	129719	185770	18.73%	1.983%
48	15.651	2115	2119	2124	rVB2	6255	9662	0.97%	0.103%
49	15.845	2149	2152	2154	rBV4	1282	1837	0.19%	0.020%
50	16.022	2179	2182	2183	rBV3	1542	1713	0.17%	0.018%
51	16.092	2192	2194	2196	rBV2	1663	1494	0.15%	0.016%
52	16.204	2207	2213	2217	rBV9	2800	5398	0.54%	0.058%
53	16.298	2221	2229	2230	rBV8	2617	4630	0.47%	0.049%
54	16.492	2259	2262	2266	rVB6	1755	2884	0.29%	0.031%
55	16.592	2278	2279	2283	rBV4	1305	1667	0.17%	0.018%
56	16.798	2311	2314	2315	rVB3	1749	1417	0.14%	0.015%
57	16.933	2333	2337	2339	rBV5	2481	3908	0.39%	0.042%
58	17.169	2371	2377	2384	rBV	247811	350036	35.29%	3.737%
59	17.269	2388	2394	2402	rBV	515388	732718	73.86%	7.822%
60	19.151	2711	2714	2717	rBV2	6229	8249	0.83%	0.088%
61	19.510	2769	2775	2781	rBV	652677	866354	87.33%	9.248%
62	21.251	3067	3071	3077	rBV	330153	408654	41.19%	4.362%
63	23.409	3432	3438	3448	rVB	501079	992002	100.00%	10.590%
64	23.556	3458	3463	3470	rVB2	227862	438534	44.21%	4.681%


Sum of corrected areas: 9367614

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP021721\
Data File : BP004805.D
Acq On : 18 Feb 2021 11:48
Operator : CG/JU
Sample : PB134658BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK58

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

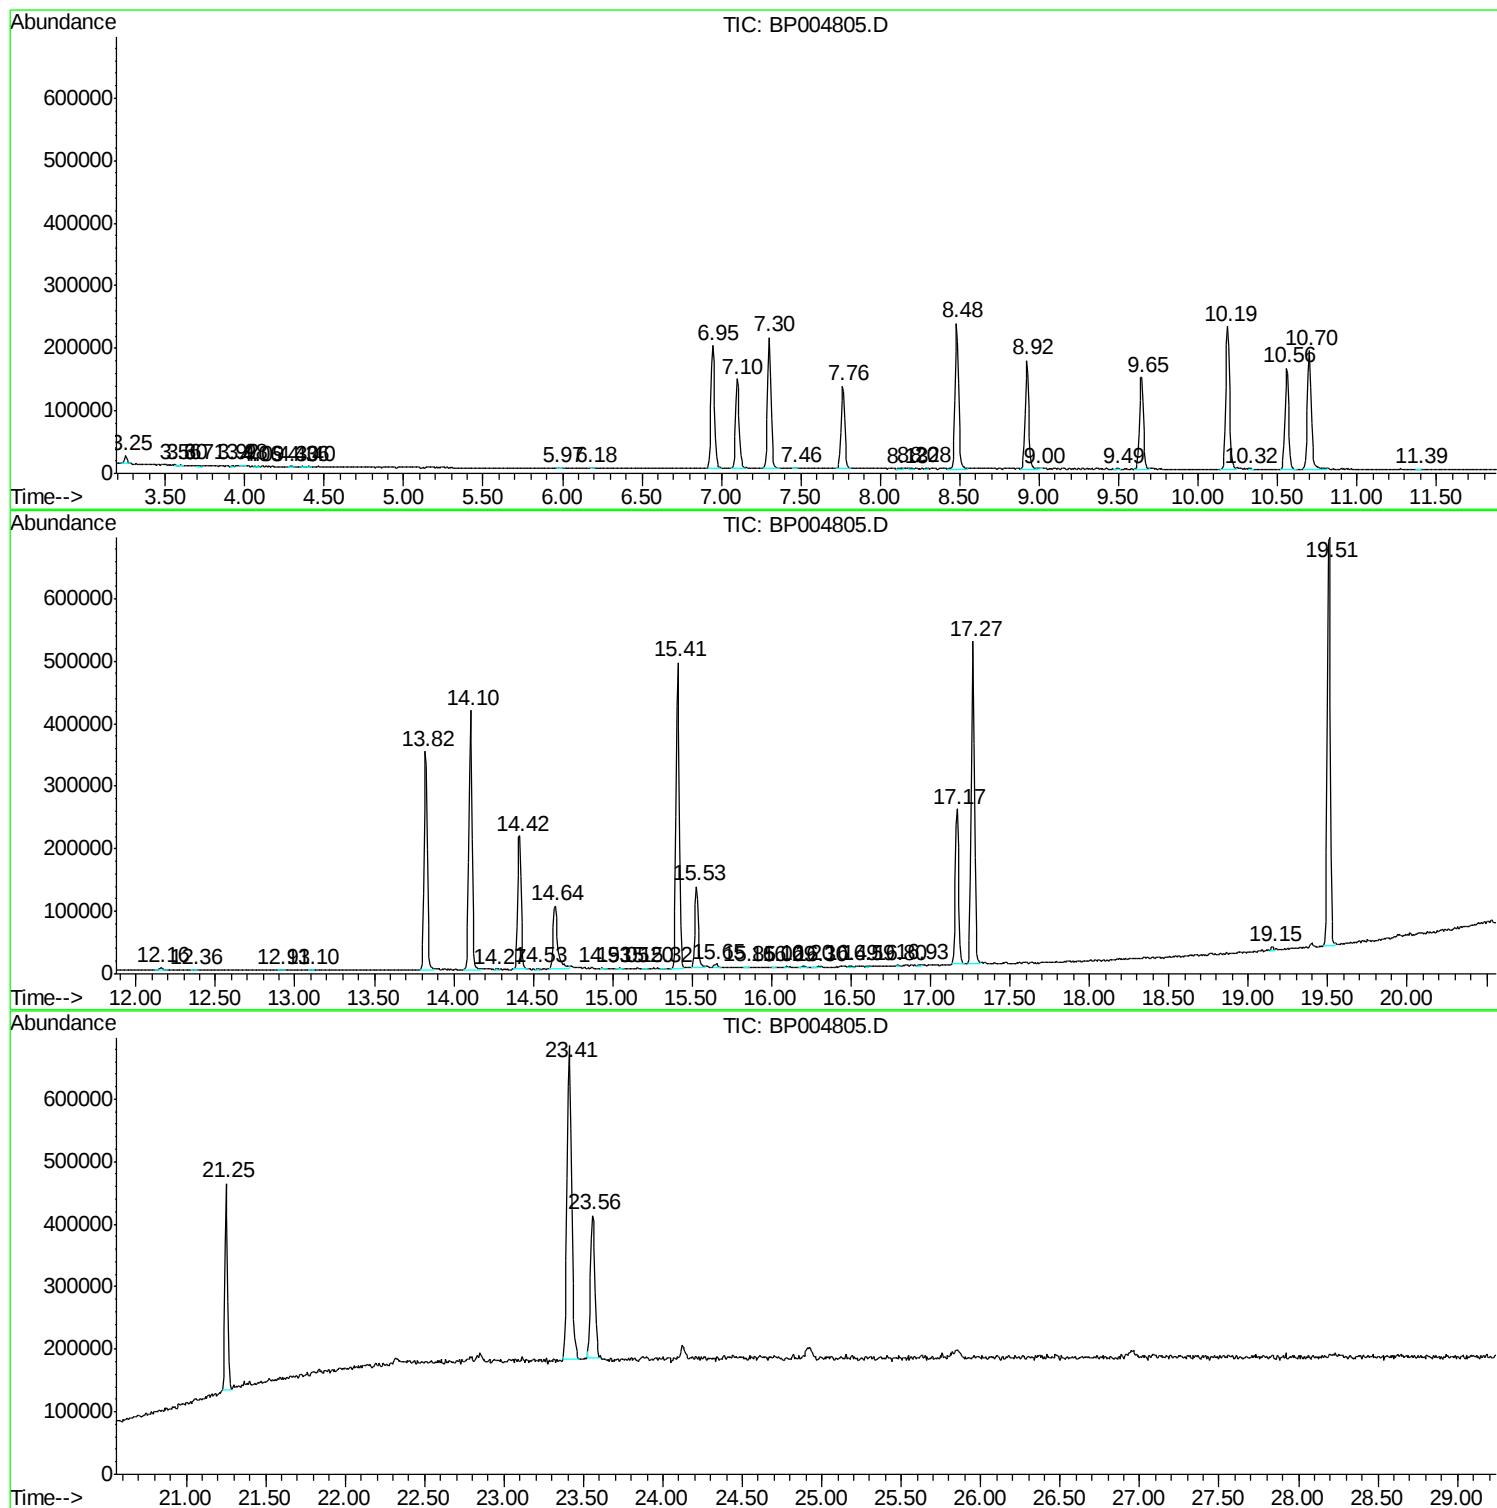

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP021721\
Data File : BP004805.D
Acq On : 18 Feb 2021 11:48
Operator : CG/JU
Sample : PB134658BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK58

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP021721\
Data File : BP004805.D
Acq On : 18 Feb 2021 11:48
Operator : CG/JU
Sample : PB134658BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK58

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc