

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP021721\
 Data File : BP004806.D
 Acq On : 18 Feb 2021 12:22
 Operator : CG/JU
 Sample : M1408-11
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBG4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	8	11	18	rVB2	7604	11100	0.75%	0.090%
2	3.887	115	119	125	rVB9	3020	6312	0.43%	0.051%
3	3.940	125	128	130	rBV4	2025	2152	0.14%	0.018%
4	3.981	132	135	138	rVB4	2503	3427	0.23%	0.028%
5	4.322	191	193	194	rBV2	1827	1641	0.11%	0.013%
6	4.340	194	196	204	rVB8	3024	5416	0.36%	0.044%
7	4.522	225	227	231	rVB5	2128	1848	0.12%	0.015%
8	6.910	631	633	634	rBV2	1965	1548	0.10%	0.013%
9	6.946	634	639	650	rVB2	50882	96389	6.49%	0.784%
10	7.099	659	665	678	rVB	148039	230574	15.53%	1.875%
11	7.299	690	699	707	rBV	185494	302616	20.38%	2.461%
12	7.763	772	778	787	rVB	192127	300630	20.24%	2.445%
13	8.481	891	900	909	rBV	124160	198362	13.36%	1.613%
14	8.922	968	975	983	rBV	194035	316201	21.29%	2.572%
15	9.340	1042	1046	1047	rBV3	2400	2720	0.18%	0.022%
16	9.463	1062	1067	1069	rVB6	1092	1620	0.11%	0.013%
17	9.640	1089	1097	1110	rBV	167068	286630	19.30%	2.331%
18	10.187	1183	1190	1203	rBV	241147	412116	27.75%	3.352%
19	10.557	1244	1253	1261	rBV	245112	408371	27.50%	3.321%
20	10.704	1271	1278	1284	rBV2	14164	26267	1.77%	0.214%
21	11.834	1465	1470	1475	rVB5	3578	6054	0.41%	0.049%
22	12.151	1520	1524	1530	rVB3	3376	5891	0.40%	0.048%
23	12.769	1625	1629	1630	rBV4	1518	2058	0.14%	0.017%
24	13.016	1669	1671	1677	rVB5	1894	2727	0.18%	0.022%
25	13.257	1709	1712	1717	rVB7	1912	2837	0.19%	0.023%
26	13.469	1743	1748	1754	rBV10	1679	3648	0.25%	0.030%
27	13.822	1802	1808	1813	rBV	487881	656373	44.20%	5.338%
28	13.869	1813	1816	1821	rVB	28079	37266	2.51%	0.303%
29	14.104	1845	1856	1866	rBV	520705	775200	52.20%	6.305%
30	14.410	1899	1908	1917	rBV	358453	531896	35.82%	4.326%
31	14.639	1940	1947	1961	rBV2	32751	71107	4.79%	0.578%
32	14.739	1961	1964	1967	rVB4	1634	2390	0.16%	0.019%
33	14.839	1979	1981	1989	rVB9	1647	2803	0.19%	0.023%
34	15.045	2013	2016	2020	rBV6	1738	1974	0.13%	0.016%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP021721\
Data File : BP004806.D
Acq On : 18 Feb 2021 12:22
Operator : CG/JU
Sample : M1408-11
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBGM4

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
Title : SVOA CALIBRATION

35	15.163	2034	2036	2040	rVB4	2247	2256	0.15%	0.018%
36	15.222	2040	2046	2047	rBV5	3742	4865	0.33%	0.040%
37	15.239	2047	2049	2051	rVB2	1954	1513	0.10%	0.012%
38	15.410	2071	2078	2086	rBV	689834	970080	65.32%	7.890%
39	15.528	2092	2098	2107	rBV	222795	293878	19.79%	2.390%
40	15.651	2115	2119	2123	rBV3	8271	10101	0.68%	0.082%
41	15.722	2128	2131	2133	rVB4	1338	1651	0.11%	0.013%
42	16.092	2191	2194	2198	rVB6	2280	2800	0.19%	0.023%
43	16.169	2203	2207	2208	rBV4	1544	1695	0.11%	0.014%
44	16.192	2208	2211	2216	rVV7	2534	3740	0.25%	0.030%
45	16.304	2227	2230	2231	rBV3	1827	1911	0.13%	0.016%
46	16.645	2286	2288	2291	rVB4	2499	2627	0.18%	0.021%
47	16.710	2295	2299	2305	rVV4	10154	13997	0.94%	0.114%
48	16.892	2328	2330	2332	rBV3	1582	1735	0.12%	0.014%
49	17.010	2349	2350	2354	rBV3	1833	2584	0.17%	0.021%
50	17.169	2371	2377	2387	rBV	438930	620582	41.79%	5.047%
51	17.269	2387	2394	2403	rBV	822877	1166826	78.57%	9.490%
52	17.557	2436	2443	2452	rBV	8140	22419	1.51%	0.182%
53	18.057	2526	2528	2532	rVB5	5444	6860	0.46%	0.056%
54	18.292	2566	2568	2571	rBV4	3278	3622	0.24%	0.029%
55	19.151	2711	2714	2719	rVB2	11512	13307	0.90%	0.108%
56	19.504	2769	2774	2782	rBV	1056867	1415472	95.32%	11.512%
57	20.963	3019	3022	3028	rVB8	41717	53175	3.58%	0.432%
58	21.251	3066	3071	3076	rBV	602424	734341	49.45%	5.972%
59	23.410	3431	3438	3448	rVB	796126	1485024	100.00%	12.078%
60	23.557	3457	3463	3471	rVB2	376746	740285	49.85%	6.021%


Sum of corrected areas: 12295510

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP021721\
Data File : BP004806.D
Acq On : 18 Feb 2021 12:22
Operator : CG/JU
Sample : M1408-11
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBGM4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

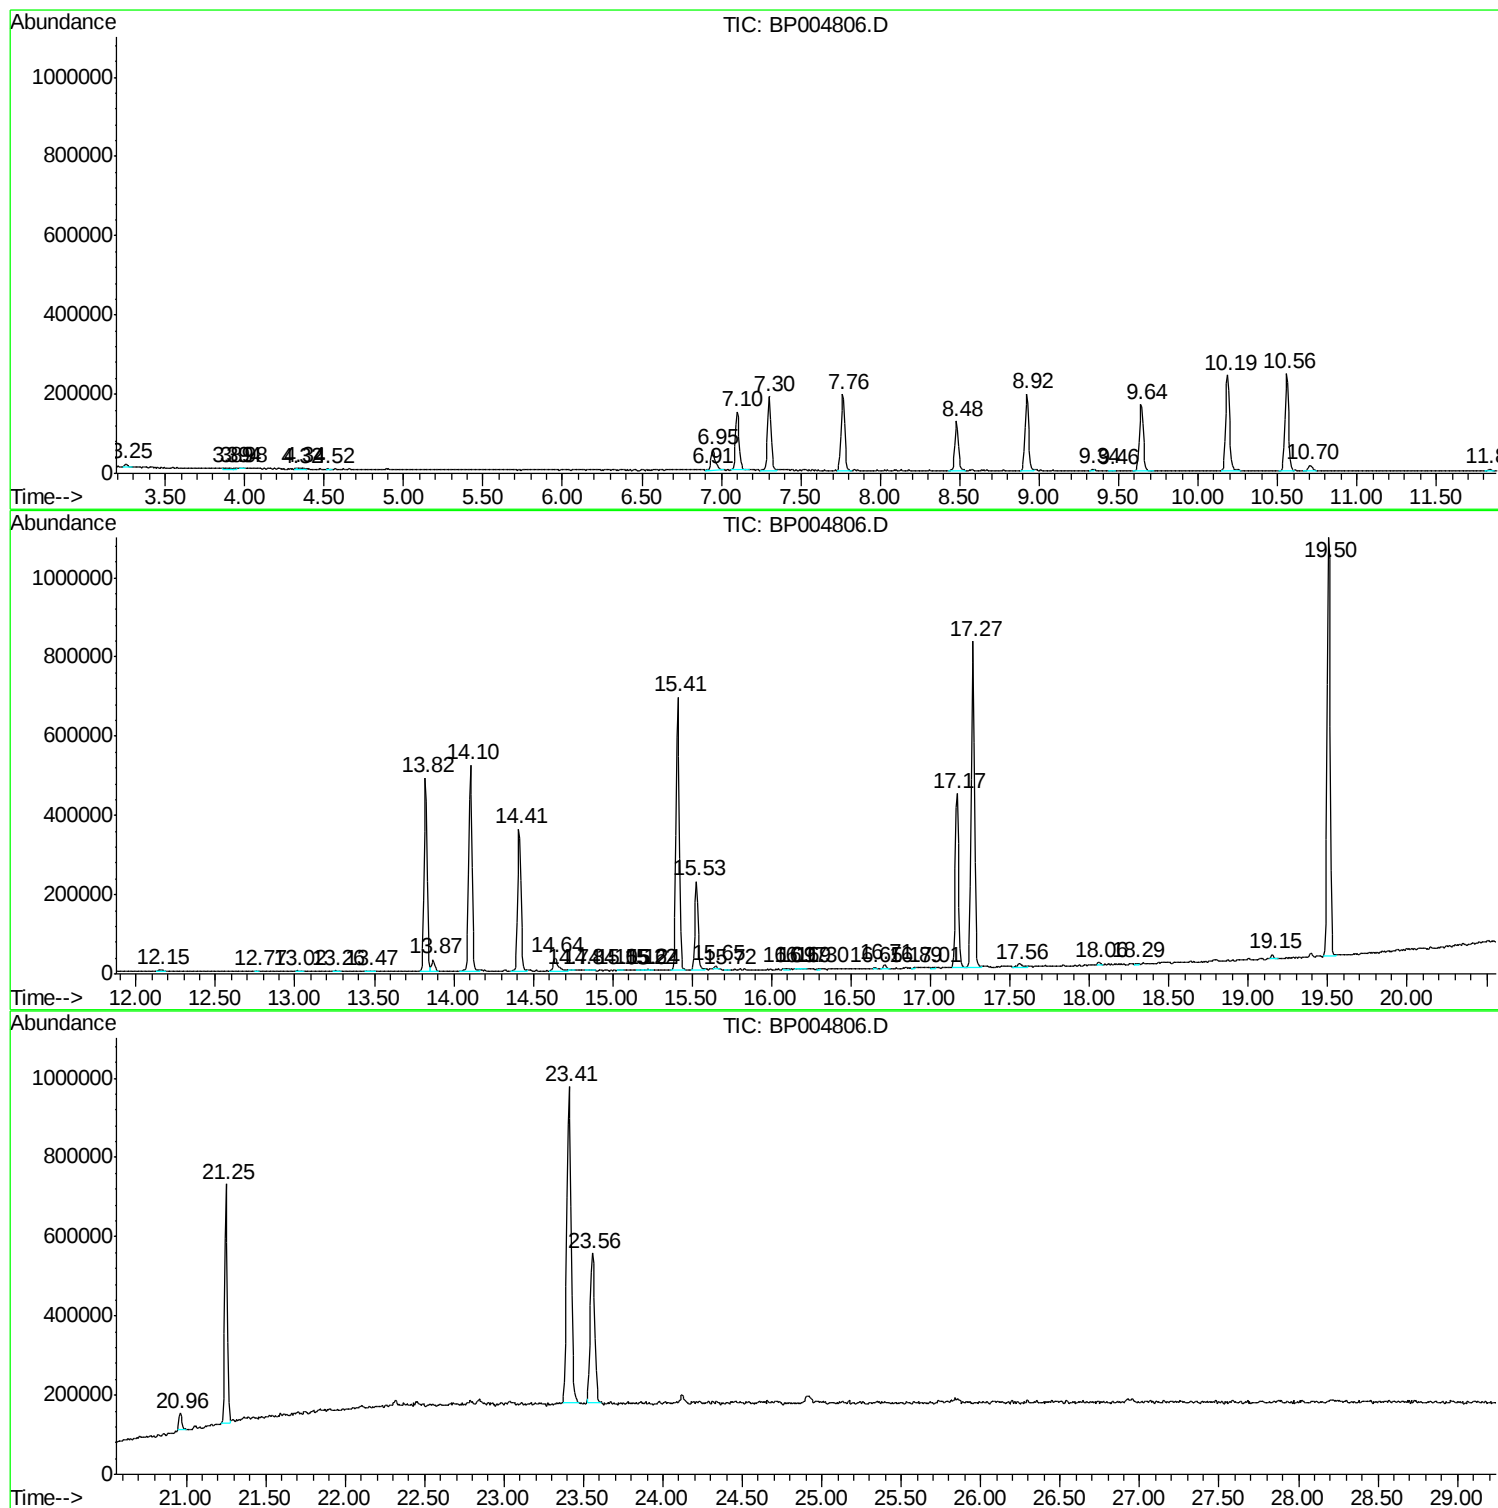

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP021721\
Data File : BP004806.D
Acq On : 18 Feb 2021 12:22
Operator : CG/JU
Sample : M1408-11
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBGM4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP021721\
Data File : BP004806.D
Acq On : 18 Feb 2021 12:22
Operator : CG/JU
Sample : M1408-11
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBGM4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc