

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP021721\
 Data File : BP004807.D
 Acq On : 18 Feb 2021 12:55
 Operator : CG/JU
 Sample : M1408-09
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBGL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	7	11	19	rVB2	12494	20127	1.62%	0.176%
2	3.311	19	21	24	rBV4	1615	1461	0.12%	0.013%
3	3.758	96	97	100	rBV3	1659	1472	0.12%	0.013%
4	3.864	112	115	117	rBV4	1411	1453	0.12%	0.013%
5	3.881	117	118	125	rVB7	2669	4020	0.32%	0.035%
6	3.981	132	135	141	rVB4	4049	5275	0.42%	0.046%
7	4.158	162	165	167	rBV3	1619	1436	0.12%	0.013%
8	4.428	209	211	216	rVB5	1579	2287	0.18%	0.020%
9	4.905	286	292	299	rVB9	2225	5191	0.42%	0.045%
10	4.975	302	304	309	rBV7	1446	2297	0.18%	0.020%
11	5.481	389	390	394	rVB4	1431	1246	0.10%	0.011%
12	6.299	525	529	533	rBV6	1285	1942	0.16%	0.017%
13	6.387	541	544	546	rBV4	929	1375	0.11%	0.012%
14	6.781	606	611	614	rBV6	2072	3950	0.32%	0.035%
15	6.840	619	621	626	rBV6	1287	1733	0.14%	0.015%
16	6.946	633	639	649	rVB3	60965	114460	9.20%	1.003%
17	7.099	659	665	678	rVB	173796	268229	21.56%	2.351%
18	7.299	691	699	708	rBV	226978	358486	28.81%	3.142%
19	7.381	709	713	719	rVV4	4286	8534	0.69%	0.075%
20	7.558	740	743	748	rBV6	1343	2237	0.18%	0.020%
21	7.763	771	778	788	rBV	230215	355323	28.56%	3.114%
22	7.987	813	816	819	rBV5	1194	1303	0.10%	0.011%
23	8.146	840	843	846	rBV5	1056	1341	0.11%	0.012%
24	8.481	893	900	911	rBV	161260	255991	20.57%	2.244%
25	8.922	967	975	984	rBV	216904	353575	28.41%	3.099%
26	9.346	1040	1047	1049	rBV7	2990	5701	0.46%	0.050%
27	9.558	1079	1083	1088	rVB7	1021	1760	0.14%	0.015%
28	9.640	1088	1097	1105	rBV	189742	316226	25.41%	2.772%
29	9.799	1119	1124	1125	rBV5	1064	1406	0.11%	0.012%
30	9.863	1132	1135	1138	rBV5	881	1377	0.11%	0.012%
31	10.187	1183	1190	1208	rVV	268445	453008	36.41%	3.971%
32	10.557	1246	1253	1267	rBV	266352	450904	36.24%	3.952%
33	10.699	1269	1277	1284	rBV2	16907	32487	2.61%	0.285%
34	11.375	1387	1392	1396	rBV8	1360	2308	0.19%	0.020%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP021721\
 Data File : BP004807.D
 Acq On : 18 Feb 2021 12:55
 Operator : CG/JU
 Sample : M1408-09
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBGL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
 Title : SVOA CALIBRATION

35	11.510	1410	1415	1416	rBV5	1098	1314	0.11%	0.012%
36	11.734	1448	1453	1456	rBV7	813	1643	0.13%	0.014%
37	11.804	1462	1465	1467	rBV3	1103	1357	0.11%	0.012%
38	12.063	1504	1509	1511	rBV5	1260	1747	0.14%	0.015%
39	12.152	1519	1524	1531	rVB5	4208	8242	0.66%	0.072%
40	12.769	1624	1629	1630	rBV5	1589	1853	0.15%	0.016%
41	13.016	1667	1671	1676	rBV7	2532	3877	0.31%	0.034%
42	13.257	1703	1712	1716	rBV8	2884	5838	0.47%	0.051%
43	13.310	1717	1721	1724	rBV5	1318	1935	0.16%	0.017%
44	13.469	1744	1748	1753	rVB8	1613	2268	0.18%	0.020%
45	13.546	1757	1761	1765	rBV7	698	1373	0.11%	0.012%
46	13.722	1789	1791	1796	rBV6	1048	1755	0.14%	0.015%
47	13.822	1802	1808	1813	rBV	443652	595805	47.88%	5.222%
48	13.869	1813	1816	1821	rVB	24458	32822	2.64%	0.288%
49	13.940	1826	1828	1835	rVB8	1702	3282	0.26%	0.029%
50	14.104	1846	1856	1863	rBV	519220	735802	59.13%	6.449%
51	14.410	1900	1908	1916	rBV2	357705	523581	42.08%	4.589%
52	14.475	1916	1919	1922	rVV4	3642	4559	0.37%	0.040%
53	14.540	1926	1930	1931	rBV4	1154	1603	0.13%	0.014%
54	14.640	1940	1947	1962	rBV2	26645	64423	5.18%	0.565%
55	15.010	2008	2010	2013	rBV4	1692	2290	0.18%	0.020%
56	15.057	2015	2018	2019	rVV3	1326	1260	0.10%	0.011%
57	15.210	2041	2044	2047	rBV4	1435	2031	0.16%	0.018%
58	15.410	2071	2078	2085	rBV	589521	865108	69.52%	7.583%
59	15.528	2092	2098	2106	rBV	170433	242013	19.45%	2.121%
60	15.651	2113	2119	2123	rBV3	7279	12699	1.02%	0.111%
61	15.734	2130	2133	2135	rBV4	1236	1477	0.12%	0.013%
62	15.898	2158	2161	2163	rBV4	1383	1810	0.15%	0.016%
63	16.087	2189	2193	2194	rBV4	1751	2638	0.21%	0.023%
64	16.140	2200	2202	2204	rBV3	1545	1447	0.12%	0.013%
65	16.204	2209	2213	2215	rVB5	3760	5043	0.41%	0.044%
66	16.263	2221	2223	2226	rVB4	1638	1513	0.12%	0.013%
67	16.475	2257	2259	2262	rVB4	2020	1809	0.15%	0.016%
68	16.534	2265	2269	2271	rBV4	1219	1855	0.15%	0.016%
69	16.628	2281	2285	2286	rBV4	1735	2225	0.18%	0.020%
70	16.839	2319	2321	2327	rBV7	1994	3997	0.32%	0.035%
71	16.904	2330	2332	2333	rBV2	1896	1591	0.13%	0.014%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP021721\
 Data File : BP004807.D
 Acq On : 18 Feb 2021 12:55
 Operator : CG/JU
 Sample : M1408-09
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBGL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
 Title : SVOA CALIBRATION

72	16.939	2336	2338	2339	rBV2	2034	1820	0.15%	0.016%
73	17.169	2370	2377	2386	rBV	385363	554790	44.59%	4.863%
74	17.263	2387	2393	2404	rBV	672402	920967	74.01%	8.072%
75	17.498	2431	2433	2435	rBV2	2369	1863	0.15%	0.016%
76	18.004	2517	2519	2521	rBV2	2859	3059	0.25%	0.027%
77	18.057	2526	2528	2533	rVB6	5209	6330	0.51%	0.055%
78	19.504	2769	2774	2782	rBV	801035	1056800	84.93%	9.263%
79	20.963	3019	3022	3027	rBV3	47772	65833	5.29%	0.577%
80	21.251	3066	3071	3080	rBV	538235	661211	53.14%	5.796%
81	23.410	3431	3438	3449	rVB	641570	1244342	100.00%	10.907%
82	23.557	3457	3463	3472	rVB2	363406	706176	56.75%	6.190%


Sum of corrected areas: 11408997

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP021721\
Data File : BP004807.D
Acq On : 18 Feb 2021 12:55
Operator : CG/JU
Sample : M1408-09
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBGL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

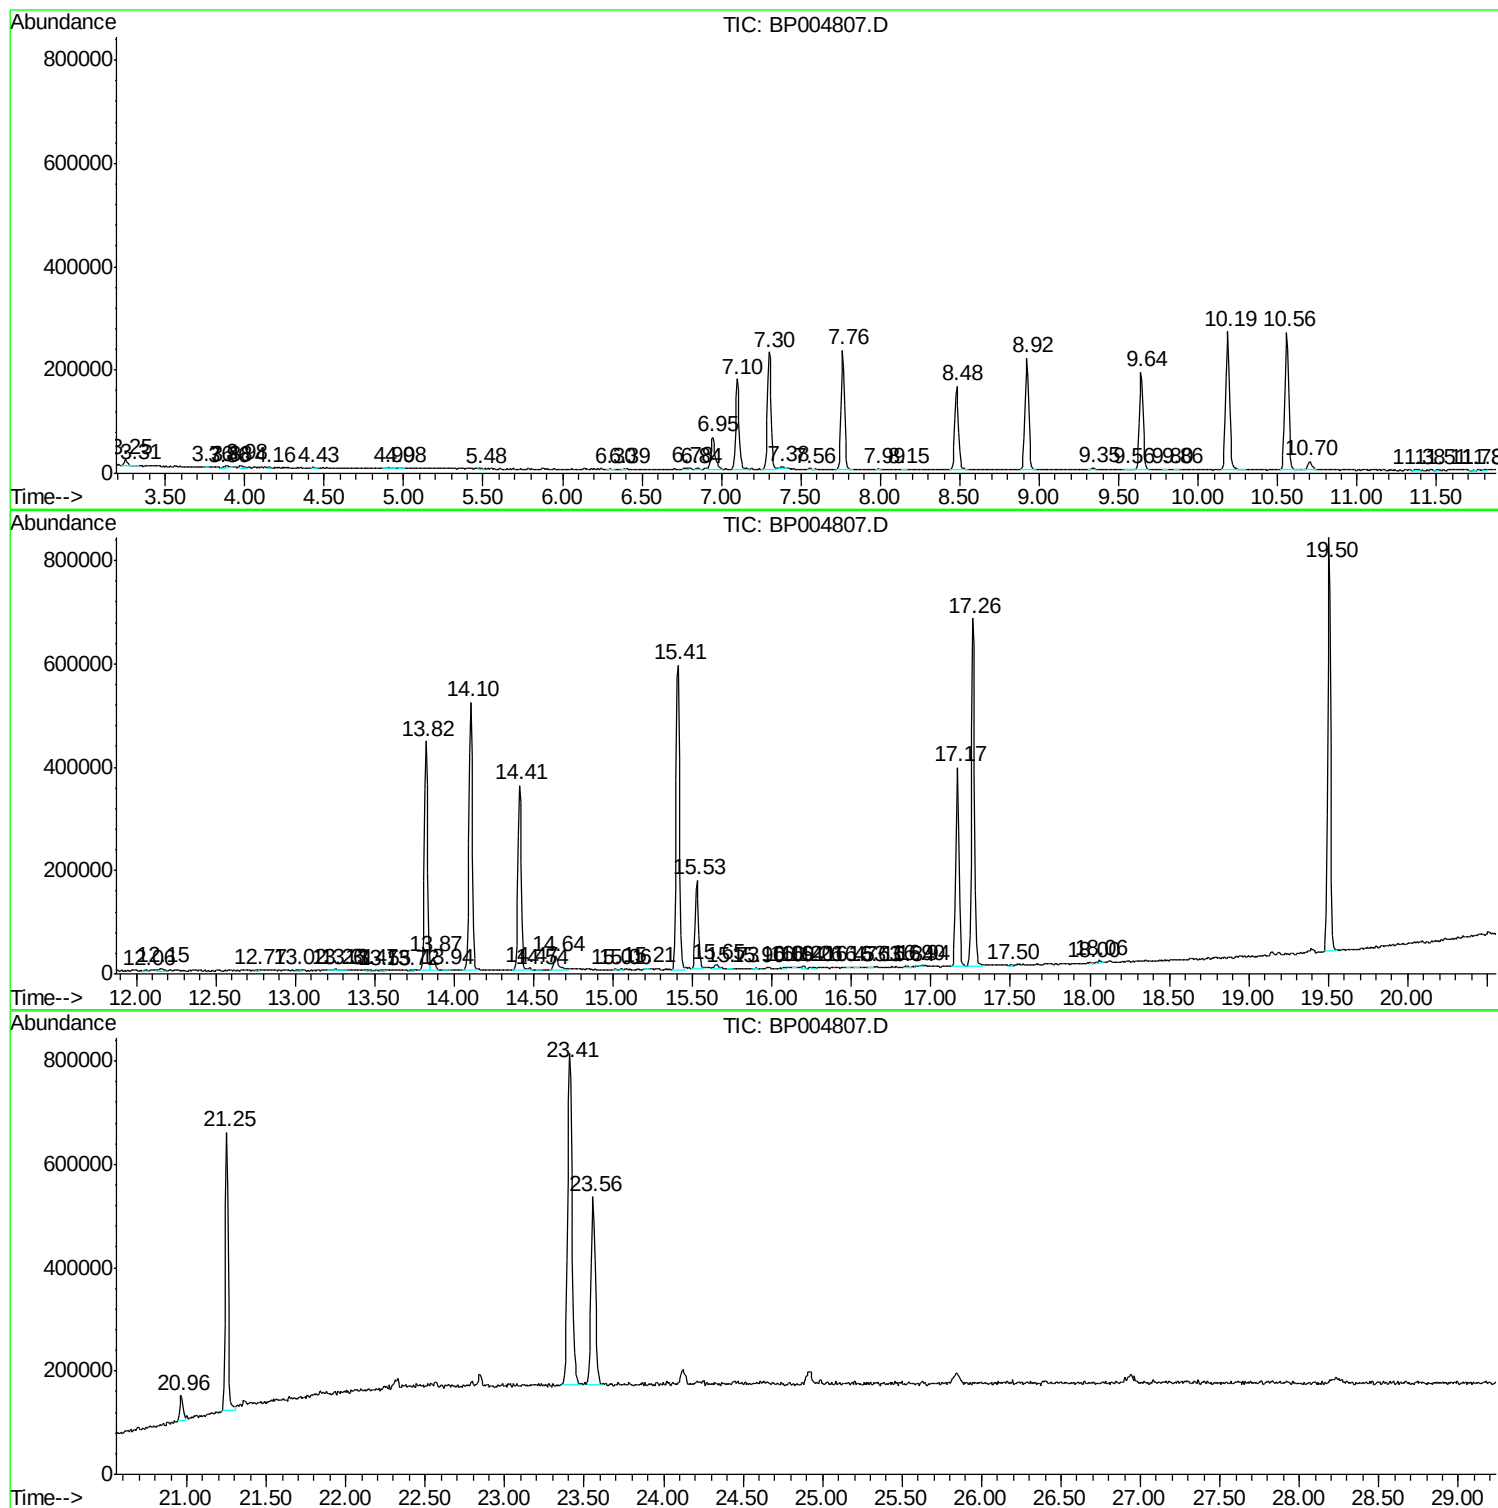

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP021721\
Data File : BP004807.D
Acq On : 18 Feb 2021 12:55
Operator : CG/JU
Sample : M1408-09
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBGL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP021721\
Data File : BP004807.D
Acq On : 18 Feb 2021 12:55
Operator : CG/JU
Sample : M1408-09
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBGL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP020821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc