


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021722\
 Data File : BP009191.D
 Acq On : 17 Feb 2022 10:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 16 14:30:24 2022

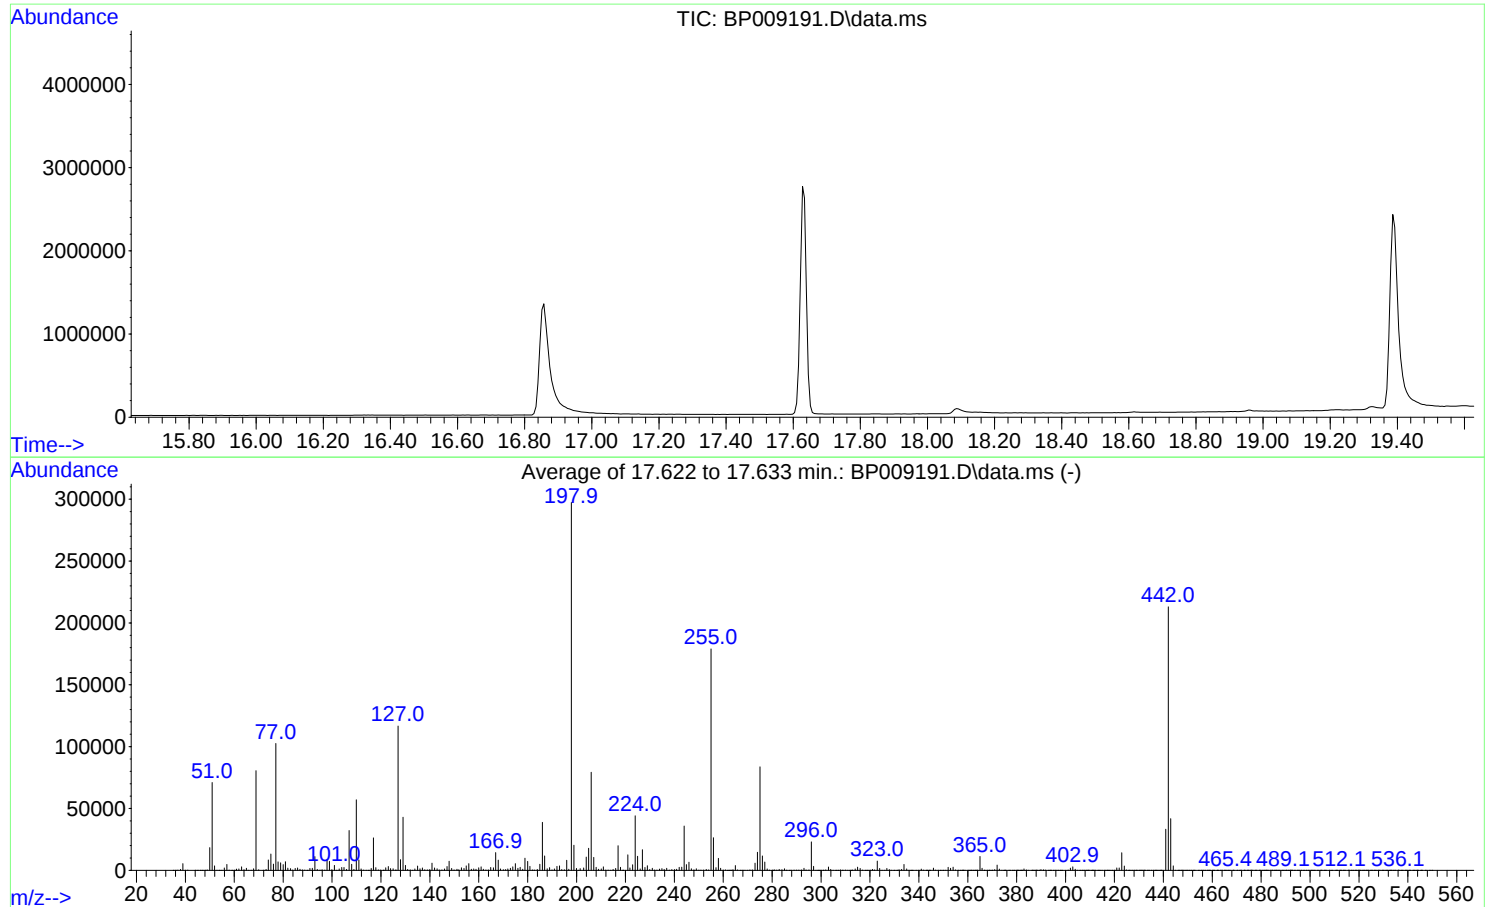




AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.9	71001	PASS
68	69	0.00	2	1.6	1270	PASS
69	198	0.00	100	27.1	80529	PASS
70	69	0.00	2	0.6	464	PASS
127	198	10	80	39.3	116721	PASS
197	198	0.00	2	0.3	909	PASS
198	198	100	100	100.0	297330	PASS
199	198	5	9	6.8	20330	PASS
275	198	10	60	28.1	83680	PASS
365	198	1	100	3.8	11200	PASS
441	198	0.01	100	11.2	33184	PASS
442	442	100	100	100.0	213010	PASS
443	442	15	24	19.6	41781	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021722\
 Data File : BP009191.D
 Acq On : 17 Feb 2022 10:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Feb 18 03:18:16 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 16 14:30:24 2022
 Response via : Initial Calibration

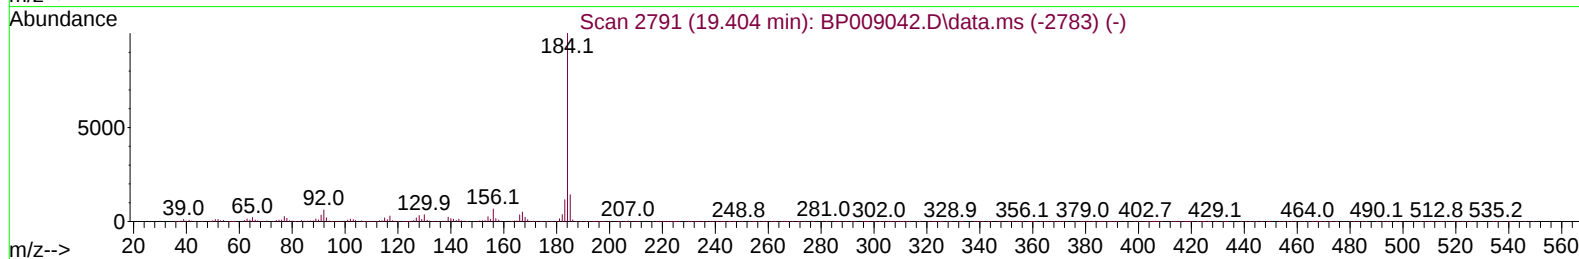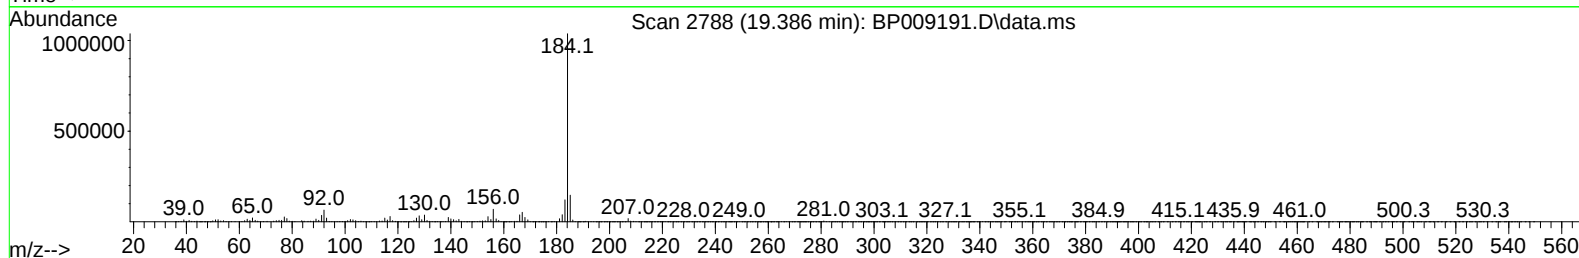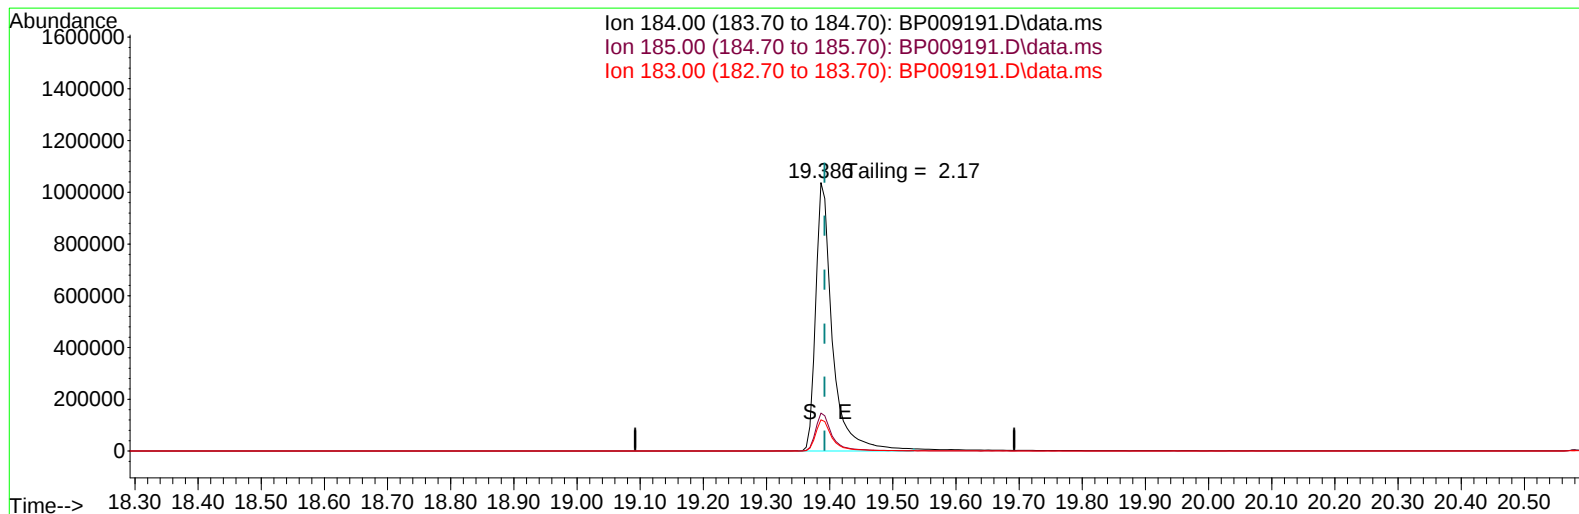

TIC: BP009191.D\data.ms

(77) Benzidine

19.386min (-0.006) 740548.01 ng




response 1934313

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.16
183.00	11.90	11.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021722\
Data File : BP009191.D
Acq On : 17 Feb 2022 10:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 18 03:18:16 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 16 14:30:24 2022
Response via : Initial Calibration

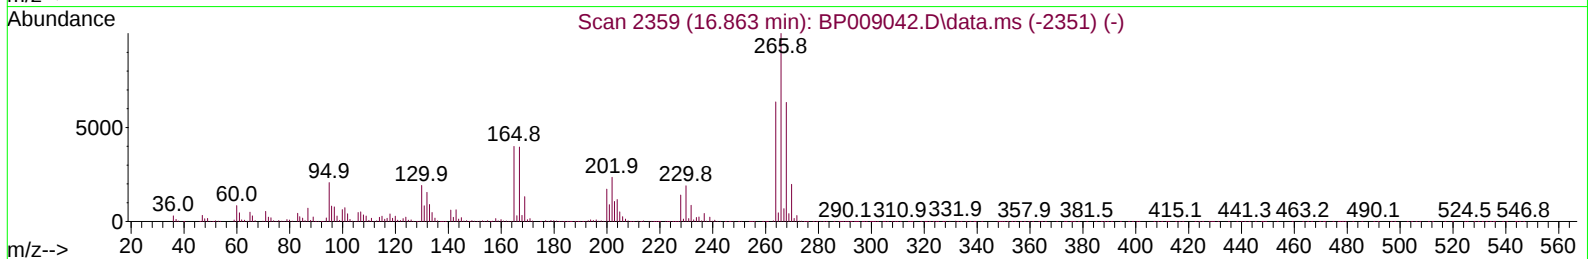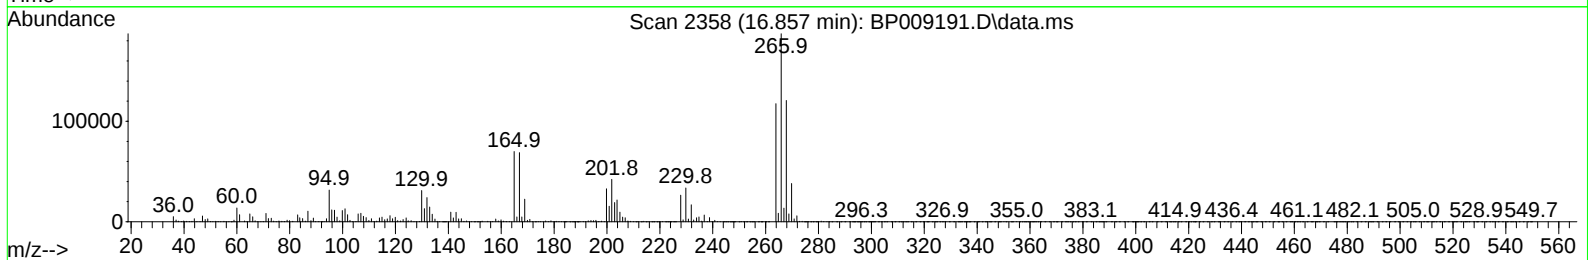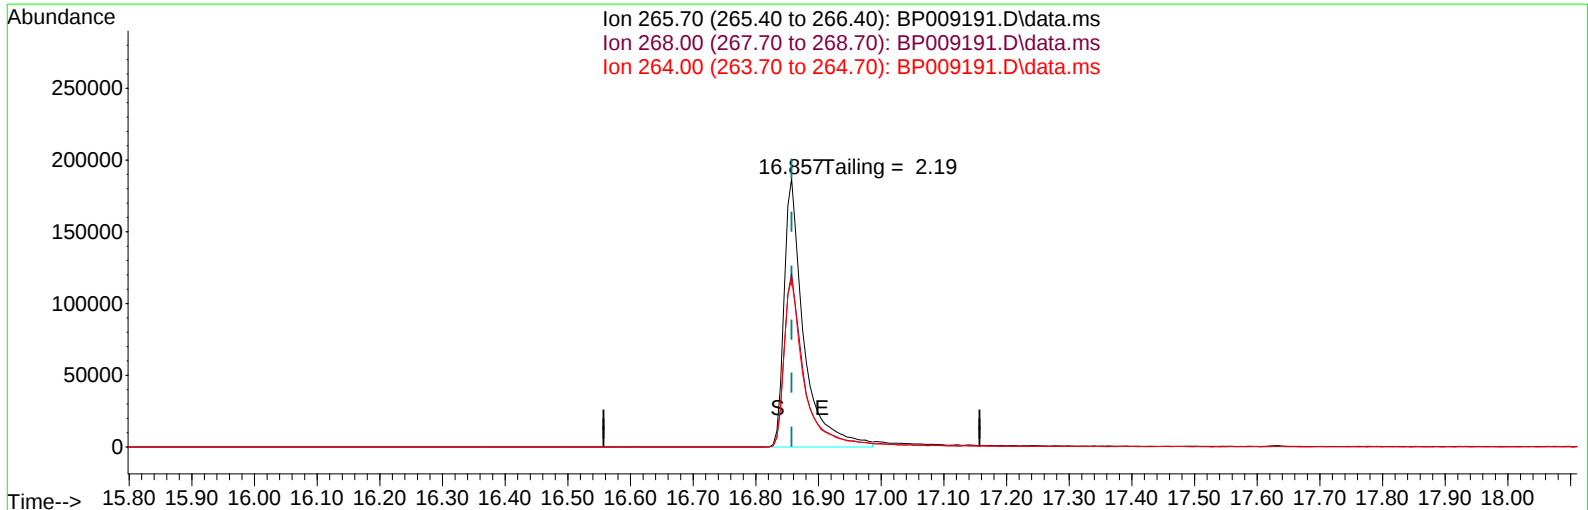

TIC: BP009191.D\data.ms

(70) Pentachlorophenol (C)

16.857min (+ 0.000) 1329671.91 ng

response 427144

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	64.55
264.00	62.90	62.80
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/17/2022	BNA_P	<u>BP009191.D</u>
Compound Name	Response	Retention Time
DDT	1099336	20.58
DDD	32391	20.157
DDE	4036	19.657
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
36427	1135763	3.21

Instrument :
BNA_P
ClientSampleId :
DFTPP