
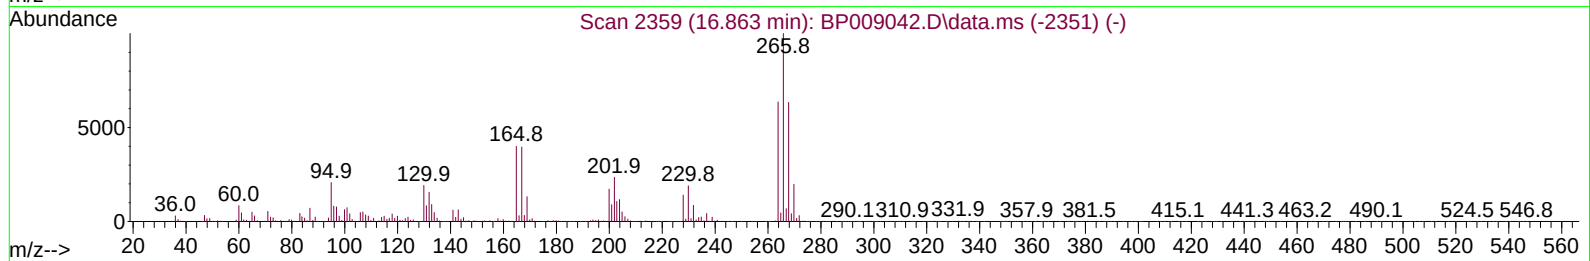
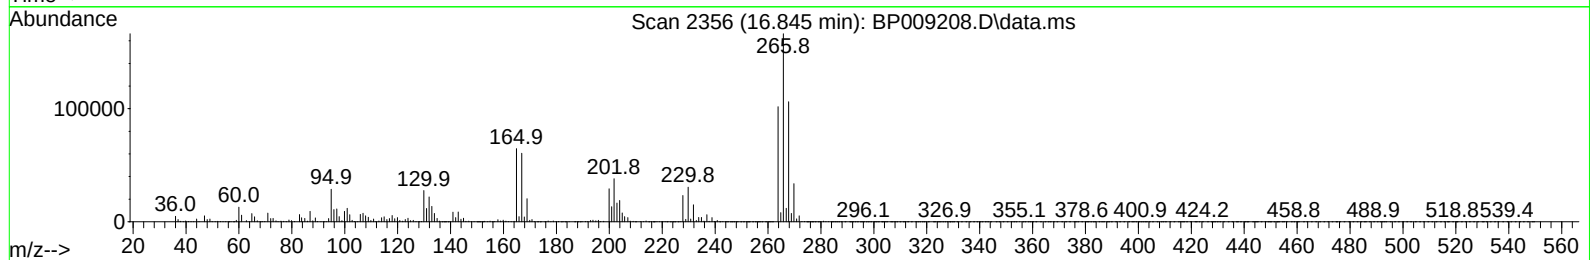


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021822\
Data File : BP009208.D
Acq On : 18 Feb 2022 11:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 19 02:50:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 19 00:46:08 2022
Response via : Initial Calibration

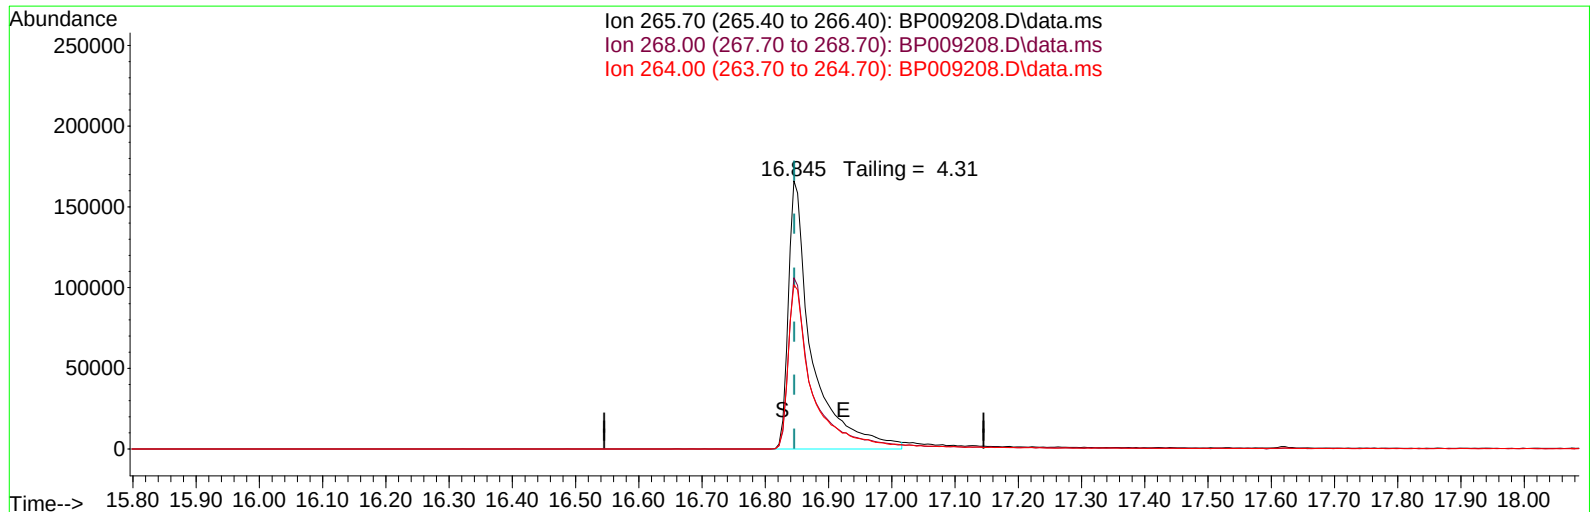

TIC: BP009208.D\data.ms

(70) Pentachlorophenol (C)




16.845min (-0.000) 4329204.64 ng

response 443845

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.82
264.00	62.90	61.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021822\
 Data File : BP009208.D
 Acq On : 18 Feb 2022 11:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 19 02:50:24 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 19 00:46:08 2022
 Response via : Initial Calibration

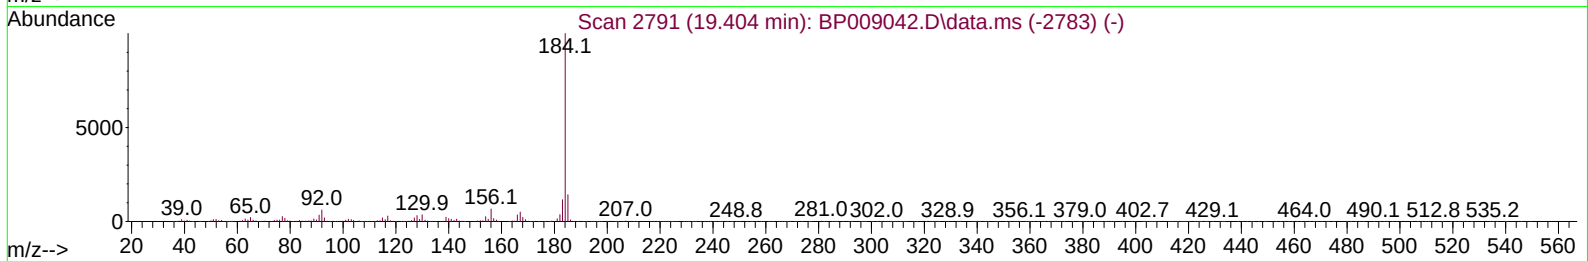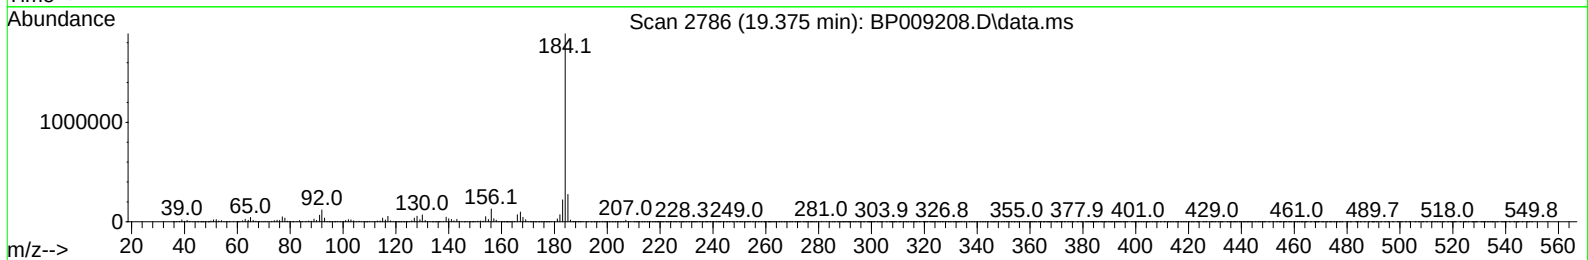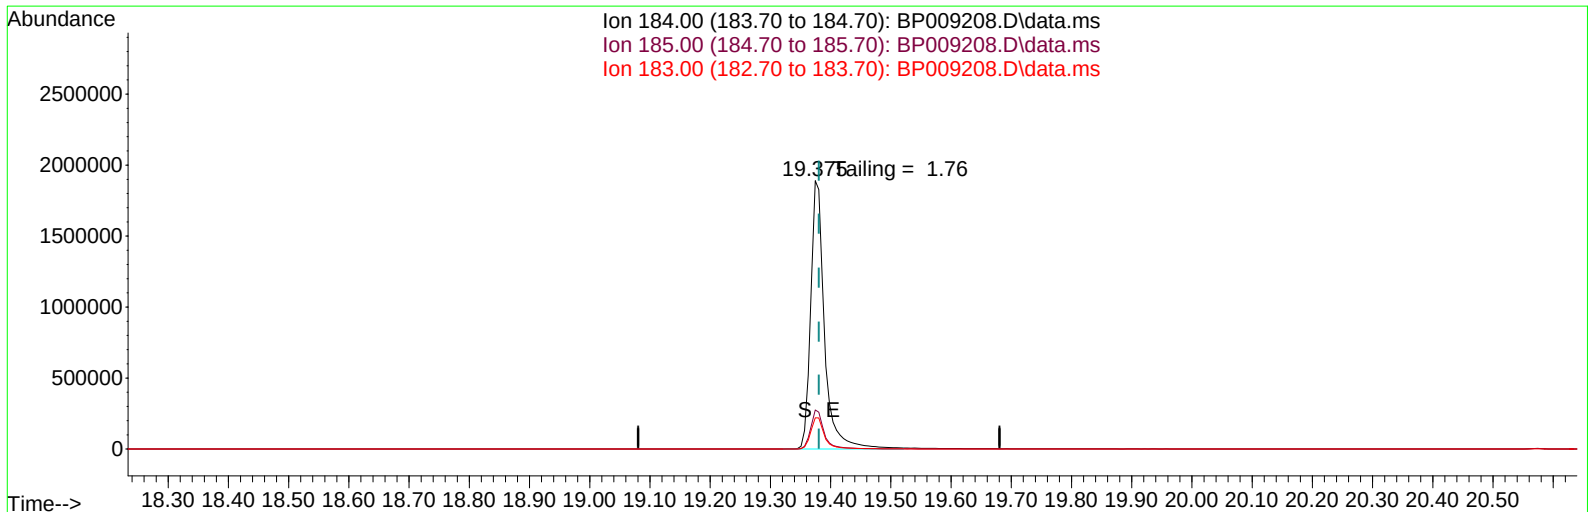

TIC: BP009208.D\data.ms

(77) Benzidine**19.375min (-0.006) 778894.48 ng****response 3059849**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.57
183.00	11.90	11.64
0.00	0.00	0.00