

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021822\
 Data File : BP009213.D
 Acq On : 18 Feb 2022 14:47
 Operator : CG/JU
 Sample : N1573-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GES-2R

Quant Time: Feb 19 00:48:58 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 19 00:46:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.763	152	158009	20.000	ng	0.00
21) Naphthalene-d8	10.557	136	605005	20.000	ng	0.00
39) Acenaphthene-d10	14.410	164	428308	20.000	ng	0.00
64) Phenanthrene-d10	17.175	188	986963	20.000	ng	0.00
76) Chrysene-d12	21.274	240	1209896	20.000	ng	0.00
86) Perylene-d12	23.657	264	1384030	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.364	112	661075	74.631	ng	0.00
7) Phenol-d6	6.969	99	509812	43.679	ng	0.00
23) Nitrobenzene-d5	8.928	82	1107351	103.218	ng	0.00
42) 2,4,6-Tribromophenol	15.916	330	1091792	190.917	ng	0.00
45) 2-Fluorobiphenyl	13.028	172	2960320	96.756	ng	0.00
79) Terphenyl-d14	19.739	244	5512639	81.937	ng	0.00
Target Compounds						
35) Caprolactam	11.587	113	6857	2.386	ng	Qvalue # 59
60) Diethylphthalate	15.239	149	102028	3.534	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021822\
Data File : BP009213.D
Acq On : 18 Feb 2022 14:47
Operator : CG/JU
Sample : N1573-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GES-2R

Quant Time: Feb 19 00:48:58 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 19 00:46:08 2022
Response via : Initial Calibration




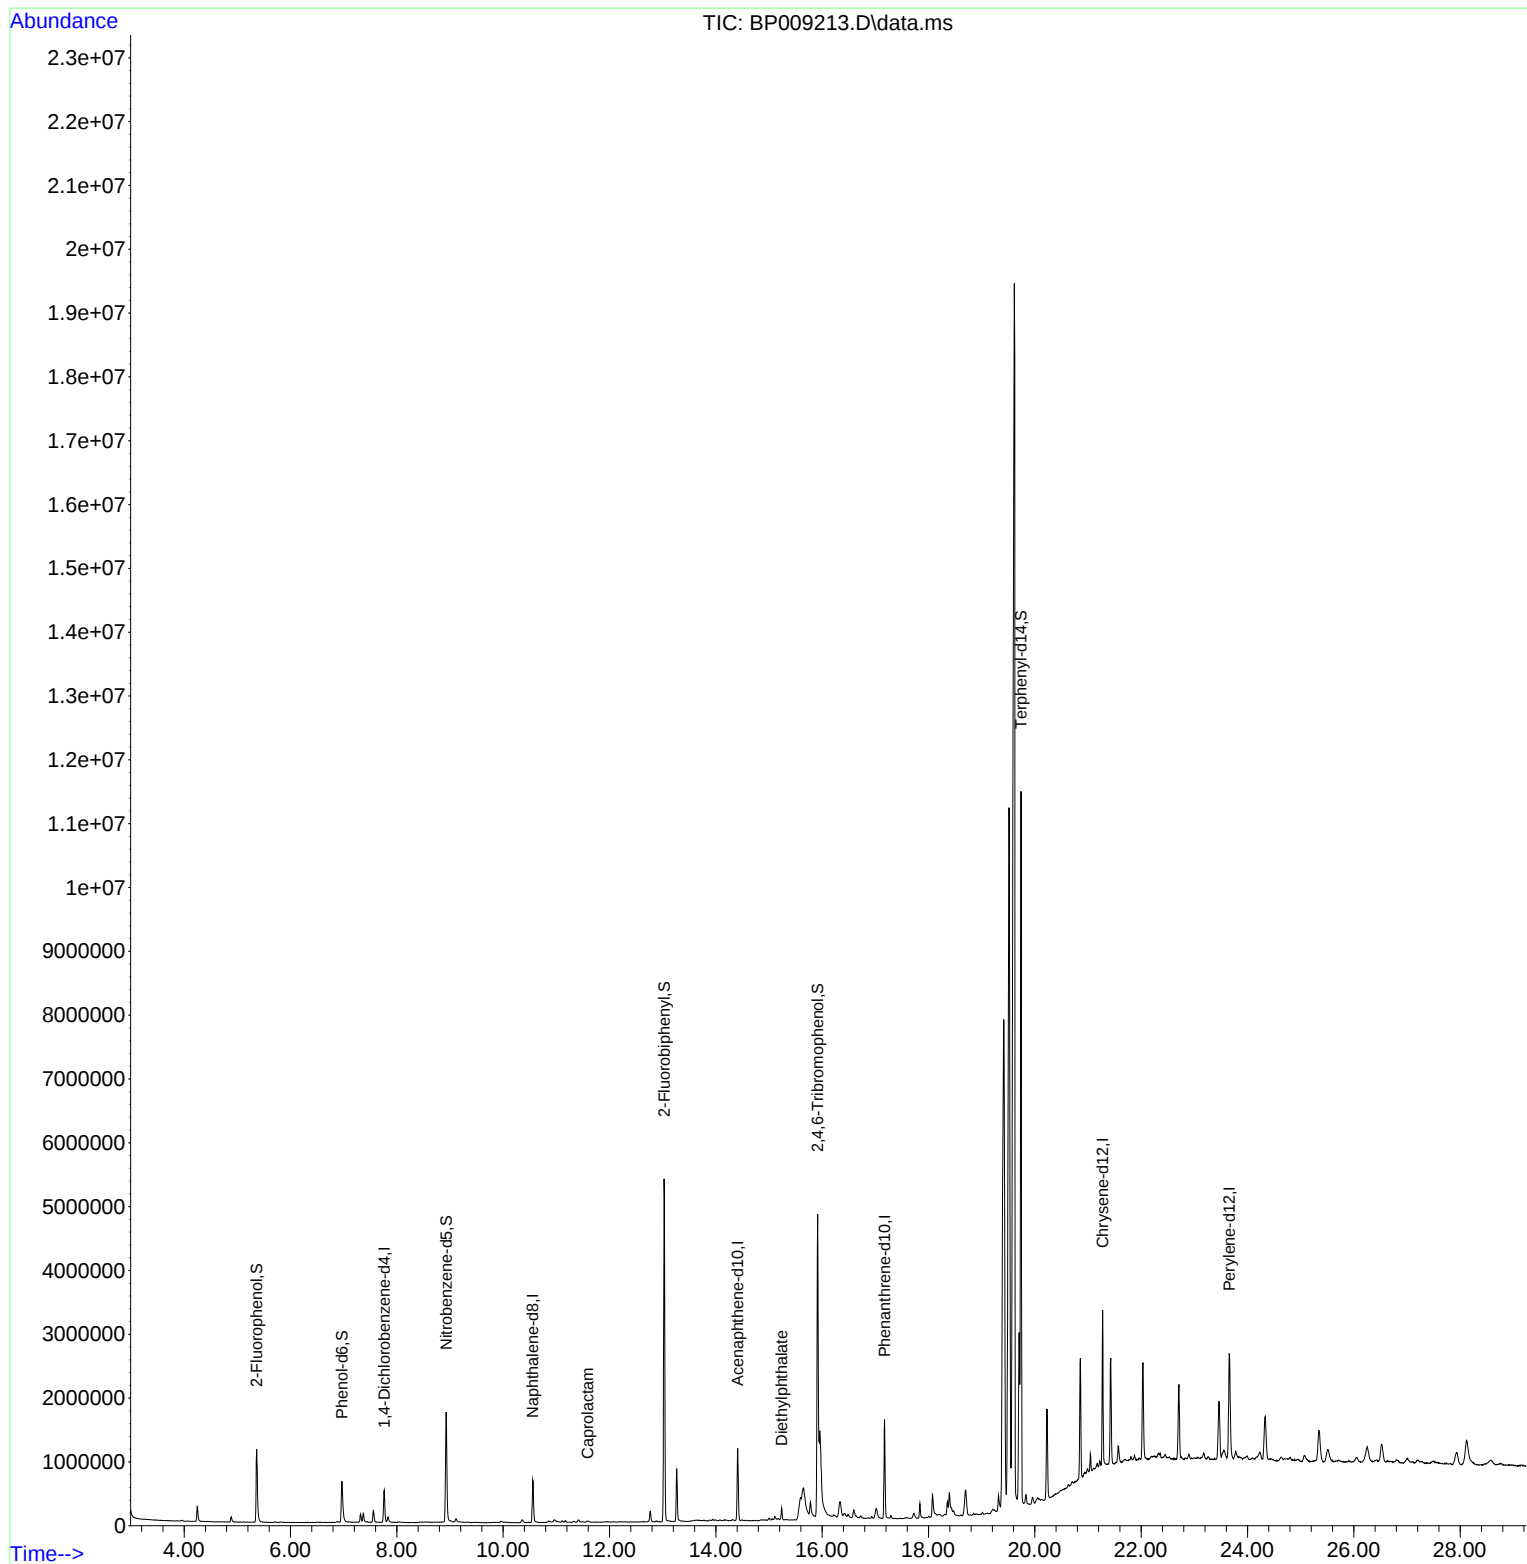


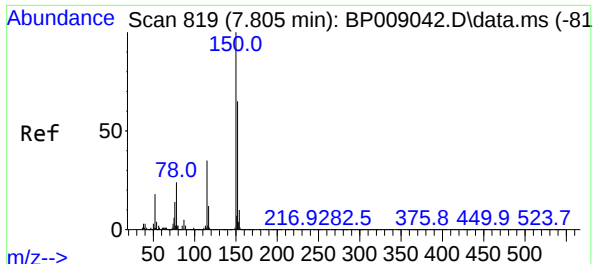

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.763 min Scan# 81
Delta R.T. -0.006 min
Lab File: BP009213.D
Acq: 18 Feb 2022 14:47




Instrument :
BNA_P
ClientSampleId :
GES-2R


Tgt Ion:152 Resp: 158009
Ion Ratio Lower Upper
152 100
150 147.9 127.0 190.6
115 52.6 43.7 65.5

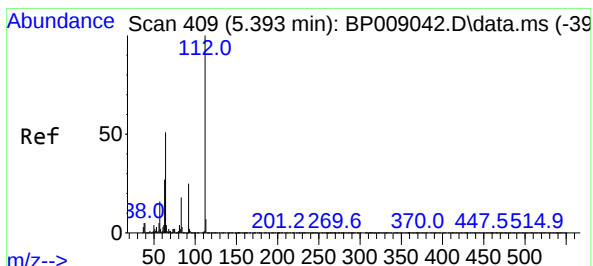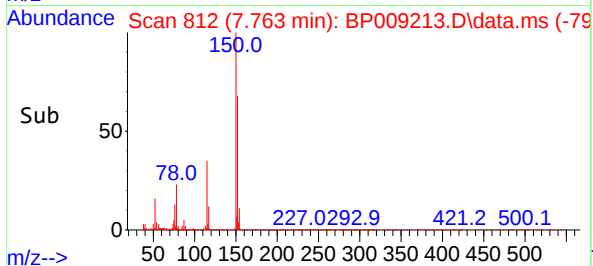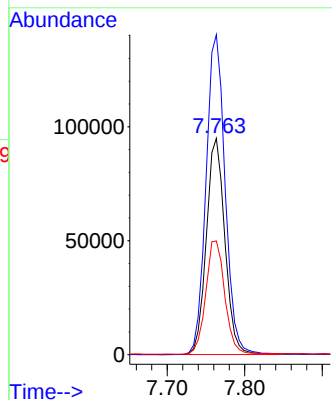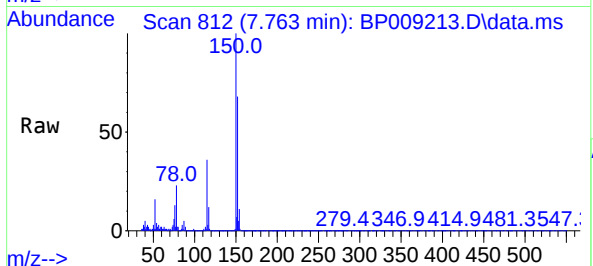

#5
2-Fluorophenol
Concen: 74.631 ng
RT: 5.364 min Scan# 404
Delta R.T. -0.000 min
Lab File: BP009213.D
Acq: 18 Feb 2022 14:47

Tgt Ion:112 Resp: 661075
Ion Ratio Lower Upper
112 100
64 52.4 39.7 59.5
63 26.8 20.0 30.0


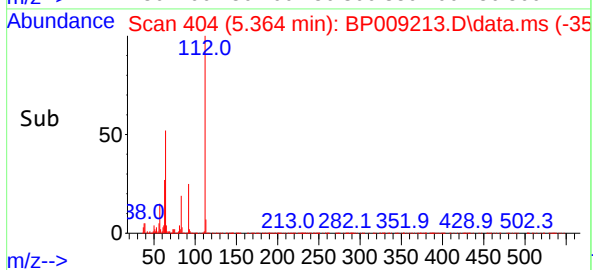
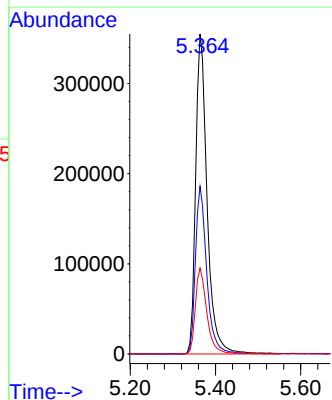
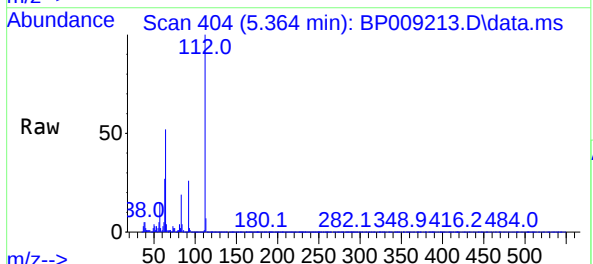


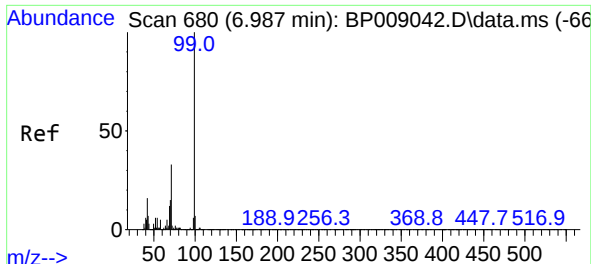

#7
Phenol-d6
Concen: 43.679 ng
RT: 6.969 min Scan# 61
Delta R.T. 0.006 min
Lab File: BP009213.D
Acq: 18 Feb 2022 14:47




Instrument :
BNA_P
ClientSampleId :
GES-2R


Tgt Ion: 99 Resp: 509812
Ion Ratio Lower Upper
99 100
42 14.8 10.8 16.2
71 31.2 23.8 35.6

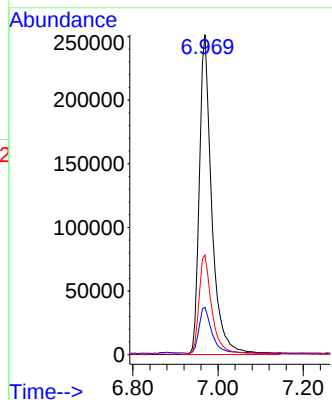

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.557 min Scan# 1287
Delta R.T. -0.006 min
Lab File: BP009213.D
Acq: 18 Feb 2022 14:47

Tgt Ion: 136 Resp: 605005
Ion Ratio Lower Upper
136 100
137 10.7 9.0 13.4
54 6.0 4.9 7.3
68 5.4 4.3 6.5

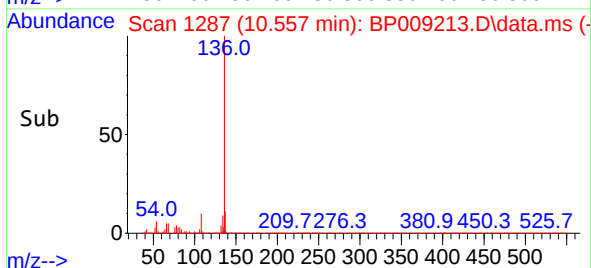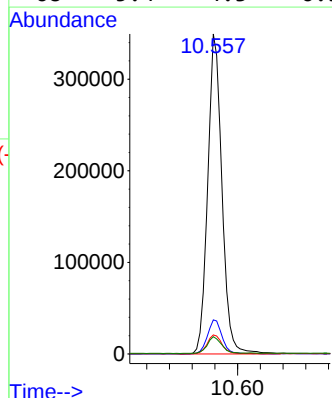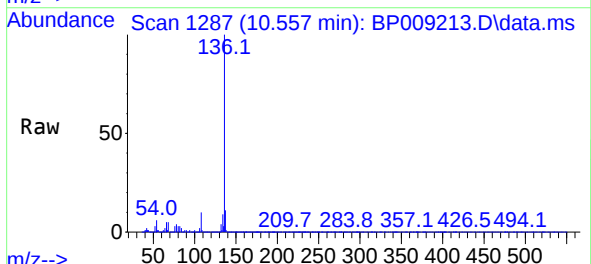

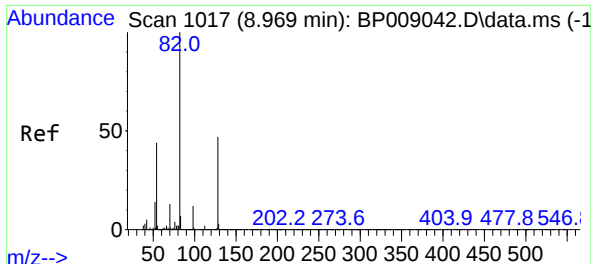

#23

Nitrobenzene-d5

Concen: 103.218 ng

RT: 8.928 min Scan# 1107

Delta R.T. -0.006 min

Lab File: BP009213.D

Acq: 18 Feb 2022 14:47

Instrument :

BNA_P

ClientSampleId :

GES-2R





Tgt Ion: 82 Resp: 1107351

Ion Ratio Lower Upper

82 100

128 46.6 39.4 59.2

54 41.8 32.6 48.8

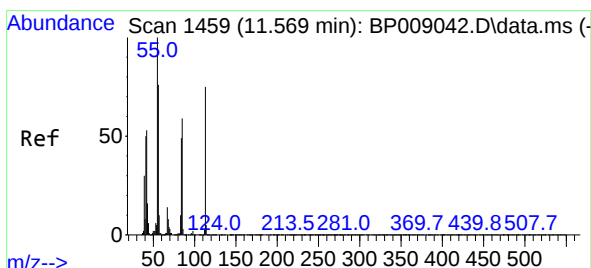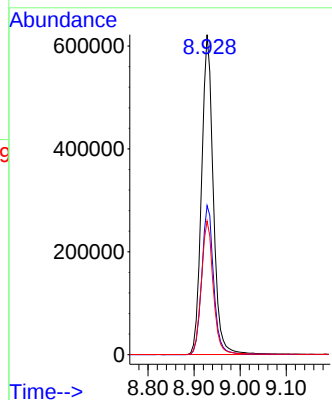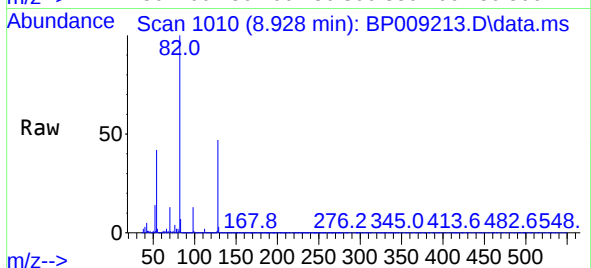

#35

Caprolactam

Concen: 2.386 ng

RT: 11.587 min Scan# 1462

Delta R.T. 0.023 min

Lab File: BP009213.D

Acq: 18 Feb 2022 14:47




Tgt Ion: 113 Resp: 6857


Ion Ratio Lower Upper

113 100

55 186.0 107.1 147.1#

56 120.3 74.1 114.1#


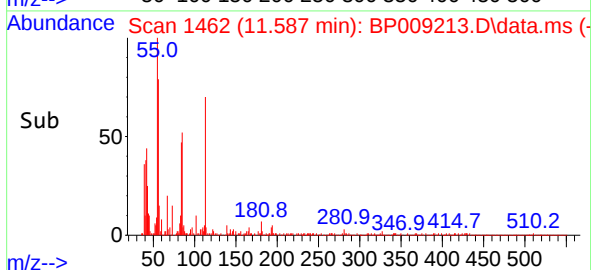
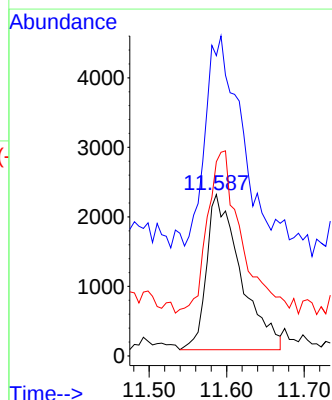





#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.410 min Scan# 1942
Delta R.T. -0.006 min
Lab File: BP009213.D
Acq: 18 Feb 2022 14:47




Instrument :
BNA_P
ClientSampleId :
GES-2R


Tgt Ion:164 Resp: 428308
Ion Ratio Lower Upper
164 100
162 98.8 79.9 119.9
160 43.0 35.5 53.3

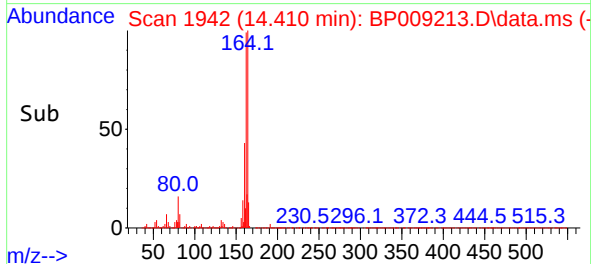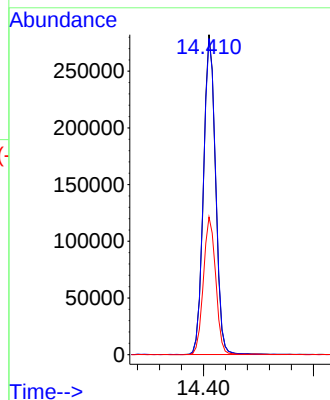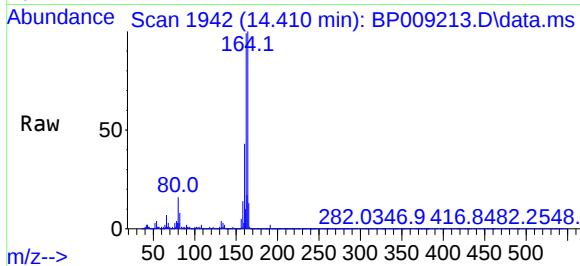

#42
2,4,6-Tribromophenol
Concen: 190.917 ng
RT: 15.916 min Scan# 2198
Delta R.T. -0.006 min
Lab File: BP009213.D
Acq: 18 Feb 2022 14:47

Tgt Ion:330 Resp: 1091792
Ion Ratio Lower Upper
330 100
332 96.3 77.0 115.4
141 26.5 21.3 31.9


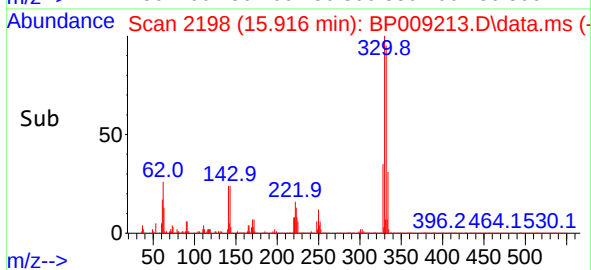
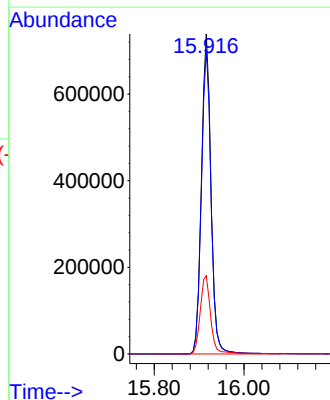
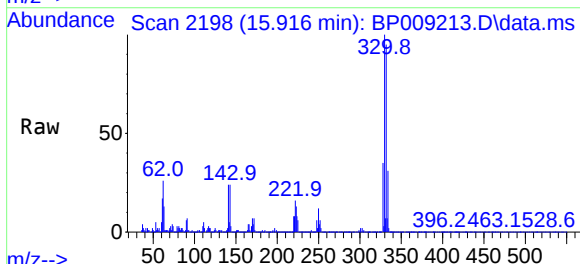




#45
2-Fluorobiphenyl
Concen: 96.756 ng
RT: 13.028 min Scan# 11
Delta R.T. -0.006 min
Lab File: BP009213.D
Acq: 18 Feb 2022 14:47




Instrument :
BNA_P
ClientSampleId :
GES-2R


Tgt Ion:172 Resp: 2960320
Ion Ratio Lower Upper
172 100
171 35.6 29.3 43.9
170 23.5 19.5 29.3

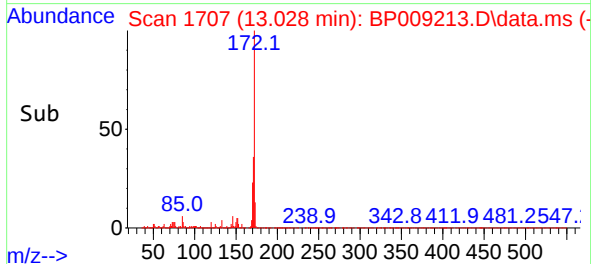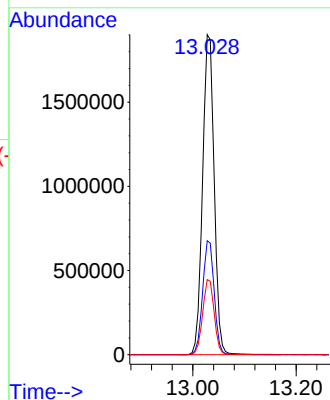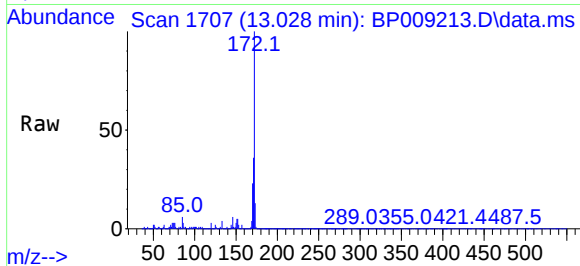

#60
Diethylphthalate
Concen: 3.534 ng
RT: 15.239 min Scan# 2083
Delta R.T. -0.006 min
Lab File: BP009213.D
Acq: 18 Feb 2022 14:47

Tgt Ion:149 Resp: 102028
Ion Ratio Lower Upper
149 100
177 25.4 19.9 29.9
150 12.5 10.3 15.5


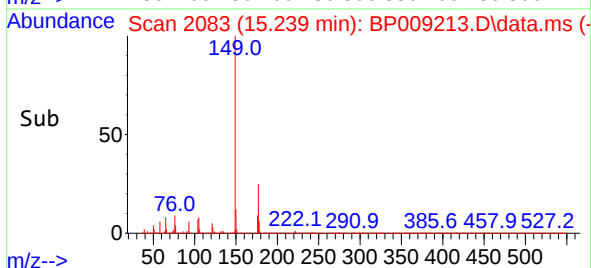
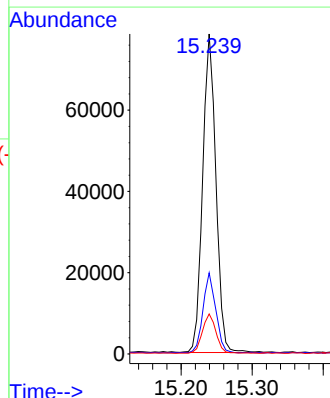
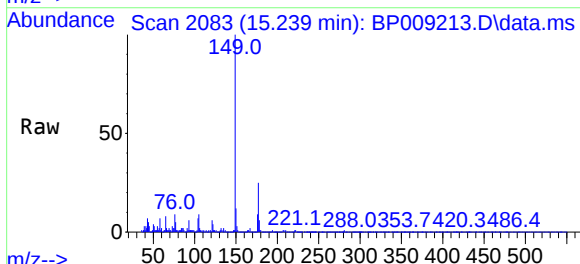




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.175 min Scan# 2417
Delta R.T. -0.000 min
Lab File: BP009213.D
Acq: 18 Feb 2022 14:47




Instrument :
BNA_P
ClientSampleId :
GES-2R


Tgt Ion:188 Resp: 986963
Ion Ratio Lower Upper
188 100
94 7.5 6.8 10.2
80 8.2 7.2 10.8

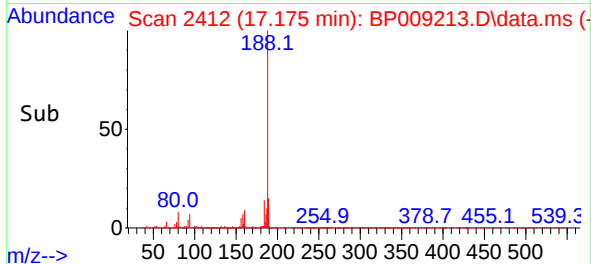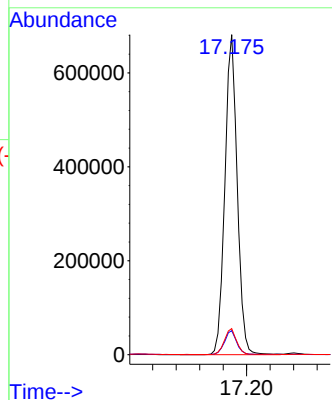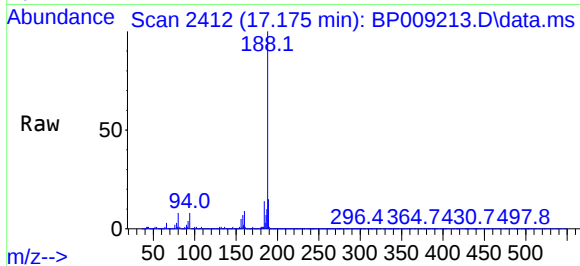

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.274 min Scan# 3109
Delta R.T. -0.006 min
Lab File: BP009213.D
Acq: 18 Feb 2022 14:47

Tgt Ion:240 Resp: 1209896
Ion Ratio Lower Upper
240 100
120 8.7 7.7 11.5
236 26.4 21.2 31.8


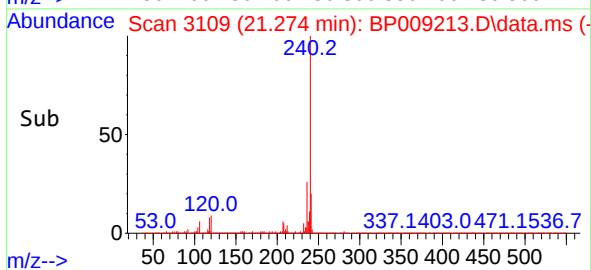
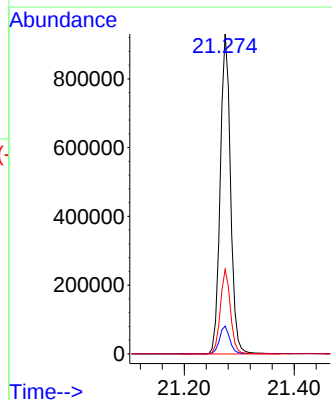
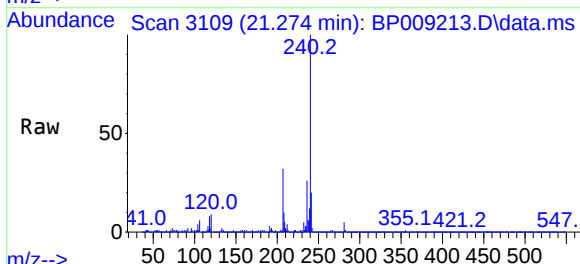


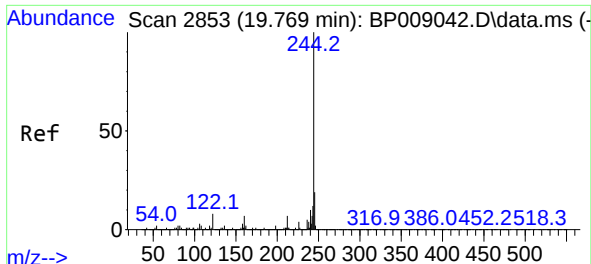

#79
 Terphenyl-d14
 Concen: 81.937 ng
 RT: 19.739 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BP009213.D
 Acq: 18 Feb 2022 14:47

Instrument :
 BNA_P
 ClientSampleId :
 GES-2R

Tgt Ion:244 Resp: 5512639
 Ion Ratio Lower Upper
 244 100
 212 7.5 6.5 9.7
 122 8.6 9.2 13.8#

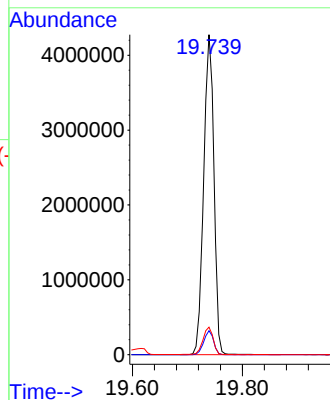

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.657 min Scan# 3514
 Delta R.T. -0.006 min
 Lab File: BP009213.D
 Acq: 18 Feb 2022 14:47

Tgt Ion:264 Resp: 1384030
 Ion Ratio Lower Upper
 264 100
 260 24.3 19.1 28.7
 265 22.8 17.1 25.7

