

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021822\
 Data File : BP009227.D
 Acq On : 18 Feb 2022 22:37
 Operator : CG/JU
 Sample : N1466-10DL 10X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A5-10-4.0DL

Quant Time: Feb 19 00:51:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 19 00:46:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.763	152	257117	20.000	ng	0.00
21) Naphthalene-d8	10.557	136	1038280	20.000	ng	0.00
39) Acenaphthene-d10	14.410	164	734536	20.000	ng	0.00
64) Phenanthrene-d10	17.169	188	1585017	20.000	ng	0.00
76) Chrysene-d12	21.275	240	1716631	20.000	ng	0.00
86) Perylene-d12	23.657	264	1522099	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.375	112	88774	6.159	ng	0.01
7) Phenol-d6	6.981	99	123925	6.525	ng	0.02
23) Nitrobenzene-d5	8.940	82	90360	4.908	ng	0.00
42) 2,4,6-Tribromophenol	15.928	330	50684	5.168	ng	0.00
45) 2-Fluorobiphenyl	13.028	172	283393	5.401	ng	0.00
79) Terphenyl-d14	19.739	244	488552	5.118	ng	0.00
Target Compounds						
						Qvalue
31) Naphthalene	10.610	128	2404845	45.412	ng	98
37) 2-Methylnaphthalene	12.228	142	2512489	67.046	ng	98
38) 1-Methylnaphthalene	12.446	142	1274000	34.792	ng	99
46) 1,1'-Biphenyl	13.240	154	173977	3.224	ng	97
58) Fluorene	15.463	166	137866	2.708	ng	# 87
71) Phenanthrene	17.216	178	409727	4.774	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021822\
Data File : BP009227.D
Acq On : 18 Feb 2022 22:37
Operator : CG/JU
Sample : N1466-10DL 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A5-10-4.0DL

Quant Time: Feb 19 00:51:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 19 00:46:08 2022
Response via : Initial Calibration




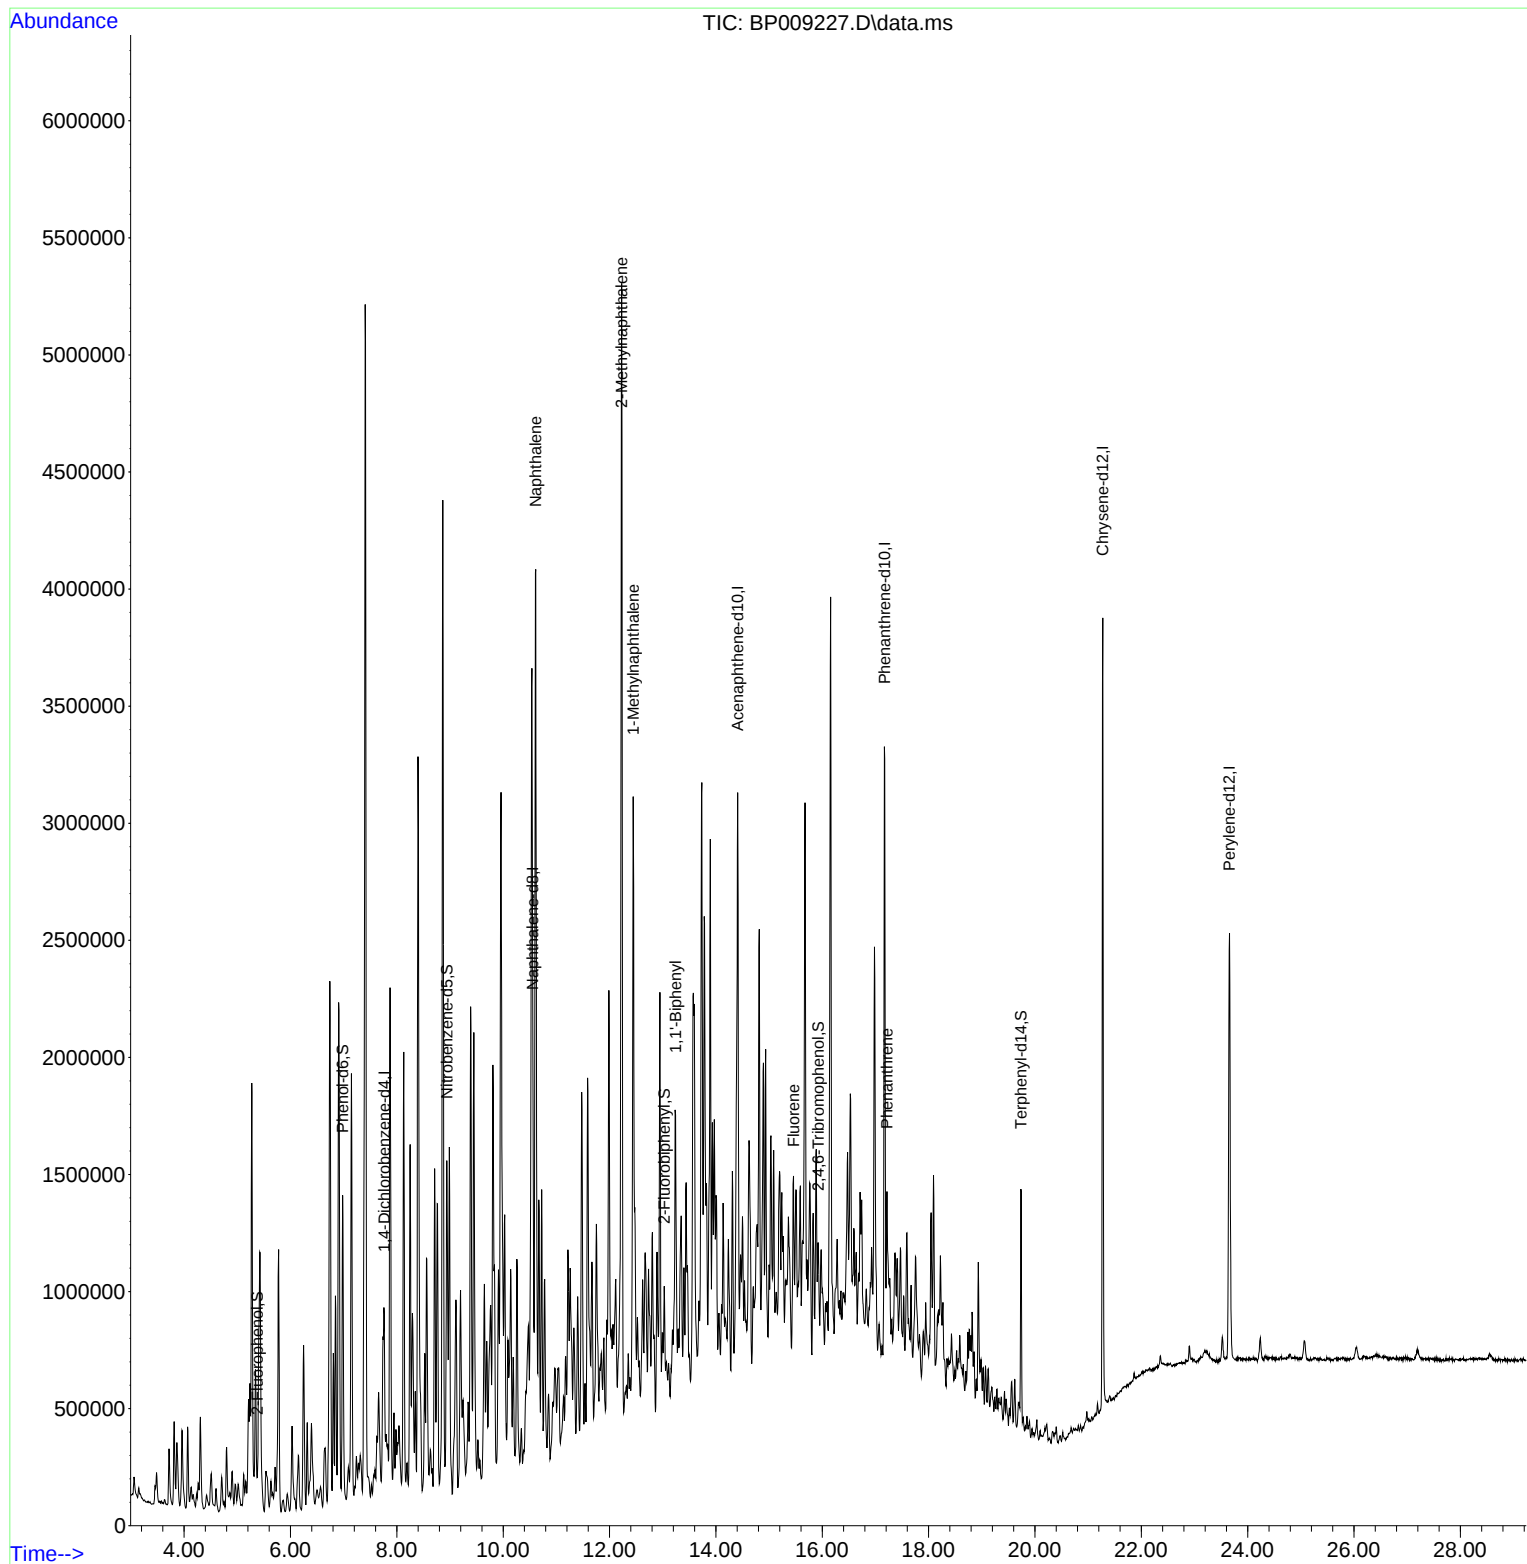




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.763 min Scan# 81
Delta R.T. -0.006 min
Lab File: BP009227.D
Acq: 18 Feb 2022 22:37




Instrument :
BNA_P
ClientSampleId :
A5-10-4.0DL


Tgt Ion:152 Resp: 257117
Ion Ratio Lower Upper
152 100
150 153.7 127.0 190.6
115 54.6 43.7 65.5

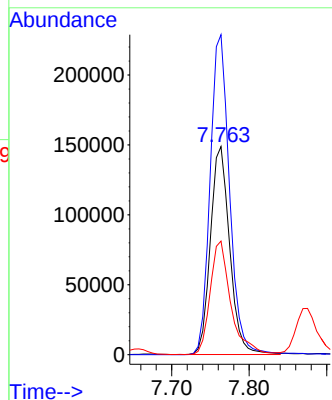

#5
2-Fluorophenol
Concen: 6.159 ng
RT: 5.375 min Scan# 406
Delta R.T. 0.012 min
Lab File: BP009227.D
Acq: 18 Feb 2022 22:37

Tgt Ion:112 Resp: 88774
Ion Ratio Lower Upper
112 100
64 48.2 39.7 59.5
63 27.7 20.0 30.0


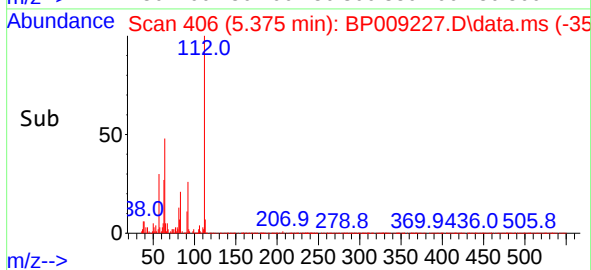
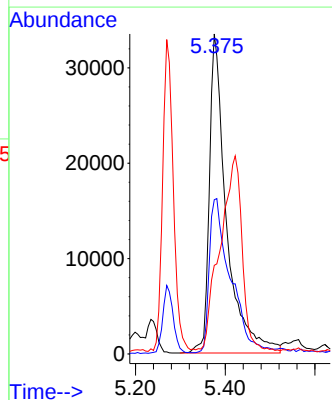





#7
Phenol-d6
Concen: 6.525 ng
RT: 6.981 min Scan# 61
Delta R.T. 0.018 min
Lab File: BP009227.D
Acq: 18 Feb 2022 22:37




Instrument :
BNA_P
ClientSampleId :
A5-10-4.0DL


Tgt Ion: 99 Resp: 123925
Ion Ratio Lower Upper
99 100
42 20.7 10.8 16.2#
71 42.4 23.8 35.6#

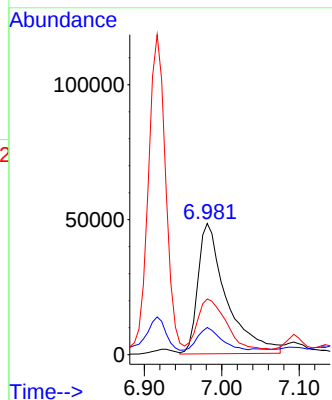

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.557 min Scan# 1287
Delta R.T. -0.006 min
Lab File: BP009227.D
Acq: 18 Feb 2022 22:37

Tgt Ion: 136 Resp: 1038280
Ion Ratio Lower Upper
136 100
137 11.0 9.0 13.4
54 6.9 4.9 7.3
68 6.3 4.3 6.5


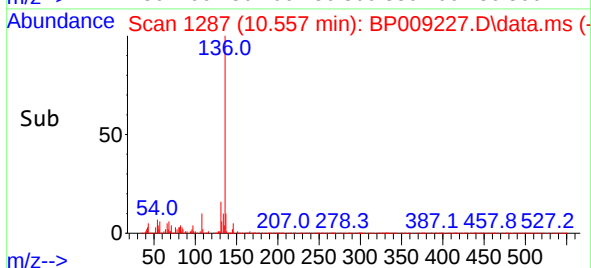
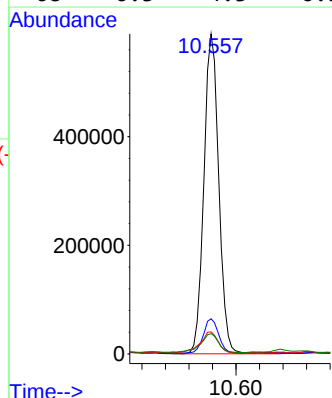





#23
Nitrobenzene-d5
Concen: 4.908 ng
RT: 8.940 min Scan# 1017
Delta R.T. 0.006 min
Lab File: BP009227.D
Acq: 18 Feb 2022 22:37




Instrument :
BNA_P
ClientSampleId :
A5-10-4.0DL


Tgt Ion: 82 Resp: 90360
Ion Ratio Lower Upper
82 100
128 83.4 39.4 59.2#
54 43.1 32.6 48.8

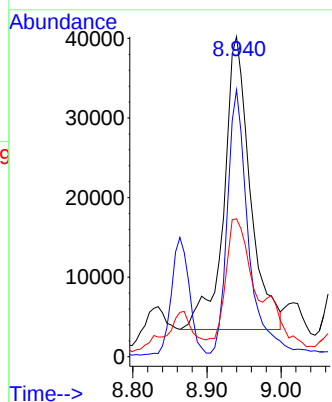

#31
Naphthalene
Concen: 45.412 ng
RT: 10.610 min Scan# 1296
Delta R.T. -0.000 min
Lab File: BP009227.D
Acq: 18 Feb 2022 22:37

Tgt Ion: 128 Resp: 2404845
Ion Ratio Lower Upper
128 100
129 12.1 8.8 13.2
127 13.5 10.4 15.6


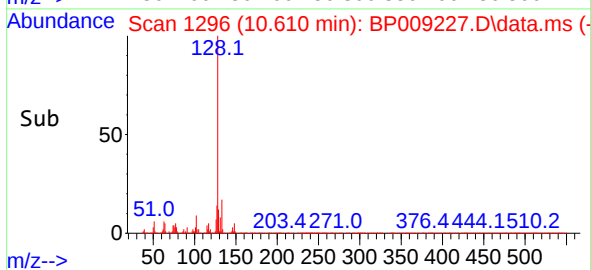
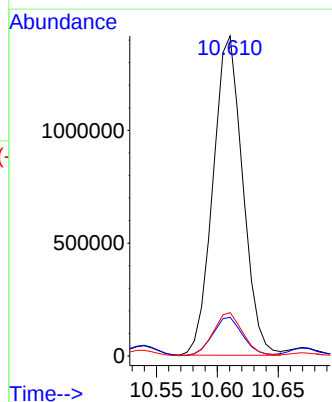





#37
2-Methylnaphthalene
Concen: 67.046 ng
RT: 12.228 min Scan# 1
Delta R.T. -0.006 min
Lab File: BP009227.D
Acq: 18 Feb 2022 22:37




Instrument :
BNA_P
ClientSampleId :
A5-10-4.0DL


Tgt Ion:142 Resp: 2512489
Ion Ratio Lower Upper
142 100
141 89.5 70.5 105.7
115 33.4 24.6 36.8

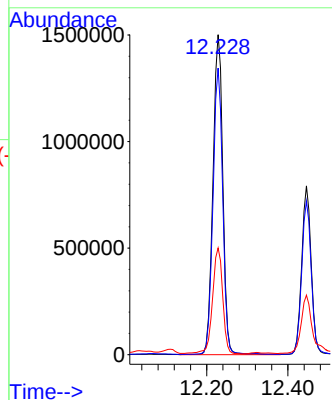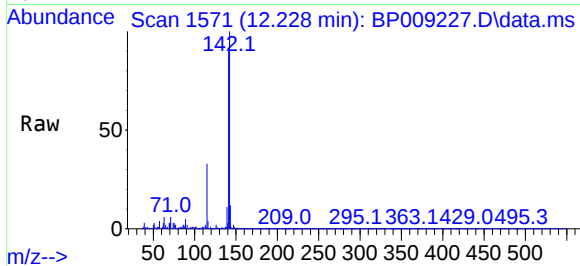

#38
1-Methylnaphthalene
Concen: 34.792 ng
RT: 12.446 min Scan# 1608
Delta R.T. -0.006 min
Lab File: BP009227.D
Acq: 18 Feb 2022 22:37

Tgt Ion:142 Resp: 1274000
Ion Ratio Lower Upper
142 100
141 91.0 73.2 109.8
116 3.8 2.7 4.1


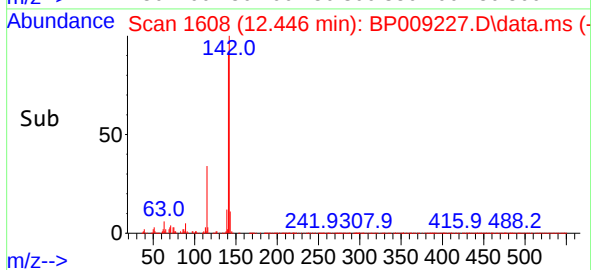
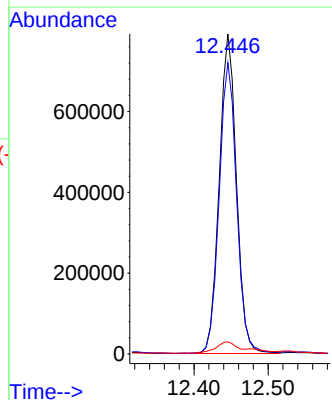
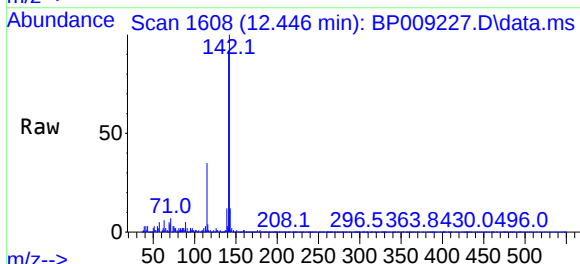




#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.410 min Scan# 1942
Delta R.T. -0.006 min
Lab File: BP009227.D
Acq: 18 Feb 2022 22:37




Instrument :
BNA_P
ClientSampleId :
A5-10-4.0DL


Tgt Ion:164 Resp: 734536
Ion Ratio Lower Upper
164 100
162 101.0 79.9 119.9
160 44.8 35.5 53.3

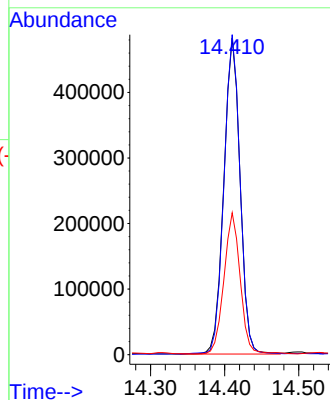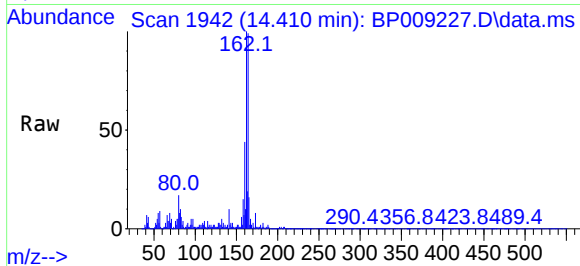

#42
2,4,6-Tribromophenol
Concen: 5.168 ng
RT: 15.928 min Scan# 2200
Delta R.T. 0.006 min
Lab File: BP009227.D
Acq: 18 Feb 2022 22:37

Tgt Ion:330 Resp: 50684
Ion Ratio Lower Upper
330 100
332 96.5 77.0 115.4
141 27.3 21.3 31.9


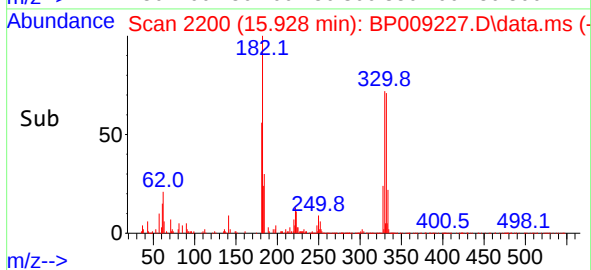
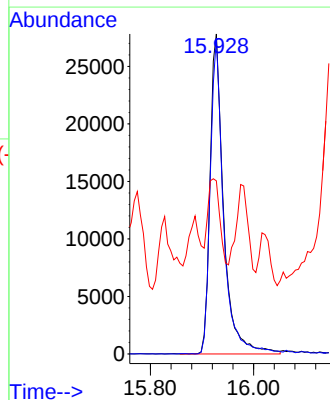
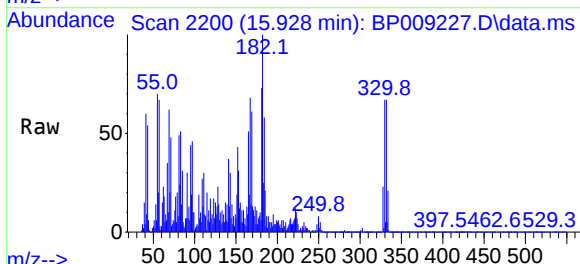




#45
2-Fluorobiphenyl
Concen: 5.401 ng
RT: 13.028 min Scan# 1714
Delta R.T. -0.006 min
Lab File: BP009227.D
Acq: 18 Feb 2022 22:37




Instrument :
BNA_P
ClientSampleId :
A5-10-4.0DL


Tgt Ion:172 Resp: 283393
Ion Ratio Lower Upper
172 100
171 34.8 29.3 43.9
170 23.5 19.5 29.3

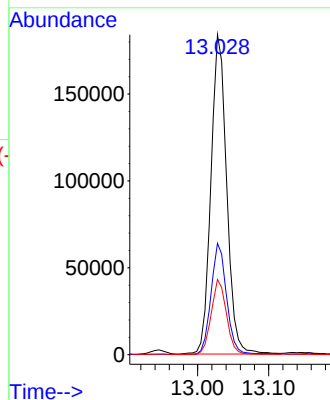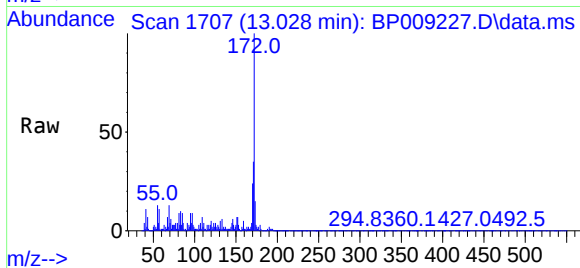

#46
1,1'-Biphenyl
Concen: 3.224 ng
RT: 13.240 min Scan# 1743
Delta R.T. -0.006 min
Lab File: BP009227.D
Acq: 18 Feb 2022 22:37

Tgt Ion:154 Resp: 173977
Ion Ratio Lower Upper
154 100
153 38.5 20.3 60.3
76 11.9 0.0 31.1


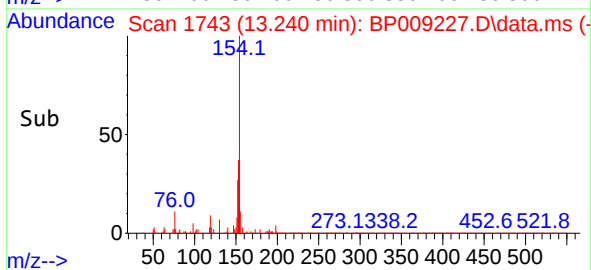
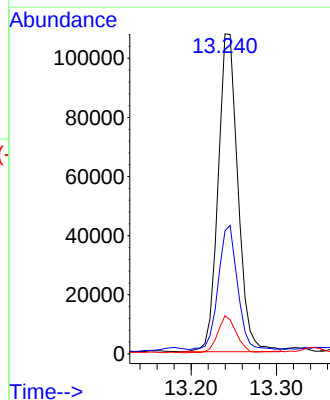
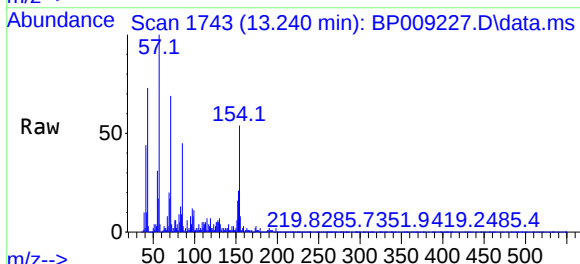




#58
Fluorene
Concen: 2.708 ng
RT: 15.463 min Scan# 2127
Delta R.T. -0.006 min
Lab File: BP009227.D
Acq: 18 Feb 2022 22:37




Instrument :
BNA_P
ClientSampleId :
A5-10-4.0DL


Tgt Ion:166 Resp: 137866
Ion Ratio Lower Upper
166 100
165 103.8 77.2 115.8
167 34.7 11.2 16.8#

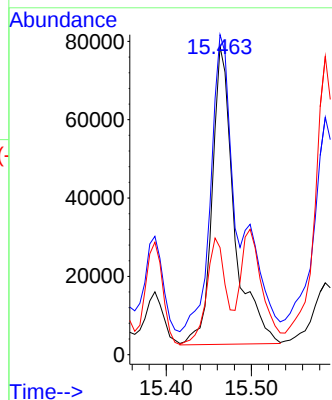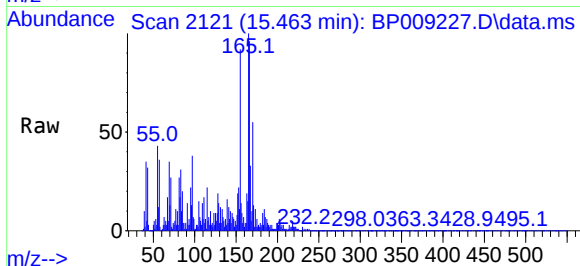

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.169 min Scan# 2411
Delta R.T. -0.006 min
Lab File: BP009227.D
Acq: 18 Feb 2022 22:37

Tgt Ion:188 Resp: 1585017
Ion Ratio Lower Upper
188 100
94 7.9 6.8 10.2
80 8.2 7.2 10.8


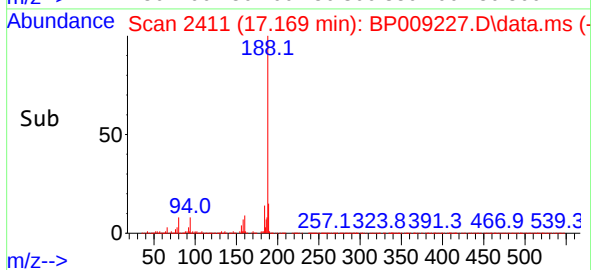
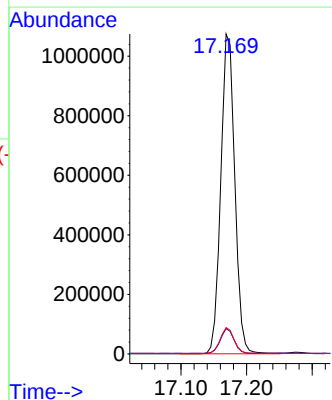
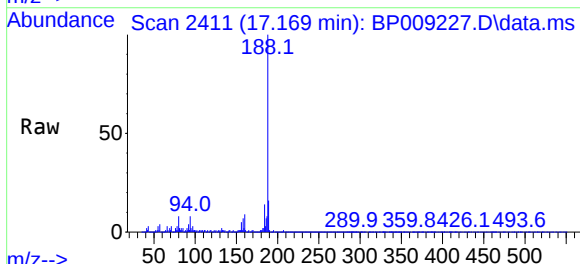




#71
Phenanthrene
Concen: 4.774 ng
RT: 17.216 min Scan# 2419
Delta R.T. -0.006 min
Lab File: BP009227.D
Acq: 18 Feb 2022 22:37




Instrument :
BNA_P
ClientSampleId :
A5-10-4.0DL


Tgt Ion:178 Resp: 409727
Ion Ratio Lower Upper
178 100
176 19.6 16.0 24.0
179 18.2 13.0 19.4

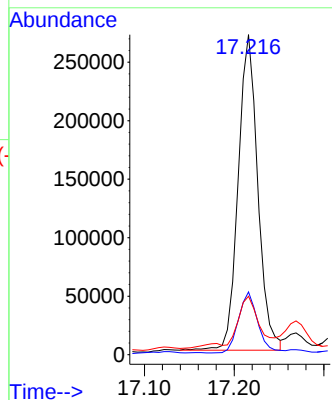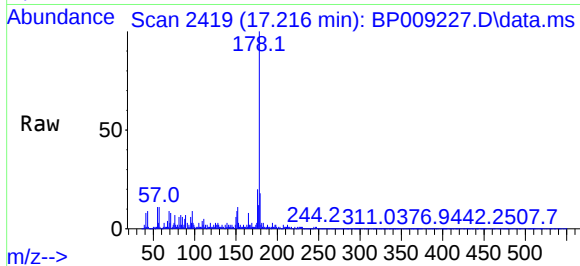

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.275 min Scan# 3109
Delta R.T. -0.006 min
Lab File: BP009227.D
Acq: 18 Feb 2022 22:37

Tgt Ion:240 Resp: 1716631
Ion Ratio Lower Upper
240 100
120 8.4 7.7 11.5
236 26.7 21.2 31.8


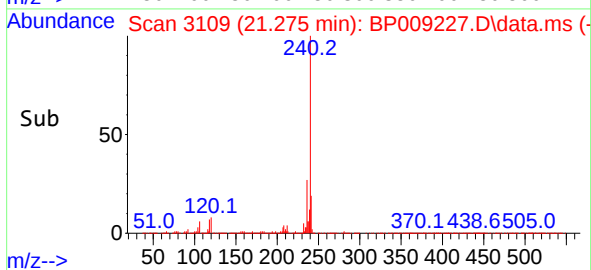
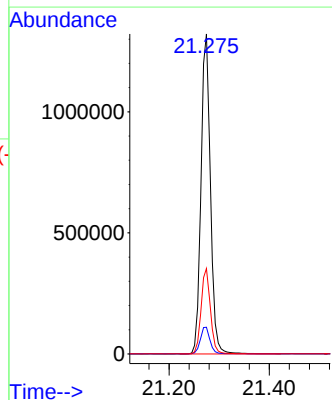
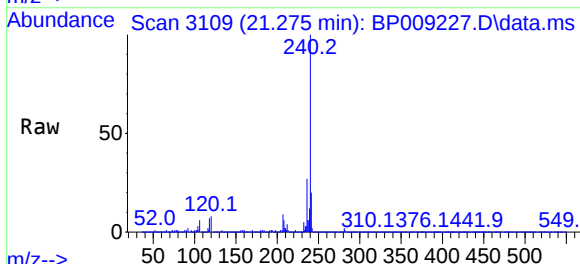




#79
 Terphenyl-d14
 Concen: 5.118 ng
 RT: 19.739 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BP009227.D
 Acq: 18 Feb 2022 22:37

Instrument :
 BNA_P
 ClientSampleId :
 A5-10-4.0DL

Tgt Ion:244 Resp: 488552
 Ion Ratio Lower Upper
 244 100
 212 6.7 6.5 9.7
 122 8.3 9.2 13.8#

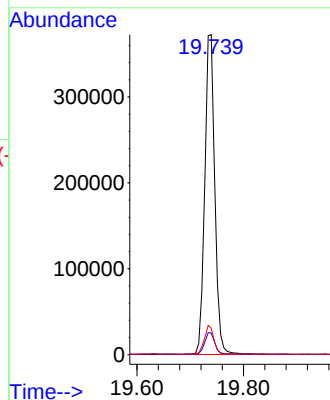

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.657 min Scan# 3514
 Delta R.T. -0.006 min
 Lab File: BP009227.D
 Acq: 18 Feb 2022 22:37

Tgt Ion:264 Resp: 1522099
 Ion Ratio Lower Upper
 264 100
 260 24.8 19.1 28.7
 265 22.1 17.1 25.7

