

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021822\
 Data File : BP009210.D
 Acq On : 18 Feb 2022 12:58
 Operator : CG/JU
 Sample : PB142739BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB142739BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009210.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.363	398	404	425	rBV	2468755	4417291	32.58%	8.310%
2	6.963	669	676	712	rBV	2216241	4598348	33.92%	8.651%
3	7.763	805	812	830	rBV	535673	983777	7.26%	1.851%
4	8.934	1003	1011	1033	rBV	1415124	2921117	21.55%	5.495%
5	10.569	1281	1289	1314	rBV	564394	1349442	9.95%	2.539%
6	13.034	1699	1708	1735	rBV	4911202	8321664	61.38%	15.655%
7	14.416	1934	1943	1967	rBV	1129742	2085793	15.38%	3.924%
8	15.916	2191	2198	2229	rBV	3576380	6525131	48.13%	12.276%
9	17.180	2406	2413	2434	rBV	1417487	2630938	19.41%	4.950%
10	19.739	2842	2848	2861	rBV	10371318	13557762	100.00%	25.506%
11	21.280	3105	3110	3122	rBV	1935809	2946110	21.73%	5.542%
12	23.668	3509	3516	3533	rVB2	1123339	2817789	20.78%	5.301%




Sum of corrected areas: 53155162

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021822\
Data File : BP009210.D
Acq On : 18 Feb 2022 12:58
Operator : CG/JU
Sample : PB142739BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142739BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

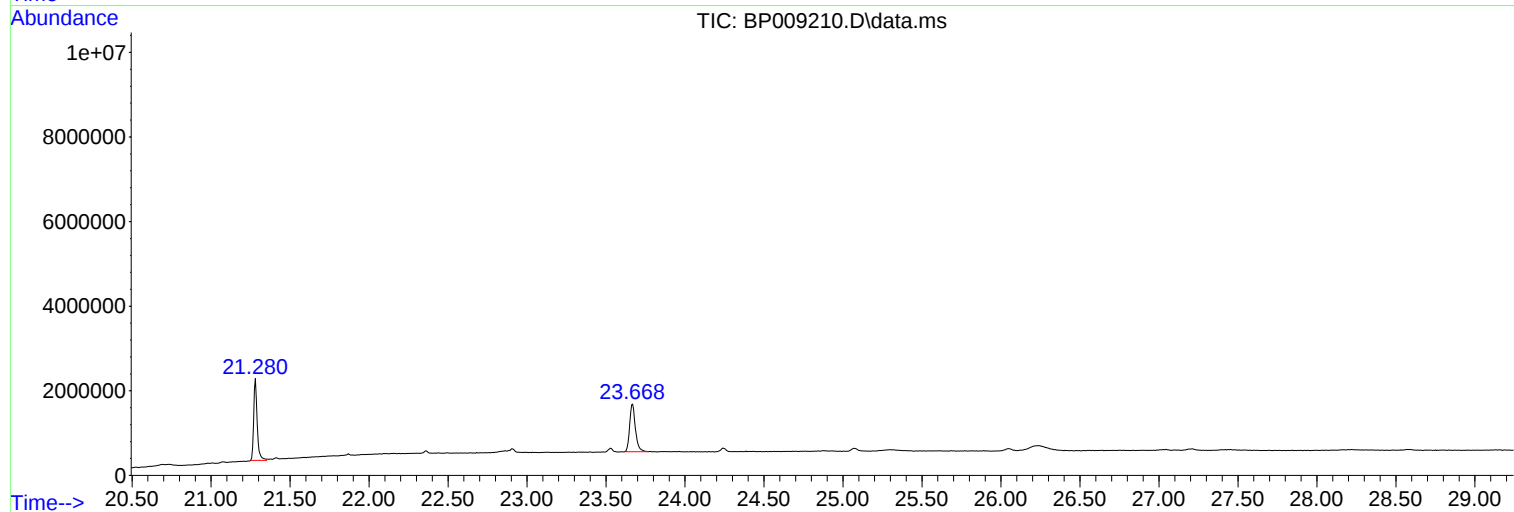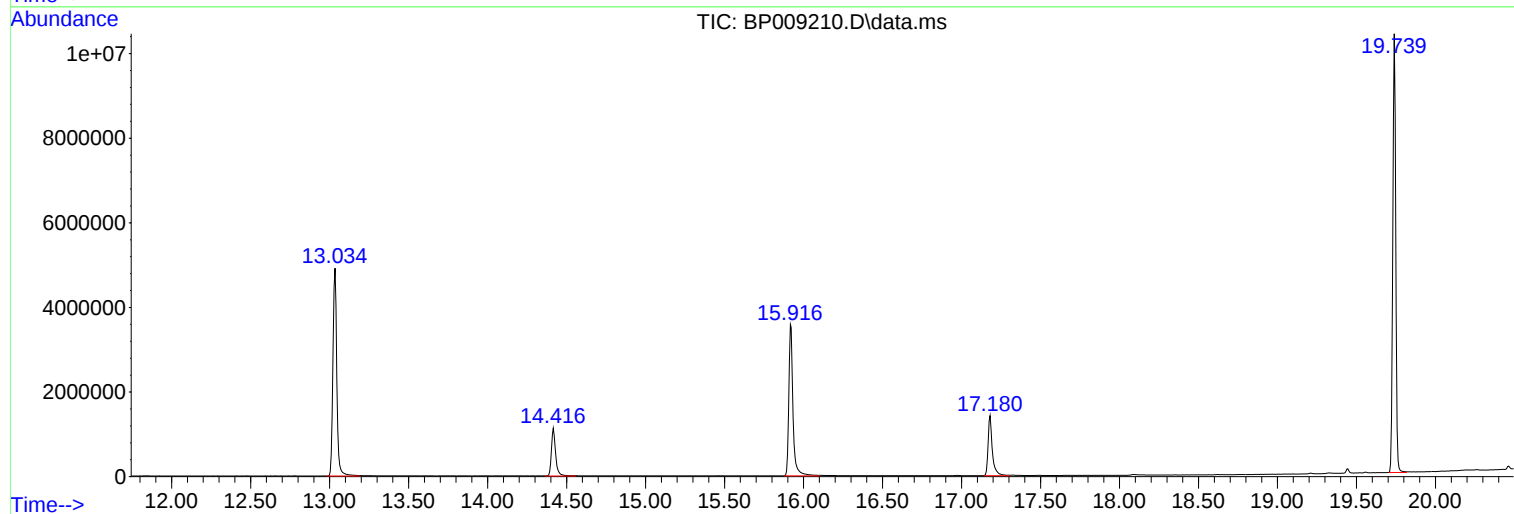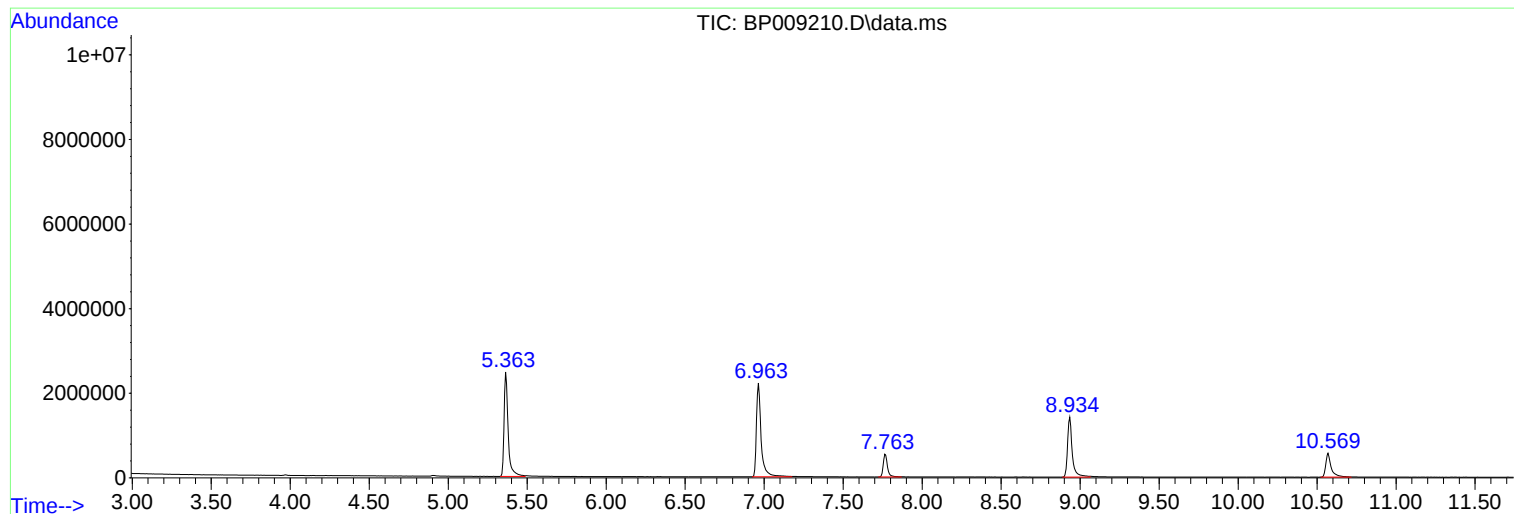

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021822\
Data File : BP009210.D
Acq On : 18 Feb 2022 12:58
Operator : CG/JU
Sample : PB142739BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142739BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021822\
Data File : BP009210.D
Acq On : 18 Feb 2022 12:58
Operator : CG/JU
Sample : PB142739BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142739BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------