

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP021822\  
 Data File : BP009219.D  
 Acq On : 18 Feb 2022 18:09  
 Operator : CG/JU  
 Sample : N1587-01  
 Misc :  
 ALS Vial : 12 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 FIELD-BLANK

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP020722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009219.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.364       | 398           | 404         | 431          | rBV      | 972453         | 2036314       | 12.32%          | 3.910%        |
| 2         | 6.969       | 671           | 677         | 711          | rBV      | 472932         | 1331445       | 8.05%           | 2.557%        |
| 3         | 7.764       | 805           | 812         | 825          | rBV      | 433325         | 841149        | 5.09%           | 1.615%        |
| 4         | 8.928       | 1003          | 1010        | 1044         | rBV      | 1377410        | 3031220       | 18.34%          | 5.821%        |
| 5         | 10.563      | 1280          | 1288        | 1314         | rBV      | 485178         | 1194041       | 7.22%           | 2.293%        |
| 6         | 13.028      | 1700          | 1707        | 1735         | rBV      | 5168231        | 8549539       | 51.72%          | 16.418%       |
| 7         | 14.410      | 1935          | 1942        | 1956         | rVB      | 1030211        | 1824639       | 11.04%          | 3.504%        |
| 8         | 15.916      | 2191          | 2198        | 2223         | rBV      | 4006963        | 7296718       | 44.14%          | 14.012%       |
| 9         | 17.175      | 2406          | 2412        | 2431         | rBV      | 1349863        | 2459149       | 14.88%          | 4.722%        |
| 10        | 19.739      | 2842          | 2848        | 2864         | rBV      | 12498691       | 16531794      | 100.00%         | 31.747%       |
| 11        | 21.275      | 3104          | 3109        | 3124         | rBV      | 2191544        | 3382055       | 20.46%          | 6.495%        |
| 12        | 23.663      | 3508          | 3515        | 3529         | rVB2     | 1510223        | 3596144       | 21.75%          | 6.906%        |




Sum of corrected areas: 52074207

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP021822\  
Data File : BP009219.D  
Acq On : 18 Feb 2022 18:09  
Operator : CG/JU  
Sample : N1587-01  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
FIELD-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP020722.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

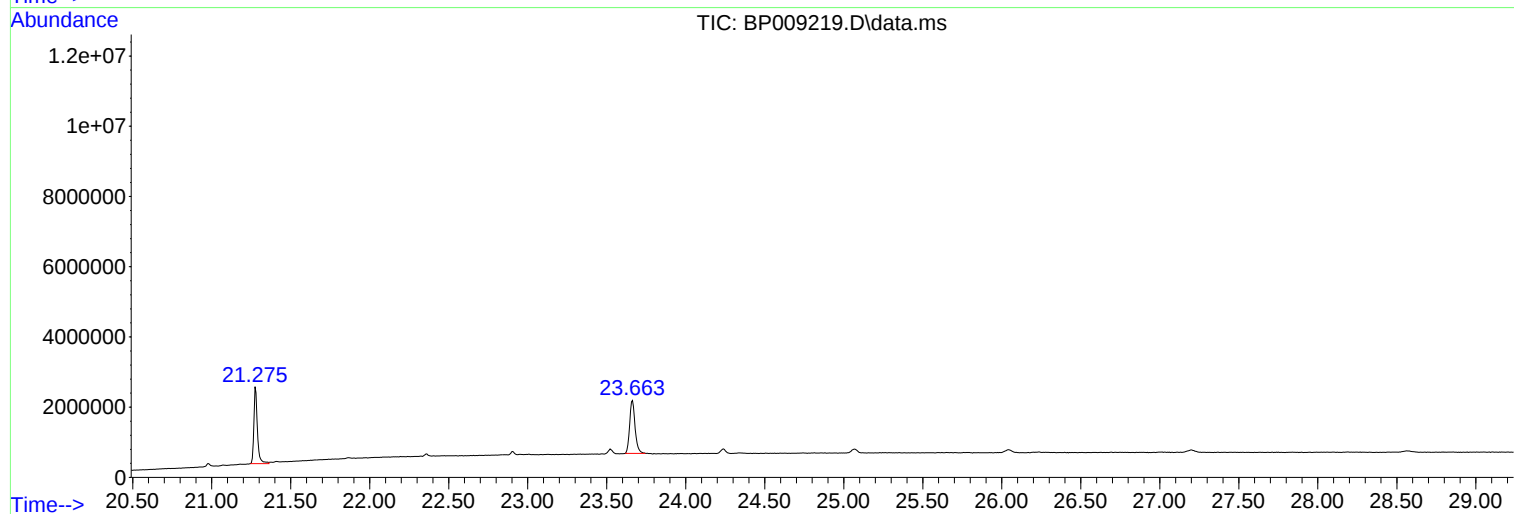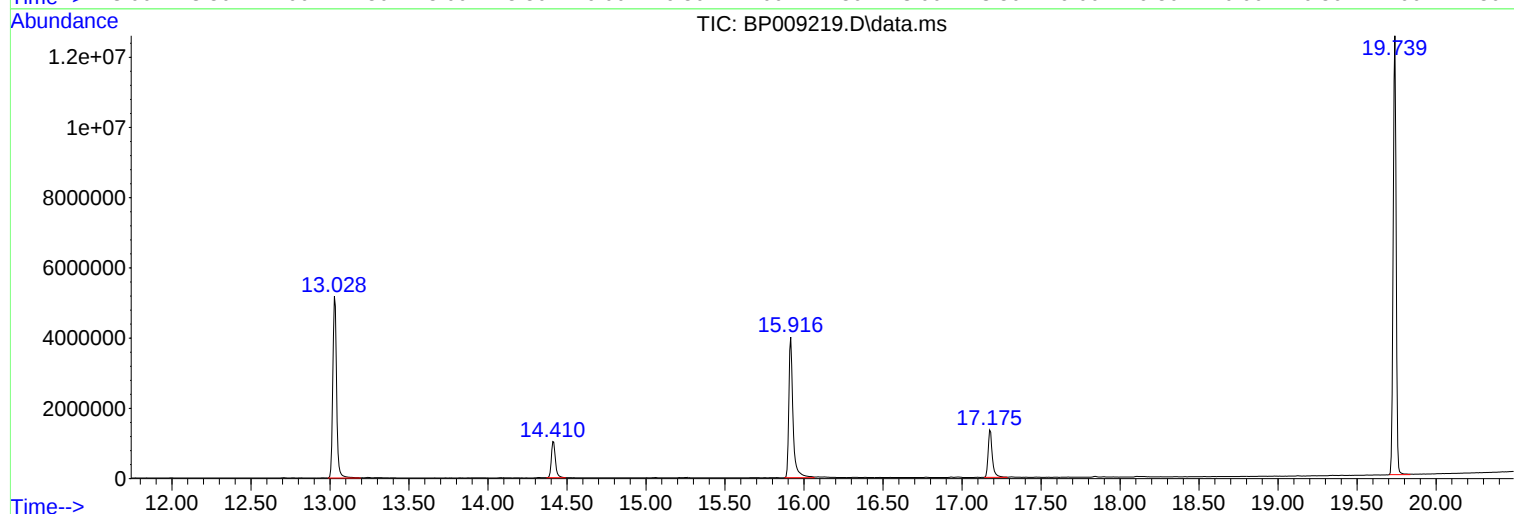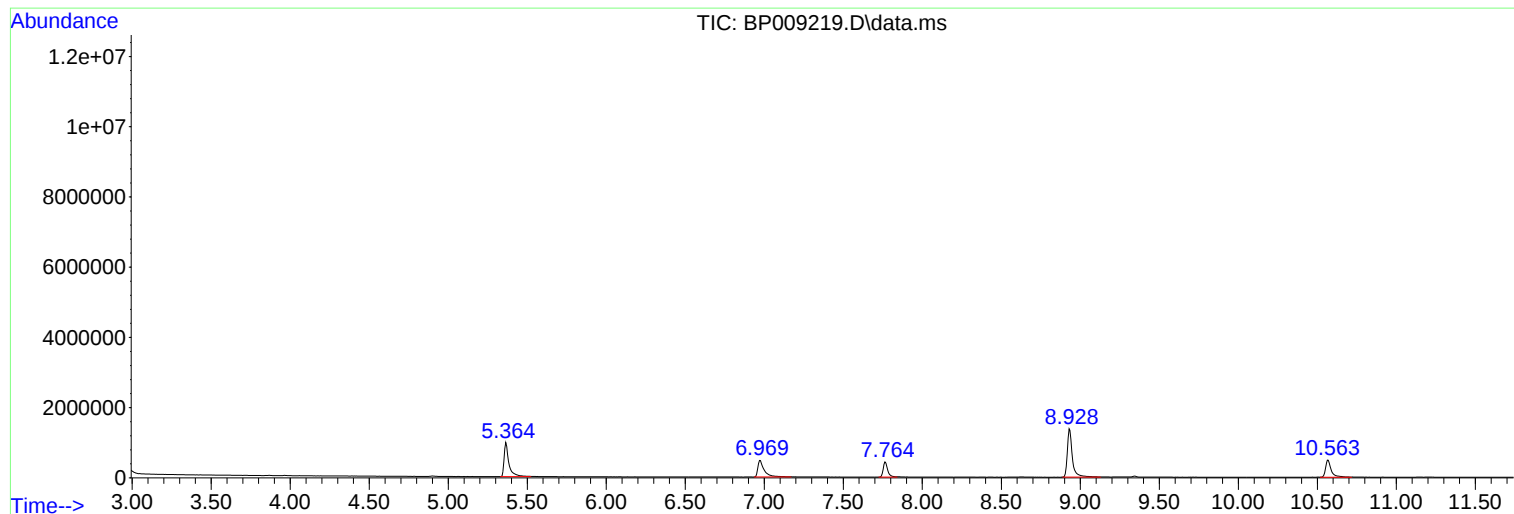

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP021822\  
Data File : BP009219.D  
Acq On : 18 Feb 2022 18:09  
Operator : CG/JU  
Sample : N1587-01  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
FIELD-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP020722.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP021822\  
Data File : BP009219.D  
Acq On : 18 Feb 2022 18:09  
Operator : CG/JU  
Sample : N1587-01  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
FIELD-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP020722.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|