
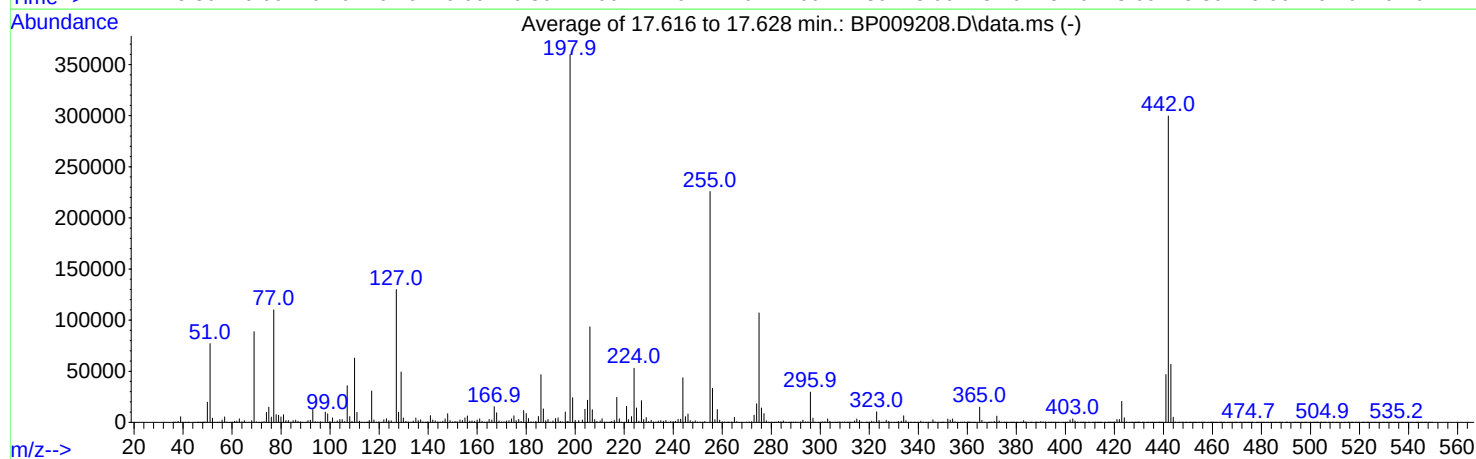


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021822\
 Data File : BP009208.D
 Acq On : 18 Feb 2022 11:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Feb 19 00:46:08 2022

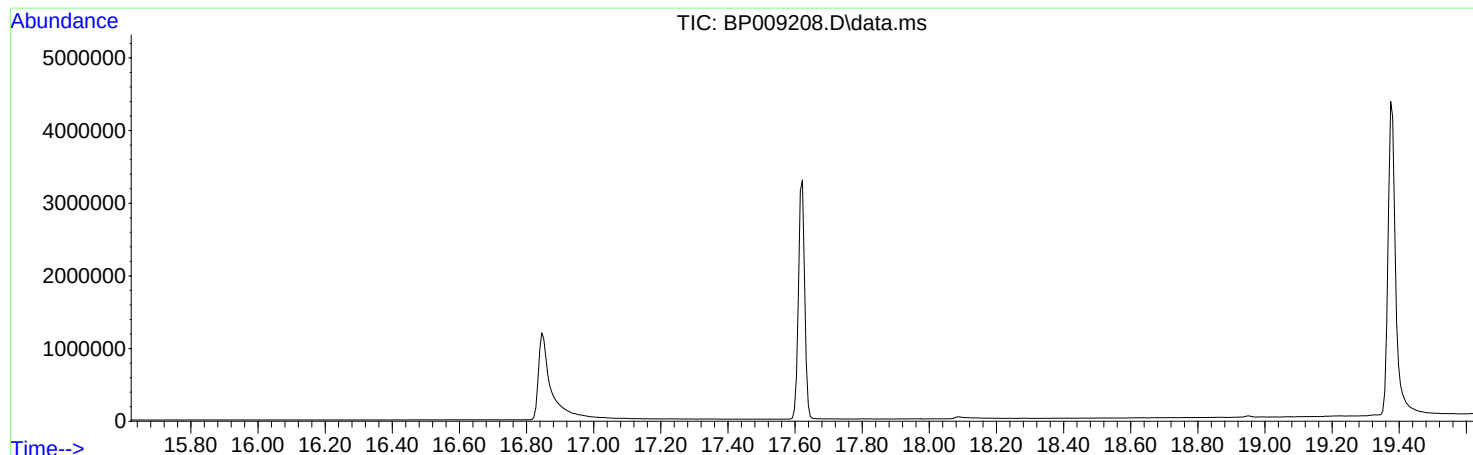




AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.4	77043	PASS
68	69	0.00	2	1.7	1515	PASS
69	198	0.00	100	24.6	88675	PASS
70	69	0.00	2	0.5	455	PASS
127	198	10	80	36.1	129915	PASS
197	198	0.00	2	0.3	989	PASS
198	198	100	100	100.0	359808	PASS
199	198	5	9	6.7	24184	PASS
275	198	10	60	29.7	106983	PASS
365	198	1	100	4.1	14854	PASS
441	198	0.01	100	13.0	46765	PASS
442	442	100	100	100.0	299725	PASS
443	442	15	24	19.0	56883	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021822\
Data File : BP009208.D
Acq On : 18 Feb 2022 11:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 19 02:50:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 19 00:46:08 2022
Response via : Initial Calibration

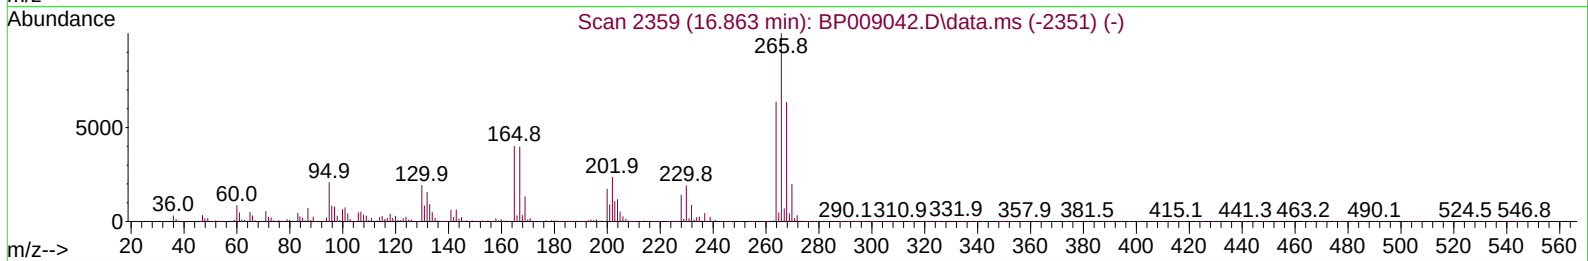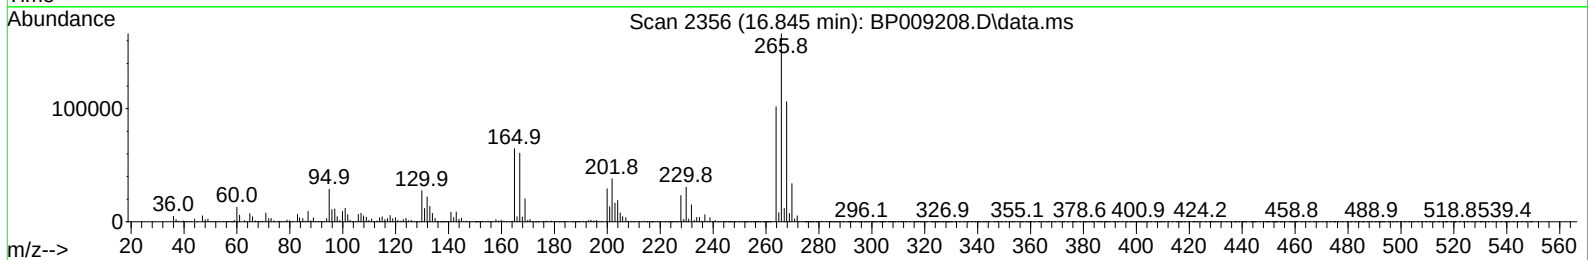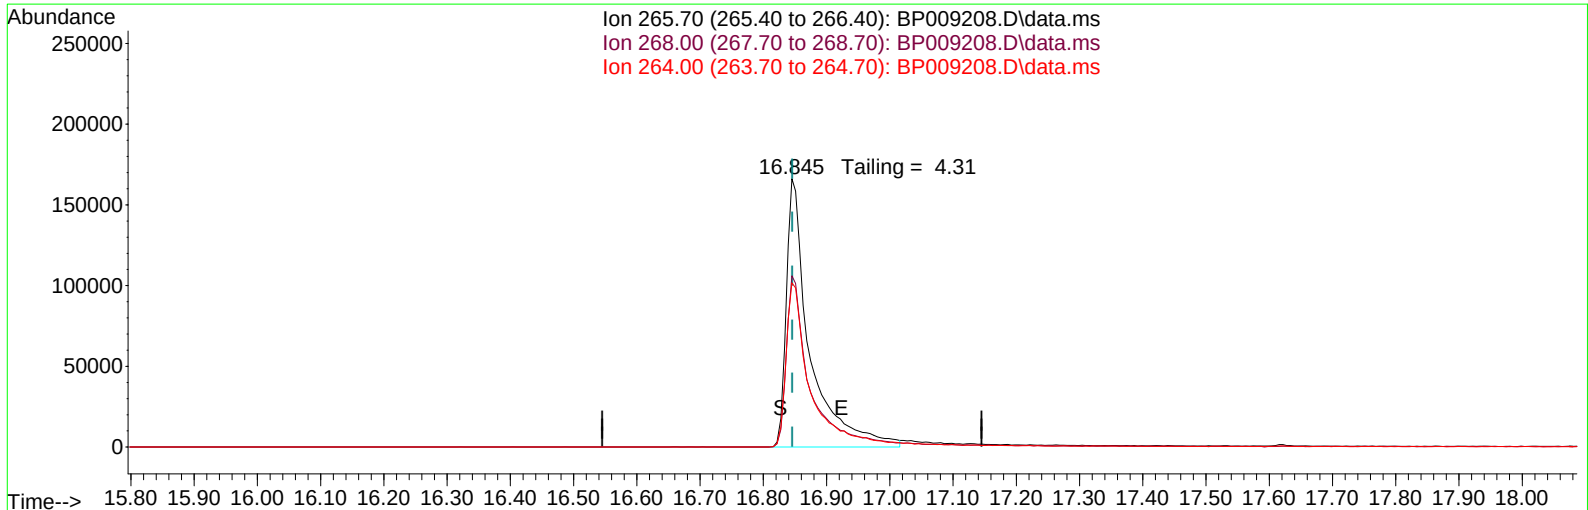

TIC: BP009208.D\data.ms

(70) Pentachlorophenol (C)

16.845min (-0.000) 4329204.64 ng




response 443845

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.82
264.00	62.90	61.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021822\
Data File : BP009208.D
Acq On : 18 Feb 2022 11:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 19 02:50:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 19 00:46:08 2022
Response via : Initial Calibration

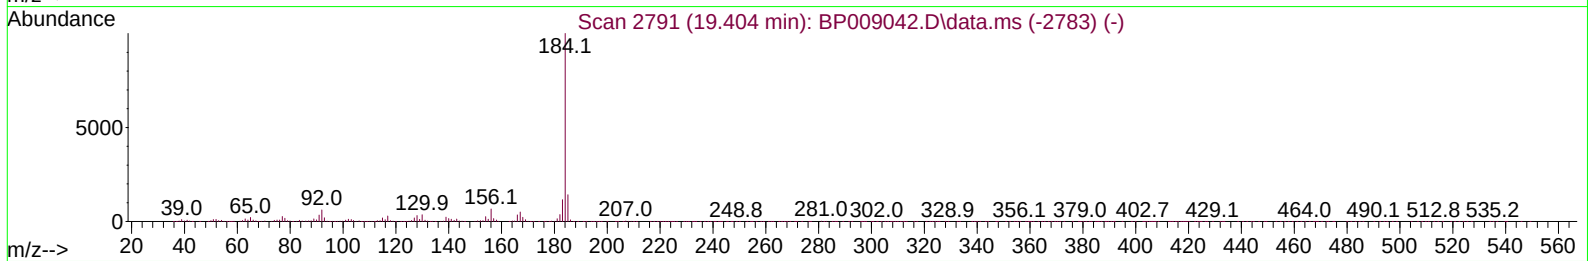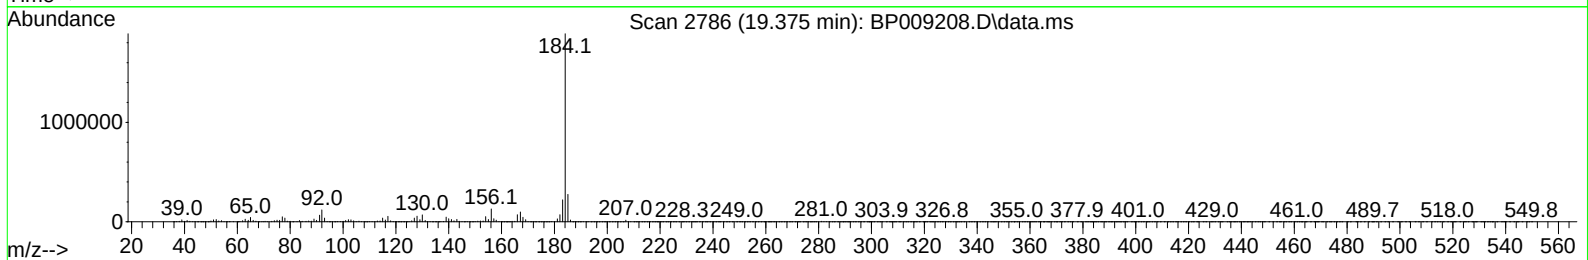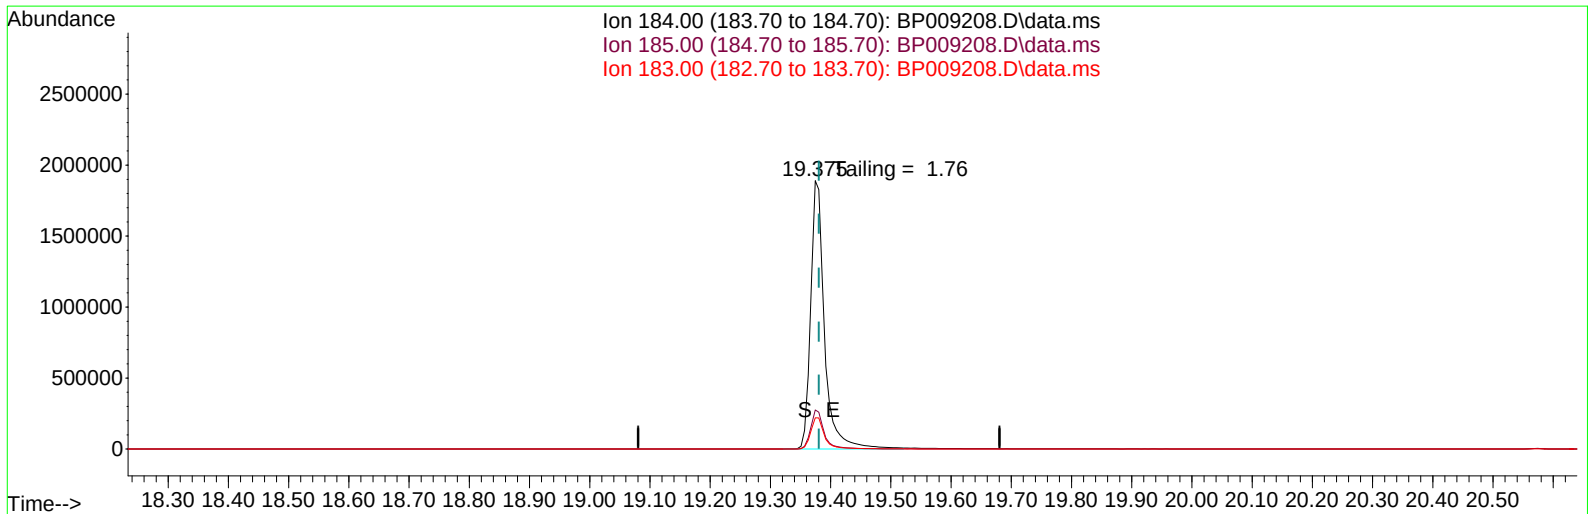

TIC: BP009208.D\data.ms

(77) Benzidine

19.375min (-0.006) 778894.48 ng

response 3059849

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.57
183.00	11.90	11.64
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/18/2022	BNA_P	<u>BP009208.D</u>
Compound Name	Response	Retention Time
DDT	1312934	20.574
DDD	20238	20.151
DDE	4304	19.663
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24542	1337476	1.83

Instrument :
BNA_P
ClientSampleId :
DFTPP