
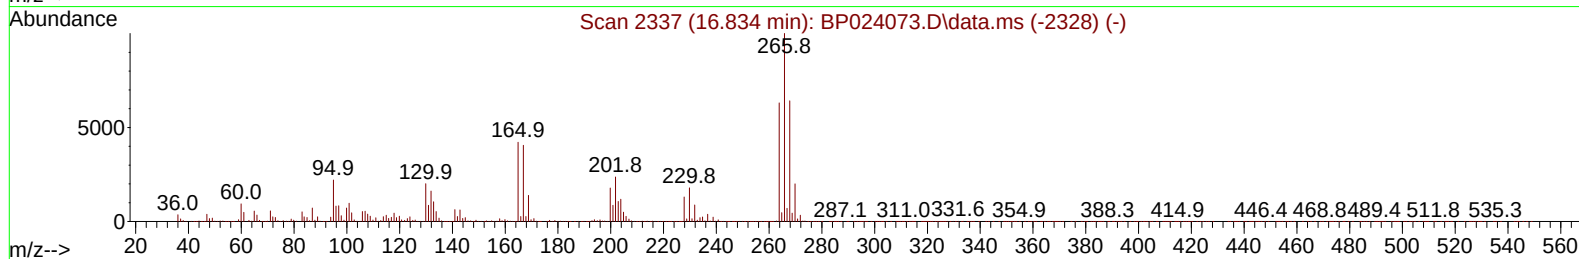
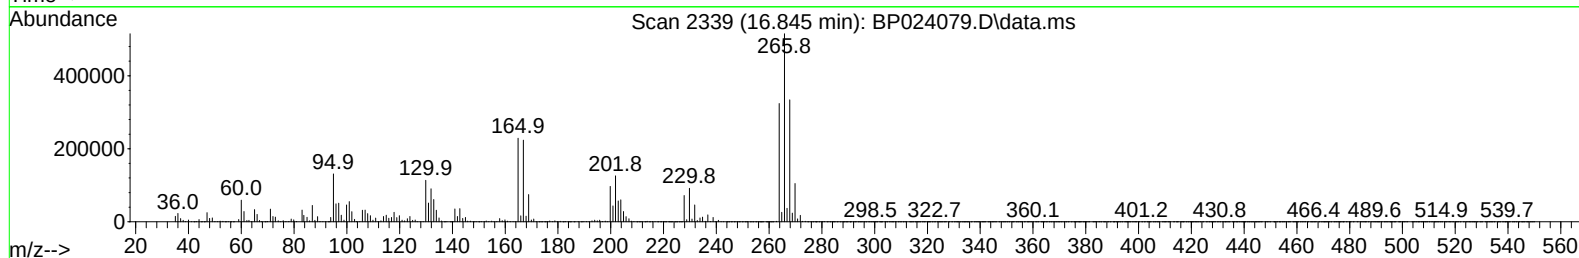


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021825\
Data File : BP024079.D
Acq On : 18 Feb 2025 09:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 18 10:43:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 18 02:25:07 2025
Response via : Initial Calibration

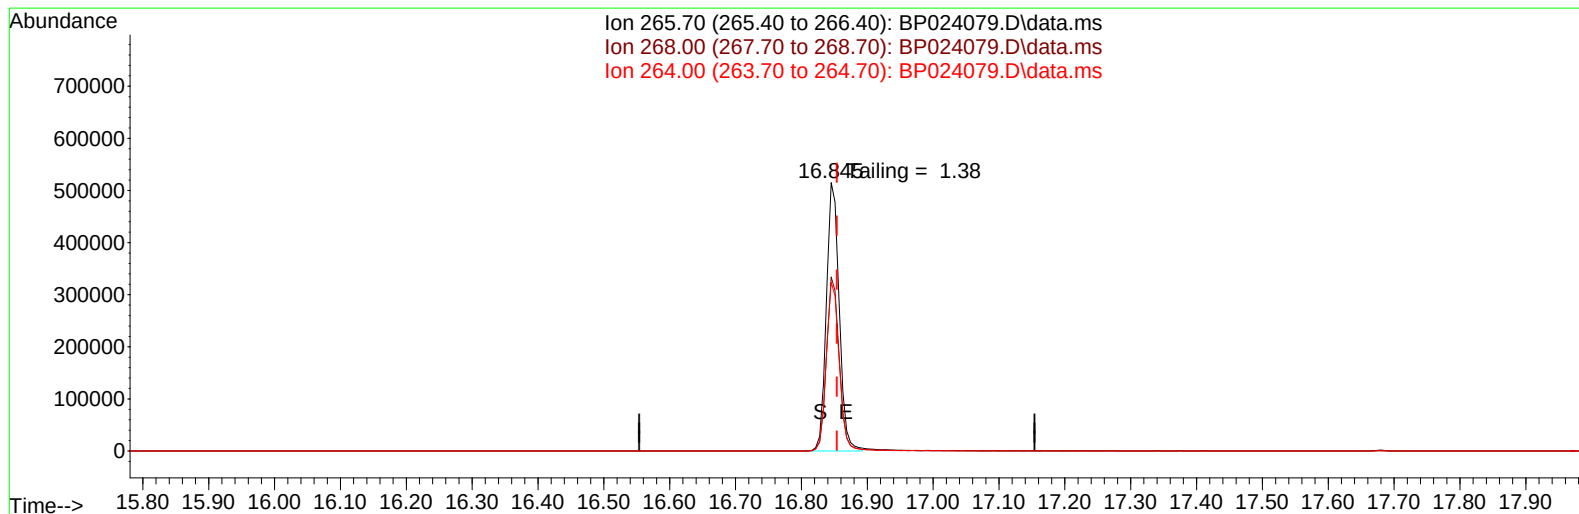

TIC: BP024079.D\data.ms

(70) Pentachlorophenol (C)




16.845min (-0.009) 265514.51 ng

response 710938

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	64.86
264.00	63.10	62.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021825\
Data File : BP024079.D
Acq On : 18 Feb 2025 09:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 18 10:43:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 18 02:25:07 2025
Response via : Initial Calibration

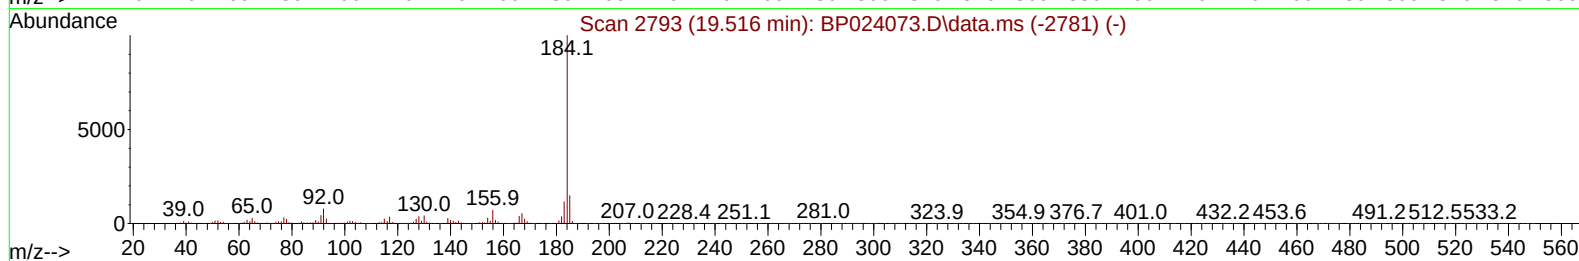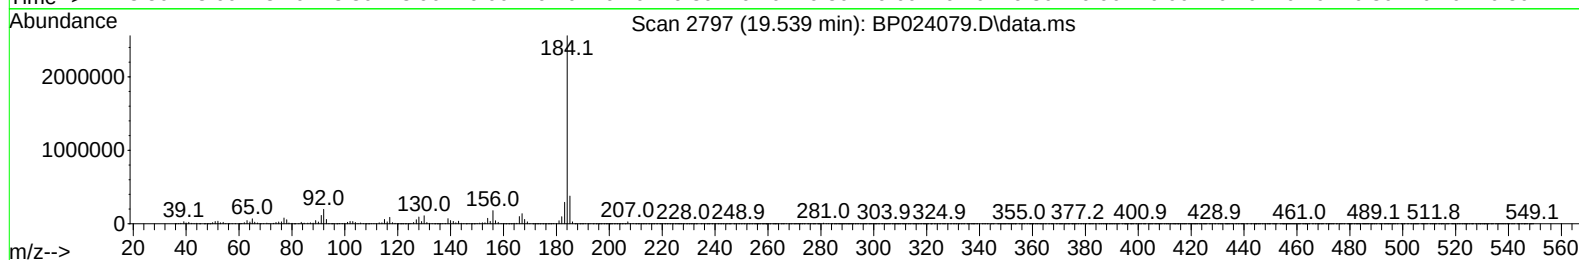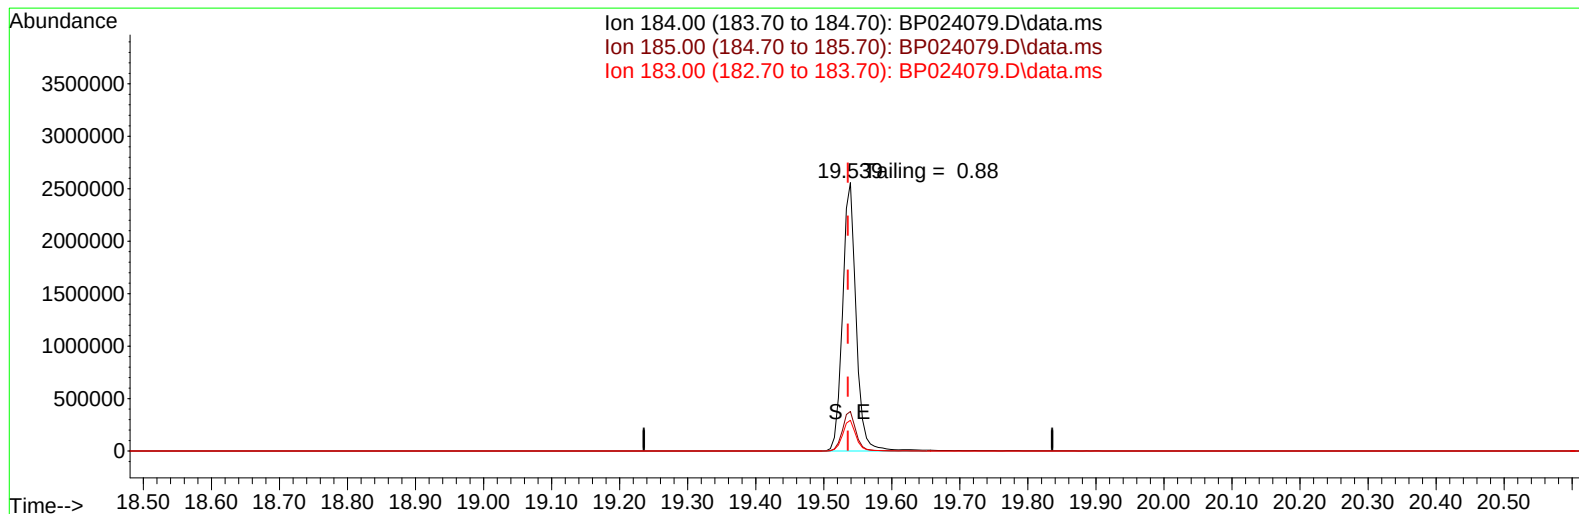

TIC: BP024079.D\data.ms

(77) Benzidine**19.539min (+ 0.003) 291364.18 ng****response 3507831**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.76
183.00	11.60	11.44
0.00	0.00	0.00