
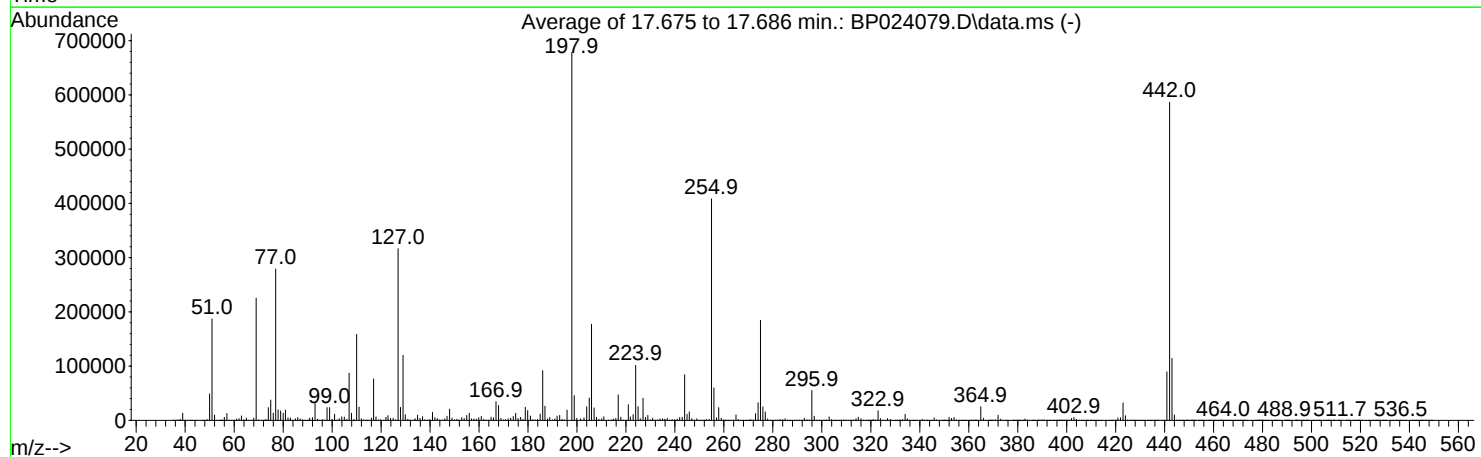


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021825\
Data File : BP024079.D
Acq On : 18 Feb 2025 09:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Feb 18 02:25:07 2025

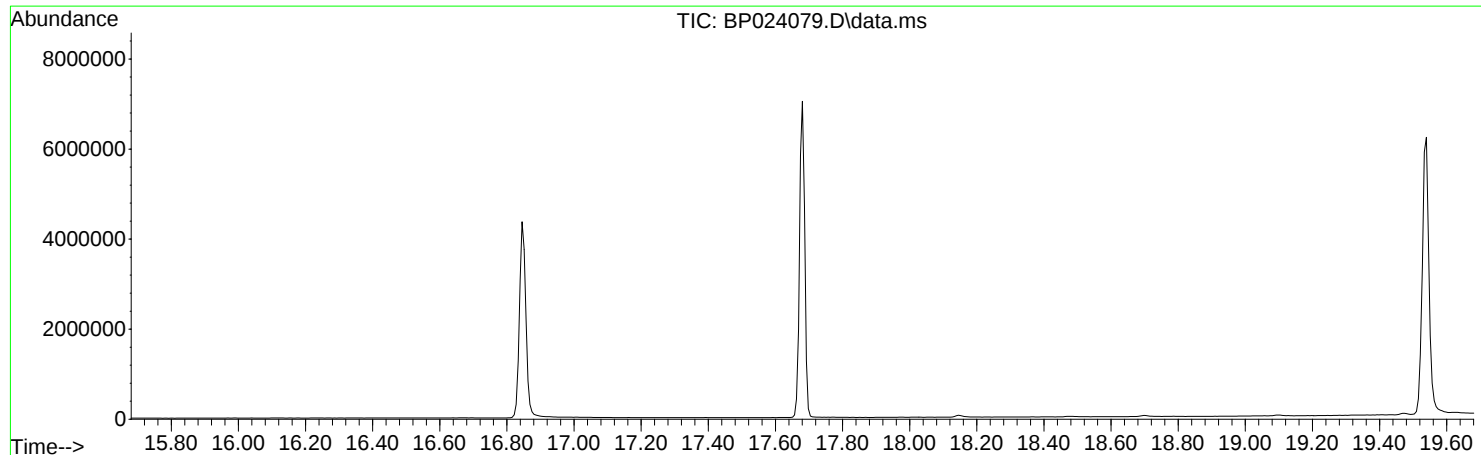




AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	27.6	187056	PASS
68	69	0.00	2	1.8	4024	PASS
69	198	0.00	100	33.2	225245	PASS
70	69	0.00	2	0.5	1019	PASS
127	198	10	80	46.7	316549	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	678126	PASS
199	198	5	9	6.7	45699	PASS
275	198	10	60	27.2	184314	PASS
365	198	1	100	3.7	25218	PASS
441	198	0.01	100	13.2	89506	PASS
442	442	100	100	100.0	586558	PASS
443	442	15	24	19.5	114424	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021825\
Data File : BP024079.D
Acq On : 18 Feb 2025 09:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 18 10:43:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 18 02:25:07 2025
Response via : Initial Calibration

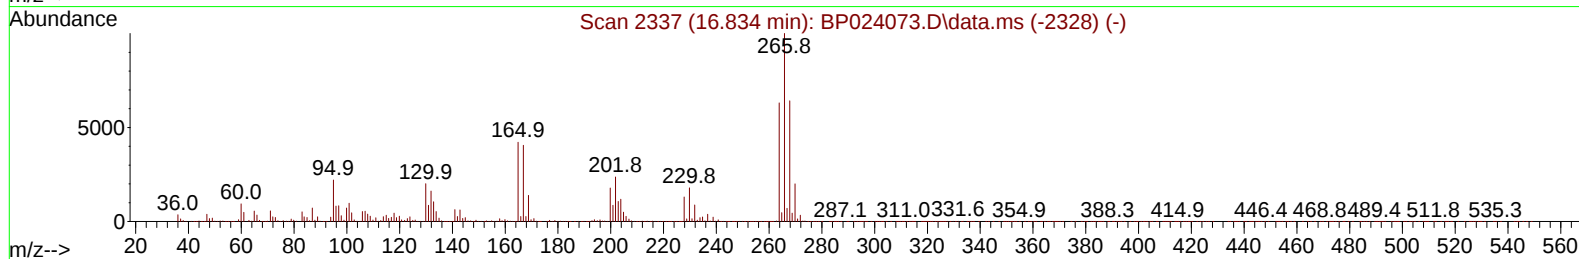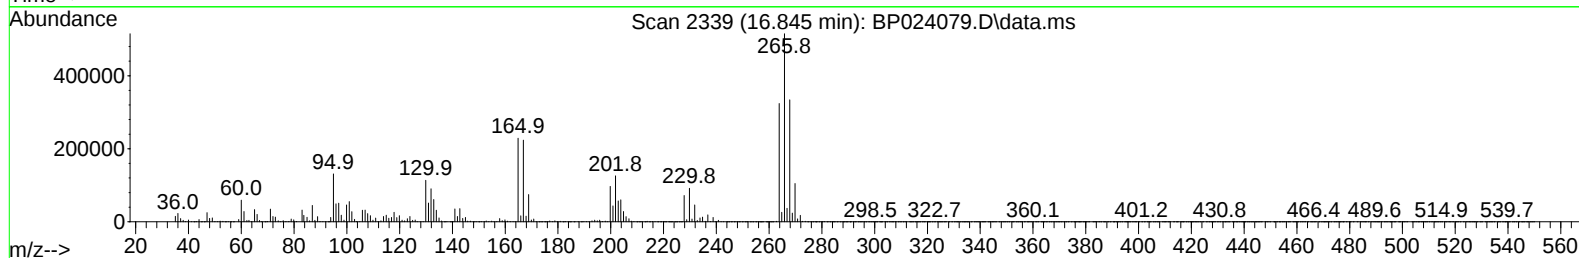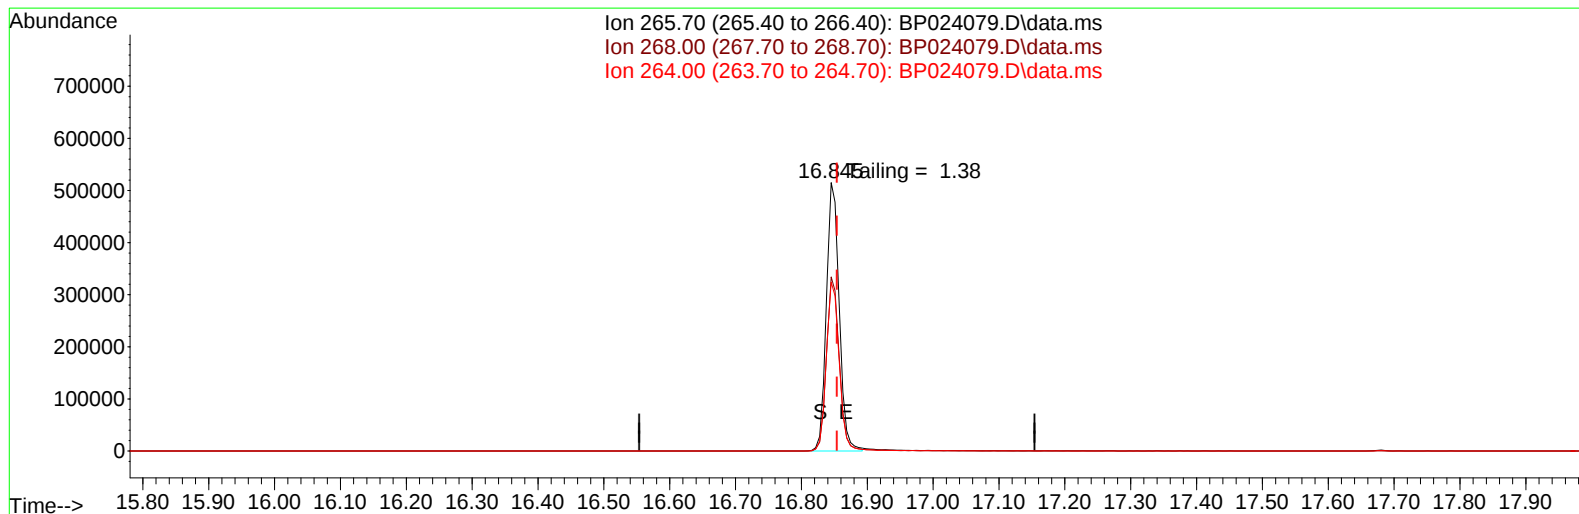

TIC: BP024079.D\data.ms

(70) Pentachlorophenol (C)

16.845min (-0.009) 265514.51 ng




response 710938

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	64.86
264.00	63.10	62.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021825\
Data File : BP024079.D
Acq On : 18 Feb 2025 09:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 18 10:43:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 18 02:25:07 2025
Response via : Initial Calibration

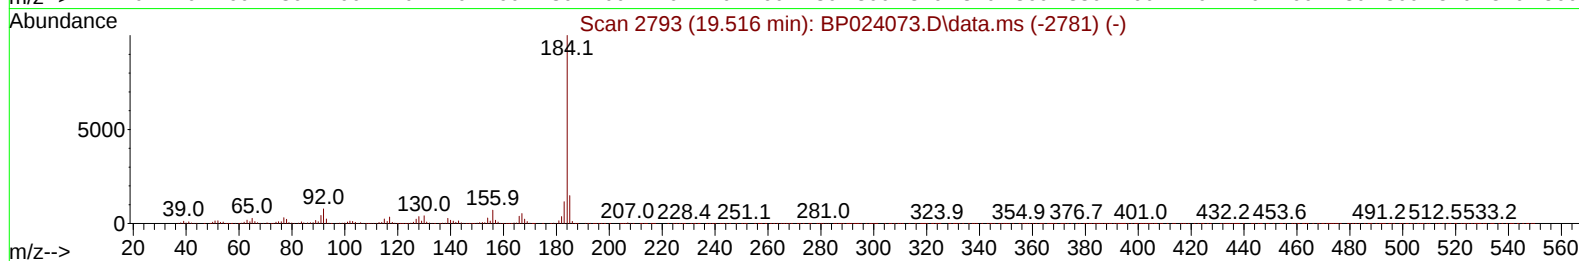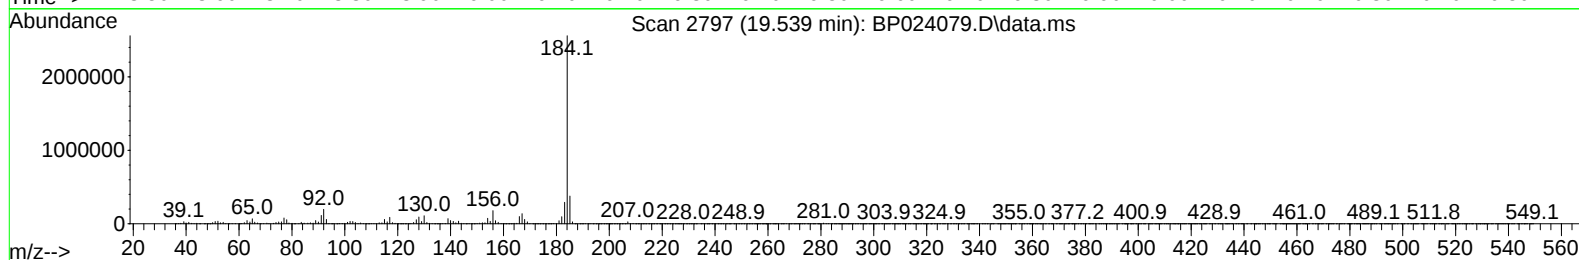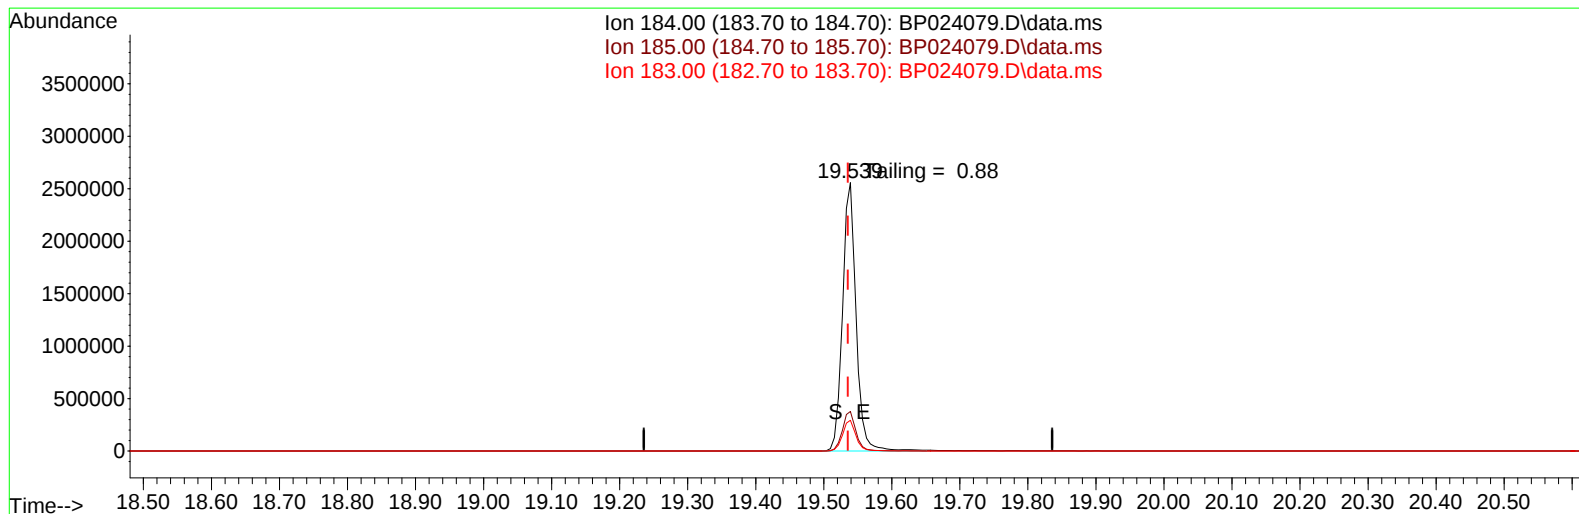

TIC: BP024079.D\data.ms

(77) Benzidine

19.539min (+ 0.003) 291364.18 ng

response 3507831

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.76
183.00	11.60	11.44
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/18/2024	BNA_P	<u>BP024079.D</u>
Compound Name	Response	Retention Time
DDT	1952571	20.833
DDD	17011	20.41
DDE	677	19.839
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17688	1970259	0.90

Instrument :
BNA_P
ClientSampleId :
DFTPP