

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP021920\
 Data File : BP001776.D
 Acq On : 19 Feb 2020 13:49
 Operator : CG/JU
 Sample : L1424-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C5B03

Quant Time: Feb 19 15:51:44 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 19 02:37:06 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	441771	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	1854202	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	1164374	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	2560674	20.00	ng/ul	0.00
78) Chrysene-d12	21.13	240	2697630	20.00	ng/ul	0.00
86) Perylene-d12	23.34	264	2878861	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.18	96	29637	2.79	ng/uL	0.00
5) Phenol-d5	6.83	99	570191	17.08	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	342259	17.65	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	477175	17.69	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	399050	15.07	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	203818	16.24	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	191132	16.84	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	463799	17.18	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	433239	13.57	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	1558790	19.08	ng/ul	0.00
47) Acenaphthylene-d8	13.98	160	1845121	18.34	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	171401	12.05	ng/ul	0.00
58) Fluorene-d10	15.29	176	1436188	19.54	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	117038	11.59	ng/ul	0.00
71) Anthracene-d10	17.14	188	2165486	19.20	ng/ul	0.00
79) Pyrene-d10	19.39	212	2652212	19.16	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.20	264	2778593	19.98	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.75	163	117606	1.367	ng/ul	100




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP021920\
Data File : BP001776.D
Acq On : 19 Feb 2020 13:49
Operator : CG/JU
Sample : L1424-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C5B03

Quant Time: Feb 19 15:51:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 19 02:37:06 2020
Response via : Initial Calibration

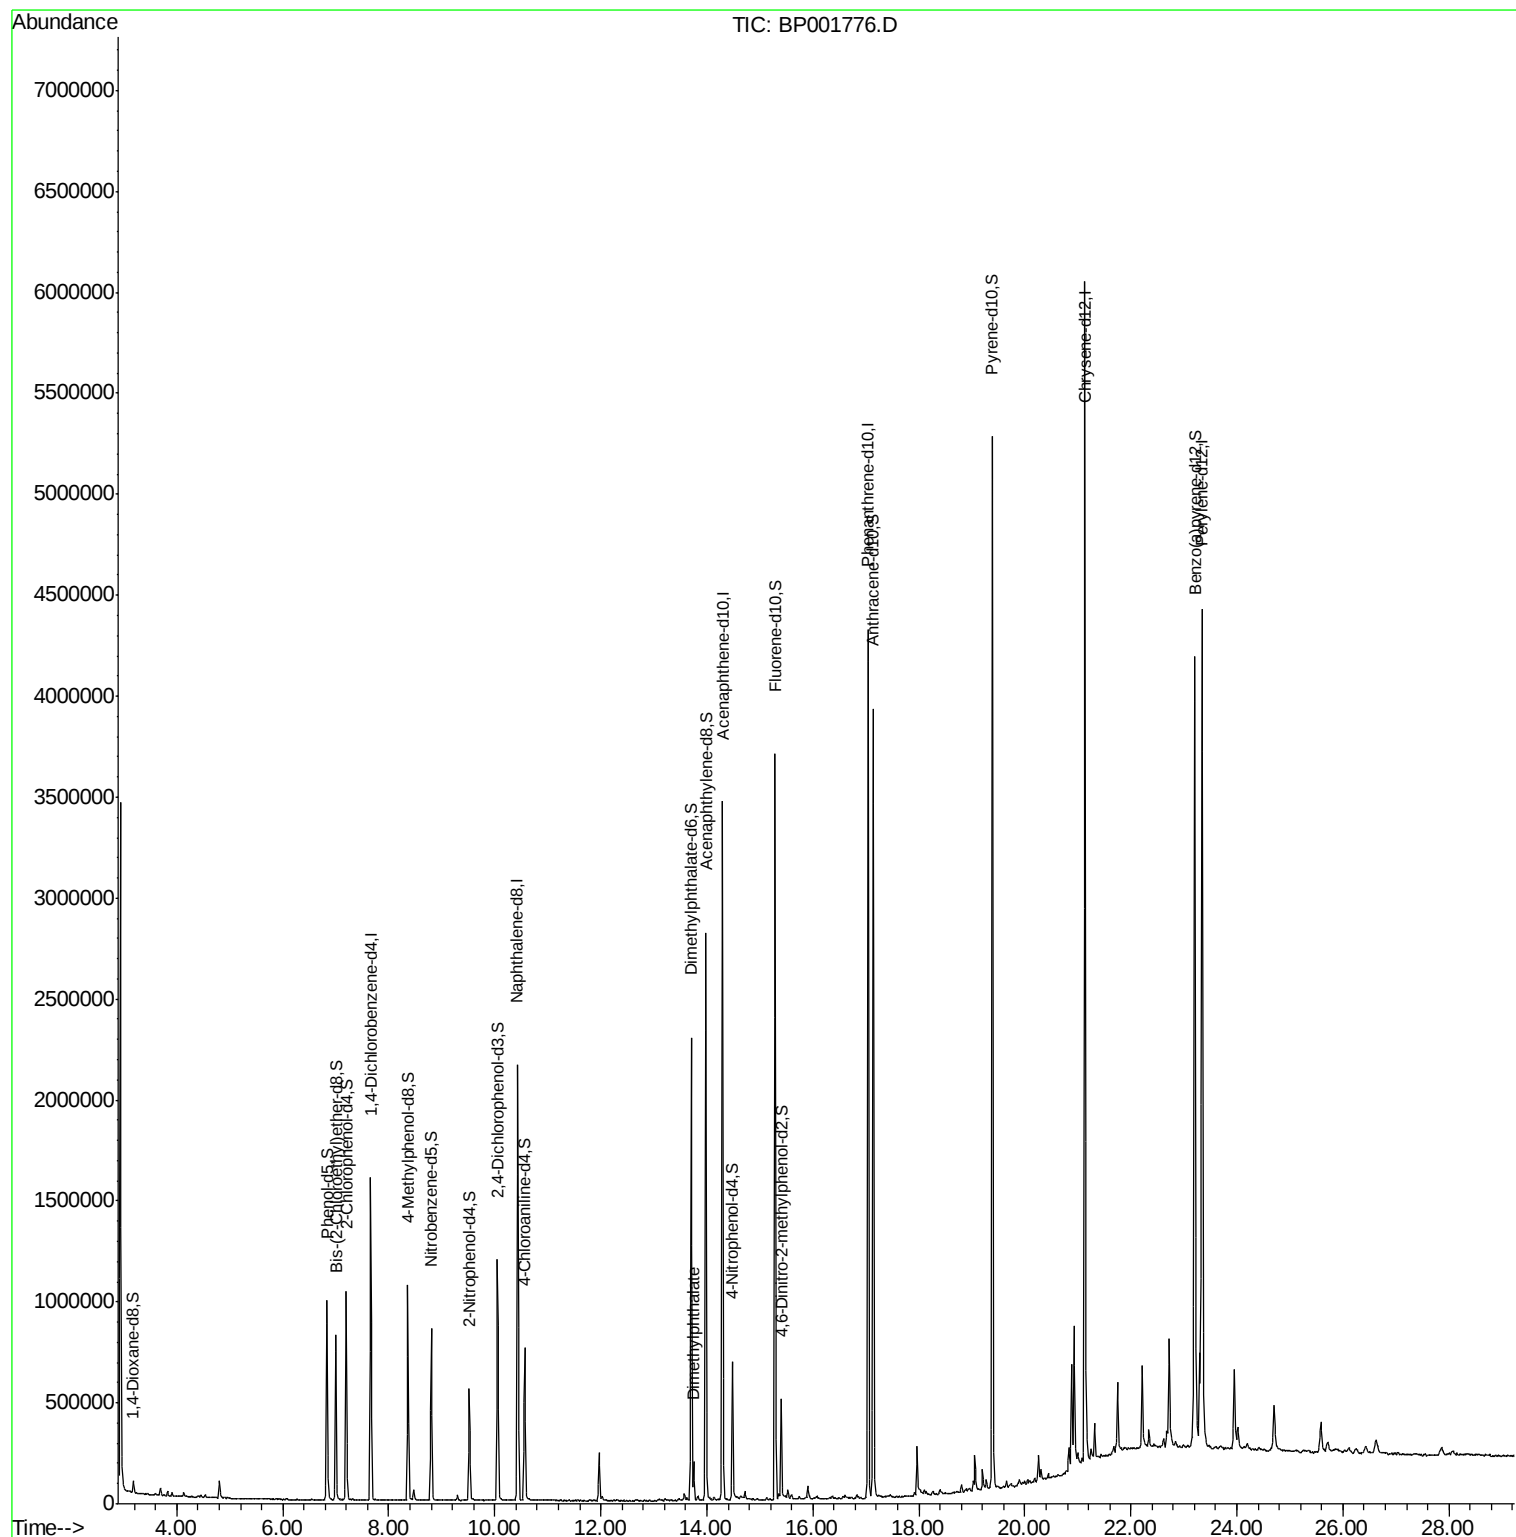

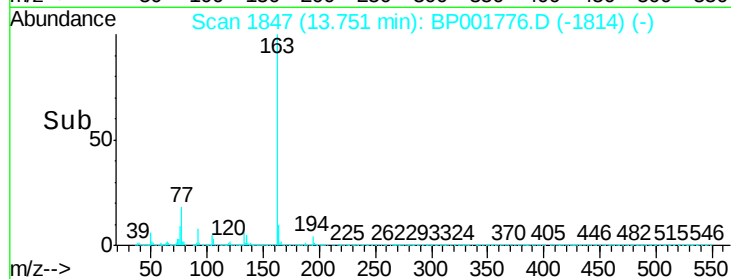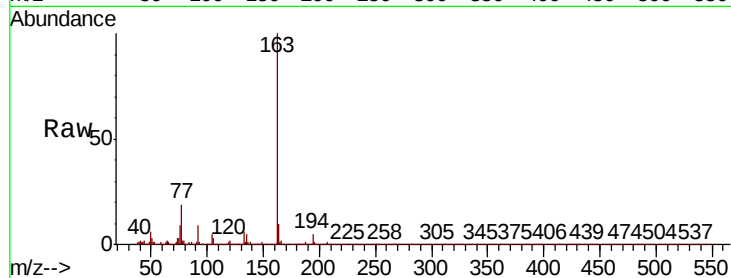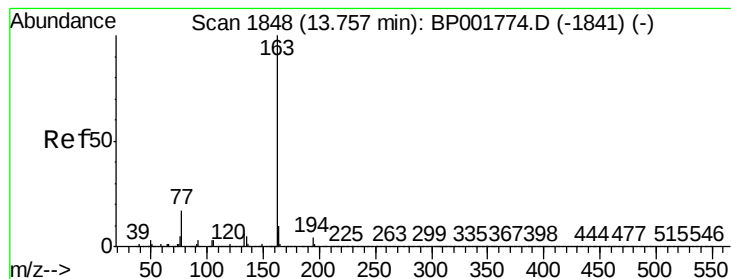

#45

Dimethylphthalate

Concen: 1.367 ng/ul

RT: 13.75 min Scan# 1847

Delta R.T. -0.01 min

Lab File: BP001776.D

Acq: 19 Feb 2020 13:49

Instrument :

BNA_P

ClientSampleId :

C5B03

Tot Ion:163 Resp: 117606

Ion Ratio Lower Upper

163 100

194 4.5 3.5 5.3

164 9.9 8.0 12.0

