

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP021920\
 Data File : BP001777.D
 Acq On : 19 Feb 2020 14:23
 Operator : CG/JU
 Sample : L1424-04
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C5B06

Quant Time: Feb 19 16:17:32 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 19 02:37:06 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	438746	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	1857695	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	1167838	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	2553931	20.00	ng/ul	0.00
78) Chrysene-d12	21.13	240	2701320	20.00	ng/ul	0.00
86) Perylene-d12	23.34	264	2904877	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.18	96	51558	4.88	ng/uL	0.00
5) Phenol-d5	6.83	99	875320	26.40	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	535415	27.80	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	755026	28.18	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	700534	26.64	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	342109	27.20	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	332200	29.21	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	708149	26.19	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	1033248	32.30	ng/ul	0.00
44) Dimethylphthalate-d6	13.71	166	2243786	27.38	ng/ul	0.00
47) Acenaphthylene-d8	13.98	160	2745396	27.21	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	292128	20.47	ng/ul	0.00
58) Fluorene-d10	15.29	176	2048525	27.79	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	187361	18.61	ng/ul	0.00
71) Anthracene-d10	17.14	188	3107312	27.62	ng/ul	0.00
79) Pyrene-d10	19.39	212	3592276	25.91	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.20	264	3943322	28.11	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.75	163	195726	2.269	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP021920\
Data File : BP001777.D
Acq On : 19 Feb 2020 14:23
Operator : CG/JU
Sample : L1424-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C5B06

Quant Time: Feb 19 16:17:32 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 19 02:37:06 2020
Response via : Initial Calibration

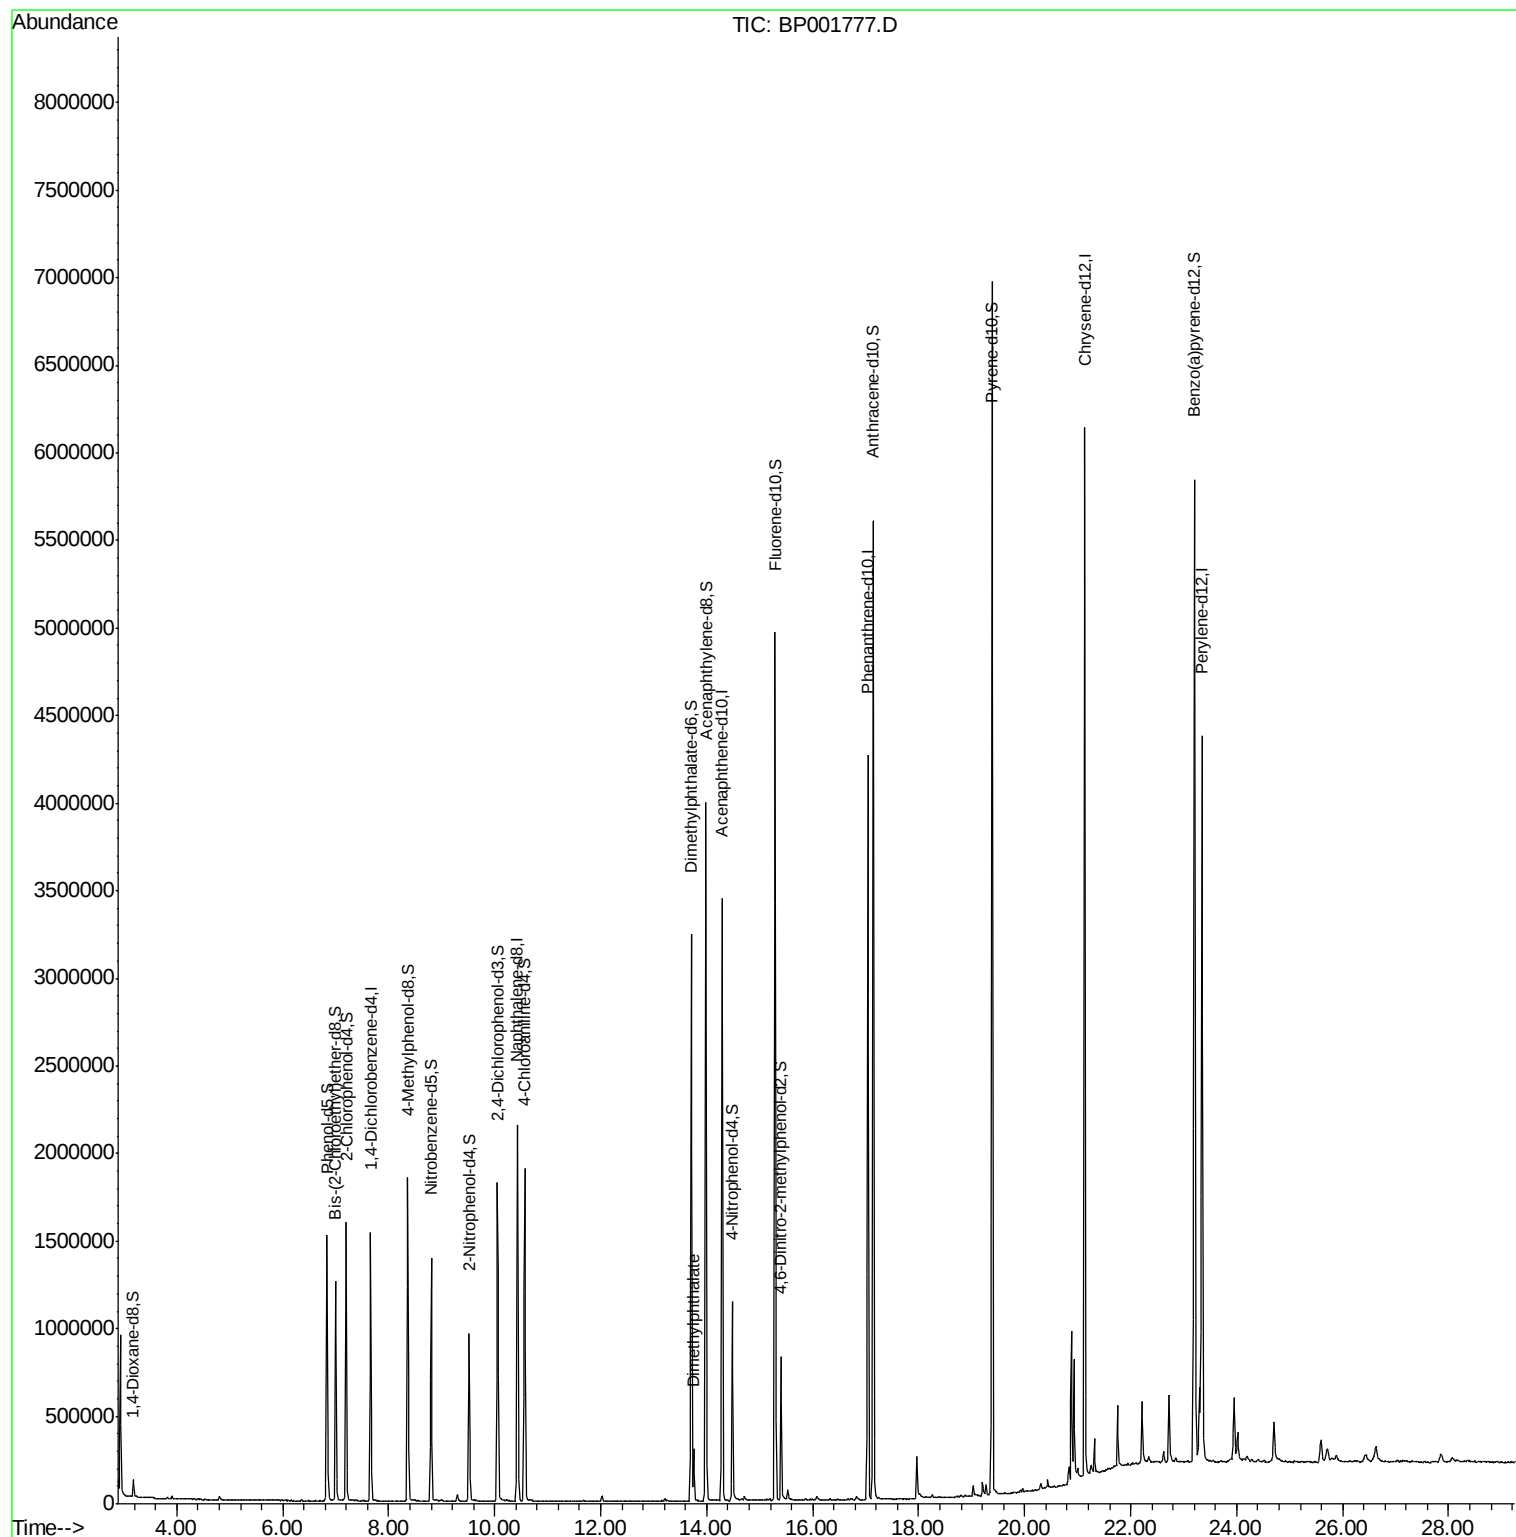

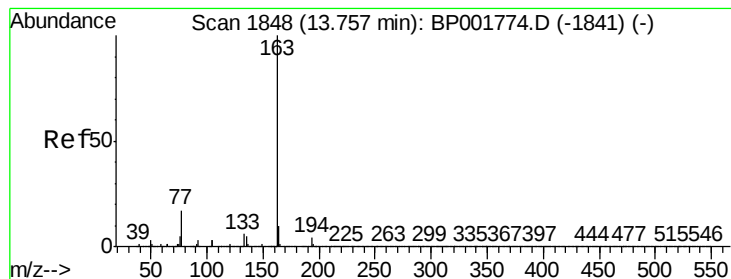

#45

Dimethylphthalate

Concen: 2.269 ng/ul

RT: 13.75 min Scan# 1847

Delta R.T. -0.01 min

Lab File: BP001777.D

Acq: 19 Feb 2020 14:23

Instrument :

BNA_P

ClientSampleId :

C5B06


Tot Ion:163 Resp: 195726

Ion Ratio Lower Upper

163 100

194 4.0 3.5 5.3

164 9.9 8.0 12.0

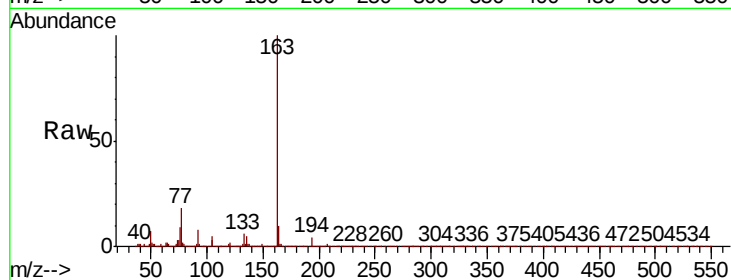

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

