
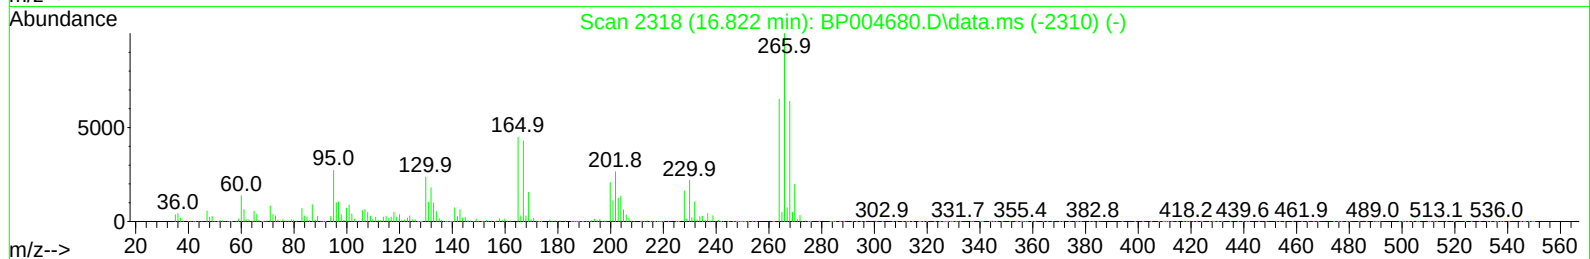
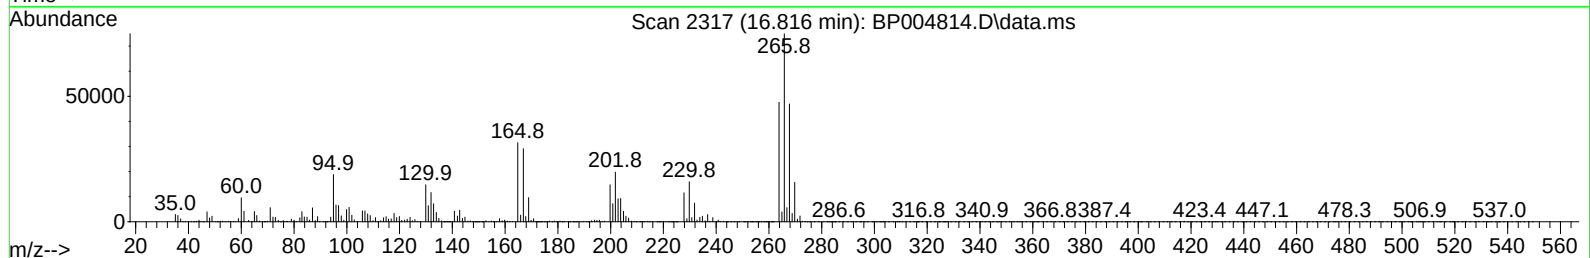


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021921\
Data File : BP004814.D
Acq On : 19 Feb 2021 10:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 19 11:22:24 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 05 18:04:48 2021
Response via : Initial Calibration

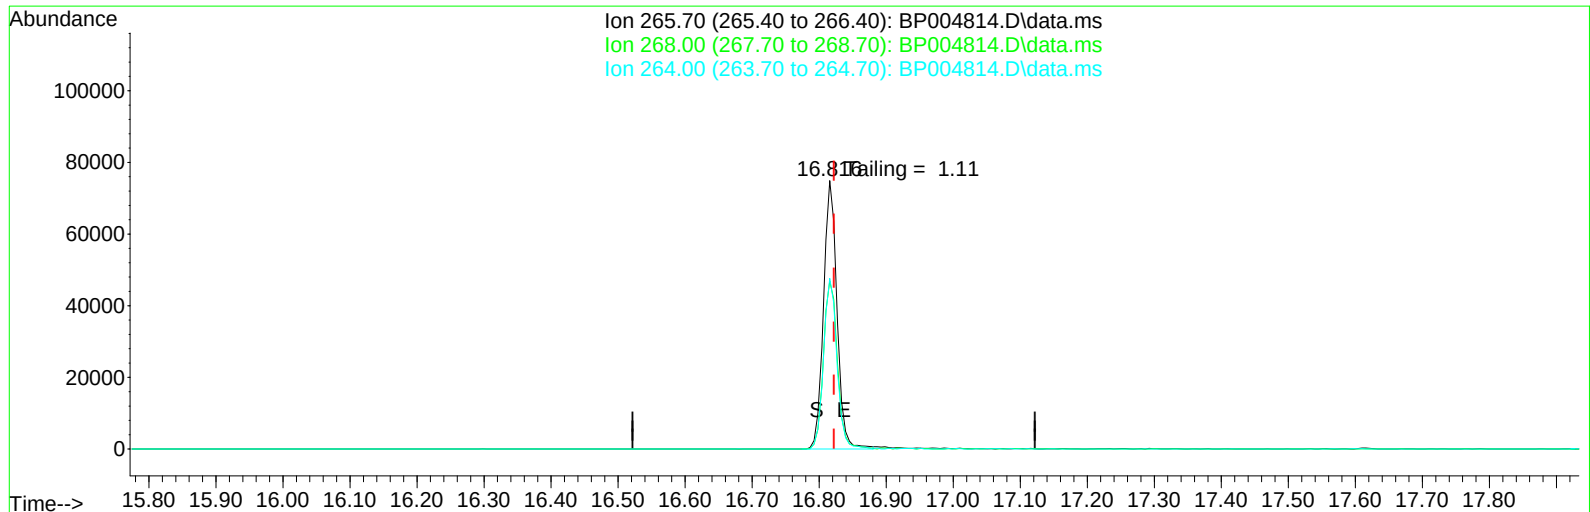

TIC: BP004814.D\data.ms

(70) Pentachlorophenol (C)




16.816min (-0.006) 564943.96 ng

response 106440

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	62.62
264.00	63.30	63.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021921\
 Data File : BP004814.D
 Acq On : 19 Feb 2021 10:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 19 11:22:24 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 05 18:04:48 2021
 Response via : Initial Calibration

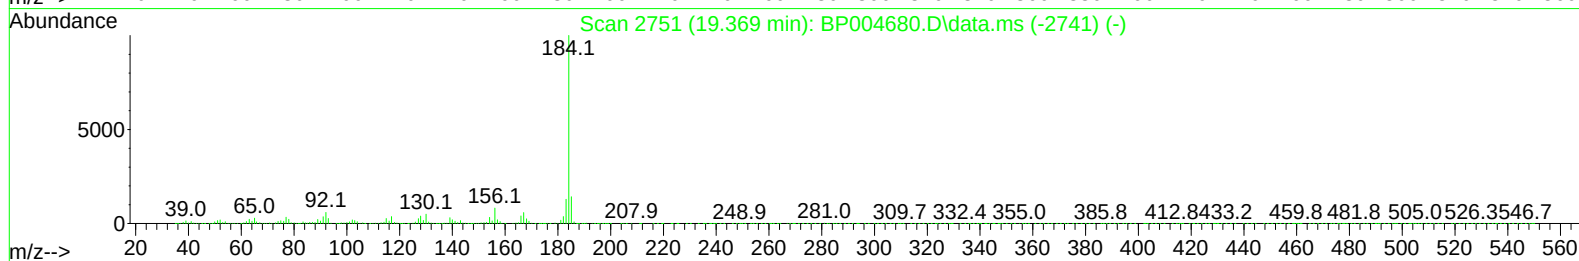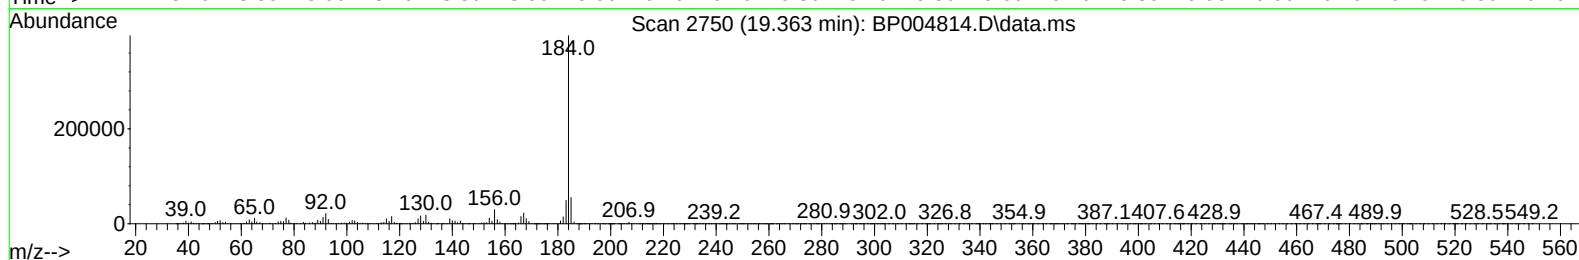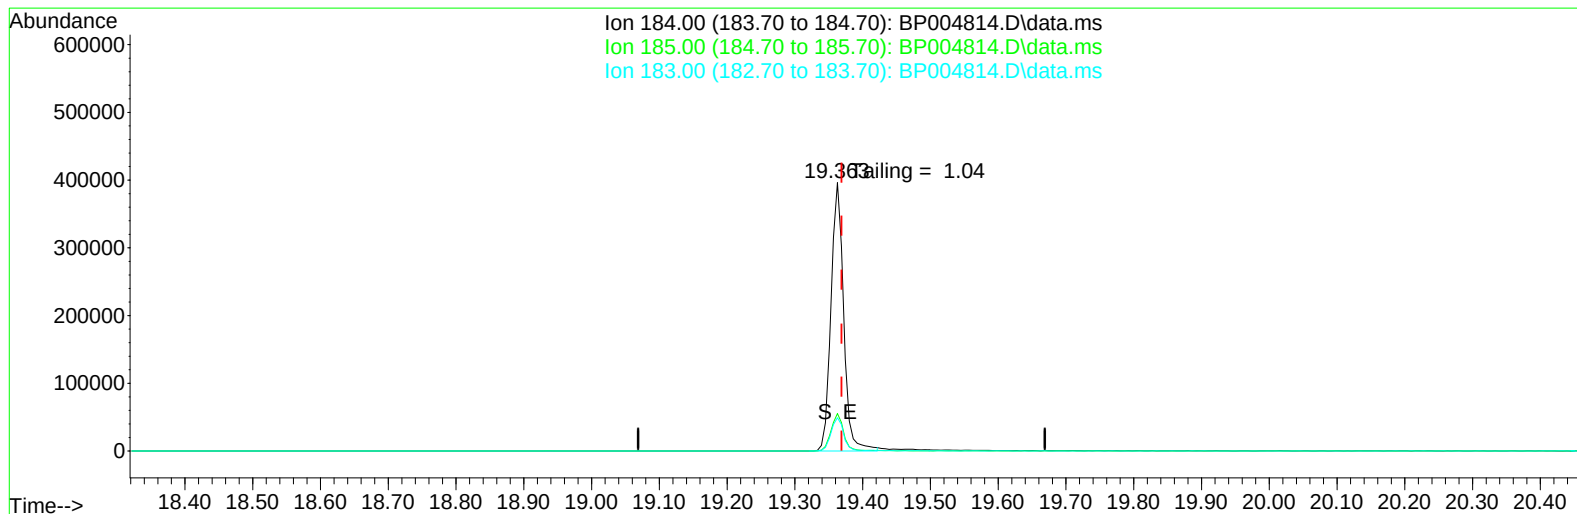

TIC: BP004814.D\data.ms

(77) Benzidine**19.363min (-0.006) 142991.84 ng****response 521431**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.97
183.00	12.00	12.42
0.00	0.00	0.00