
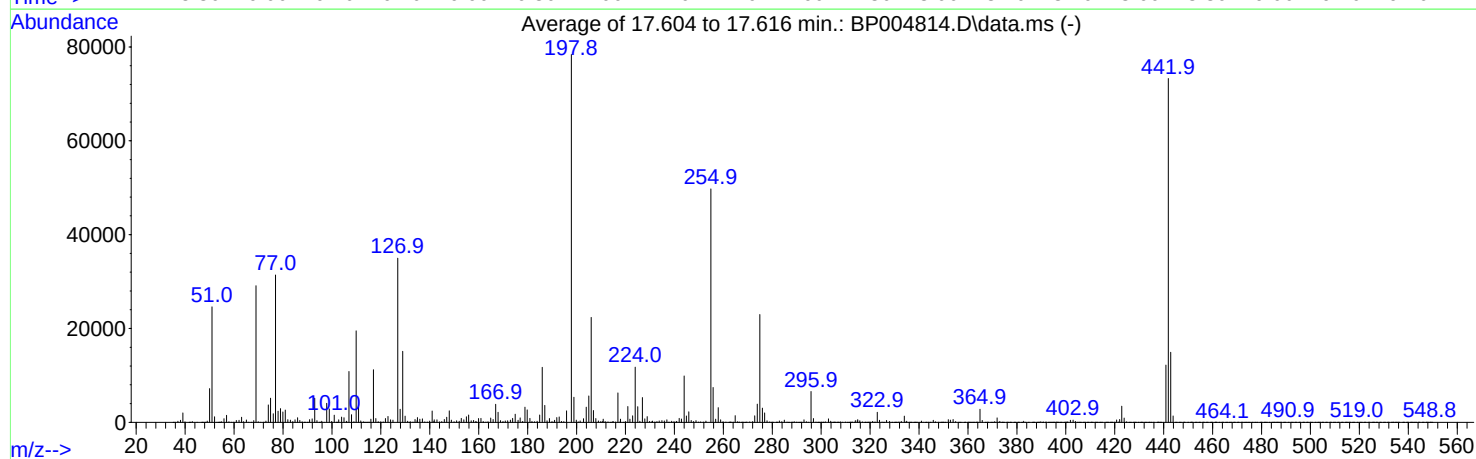


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021921\
 Data File : BP004814.D
 Acq On : 19 Feb 2021 10:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 19 12:04:44 2021

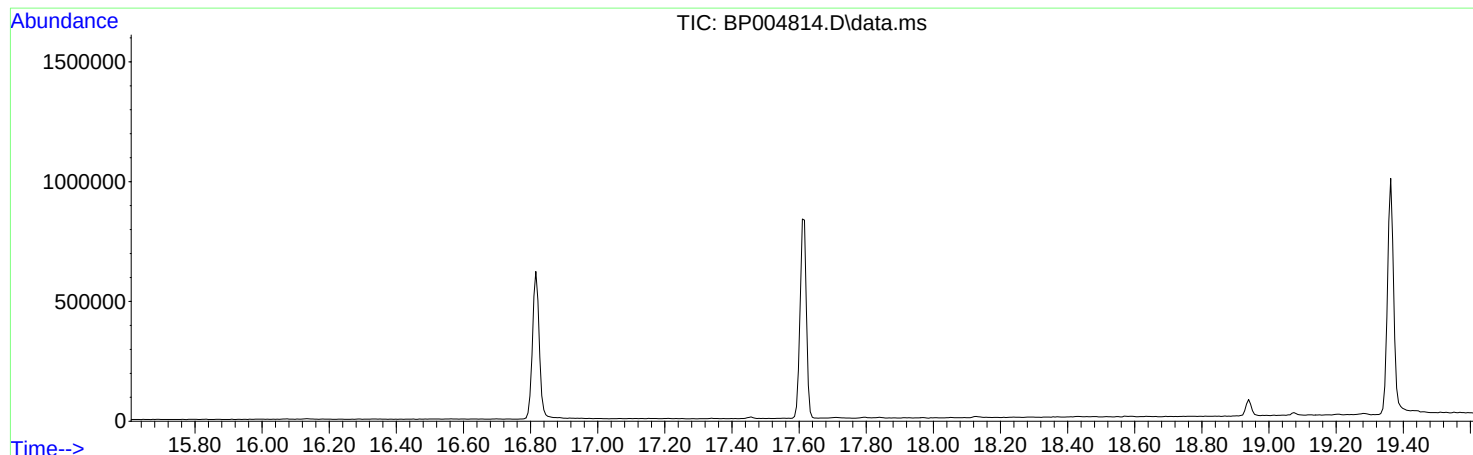




AutoFind: Scans 2451, 2452, 2453; Background Corrected with Scan 2444

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.4	24608	PASS
68	69	0.00	2	1.4	395	PASS
69	198	0.00	100	37.1	29106	PASS
70	69	0.00	2	0.5	138	PASS
127	198	10	80	44.6	34990	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	78388	PASS
199	198	5	9	6.8	5343	PASS
275	198	10	60	29.3	22989	PASS
365	198	1	100	3.6	2783	PASS
441	198	0.01	100	15.6	12219	PASS
442	442	100	100	100.0	73272	PASS
443	442	15	24	20.4	14939	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021921\
Data File : BP004814.D
Acq On : 19 Feb 2021 10:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 19 11:22:24 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 05 18:04:48 2021
Response via : Initial Calibration

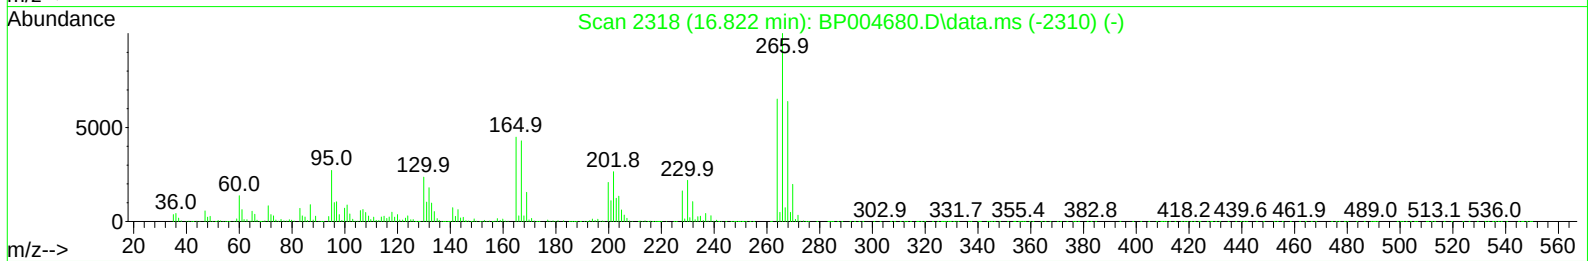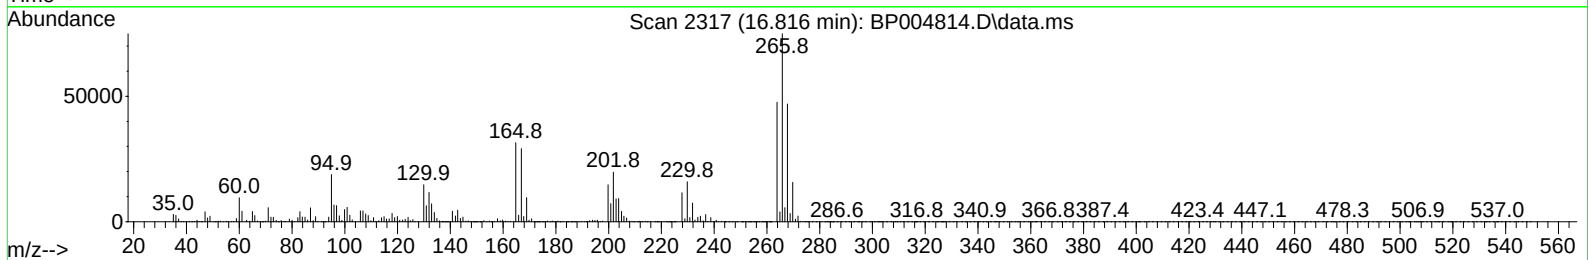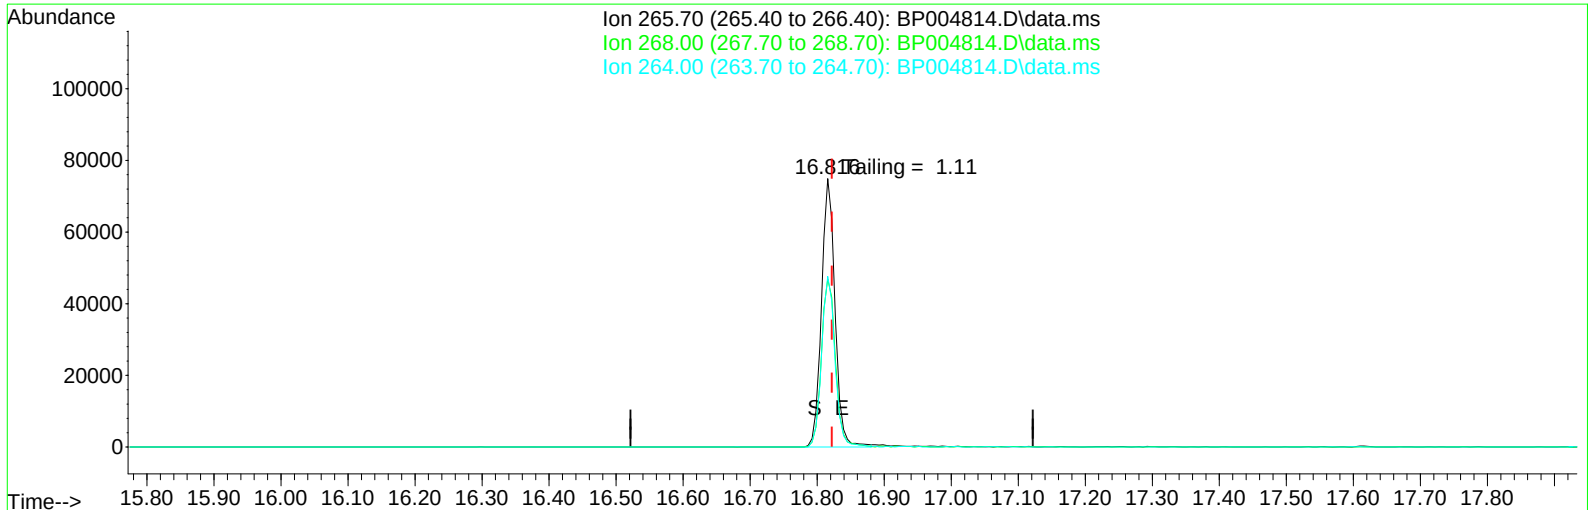

TIC: BP004814.D\data.ms

(70) Pentachlorophenol (C)

16.816min (-0.006) 564943.96 ng




response 106440

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	62.62
264.00	63.30	63.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021921\
Data File : BP004814.D
Acq On : 19 Feb 2021 10:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 19 11:22:24 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 05 18:04:48 2021
Response via : Initial Calibration

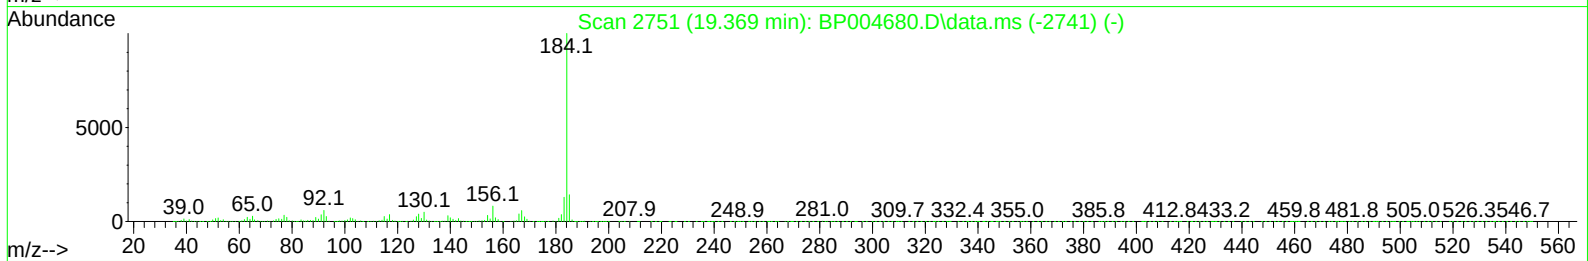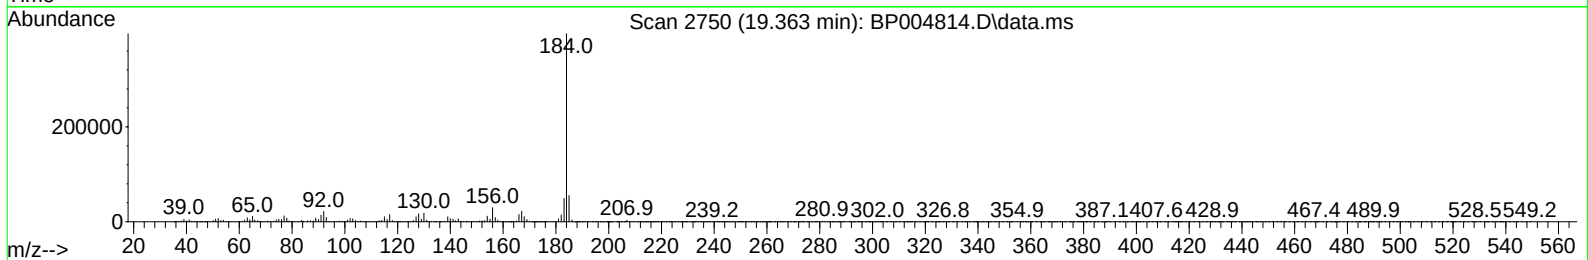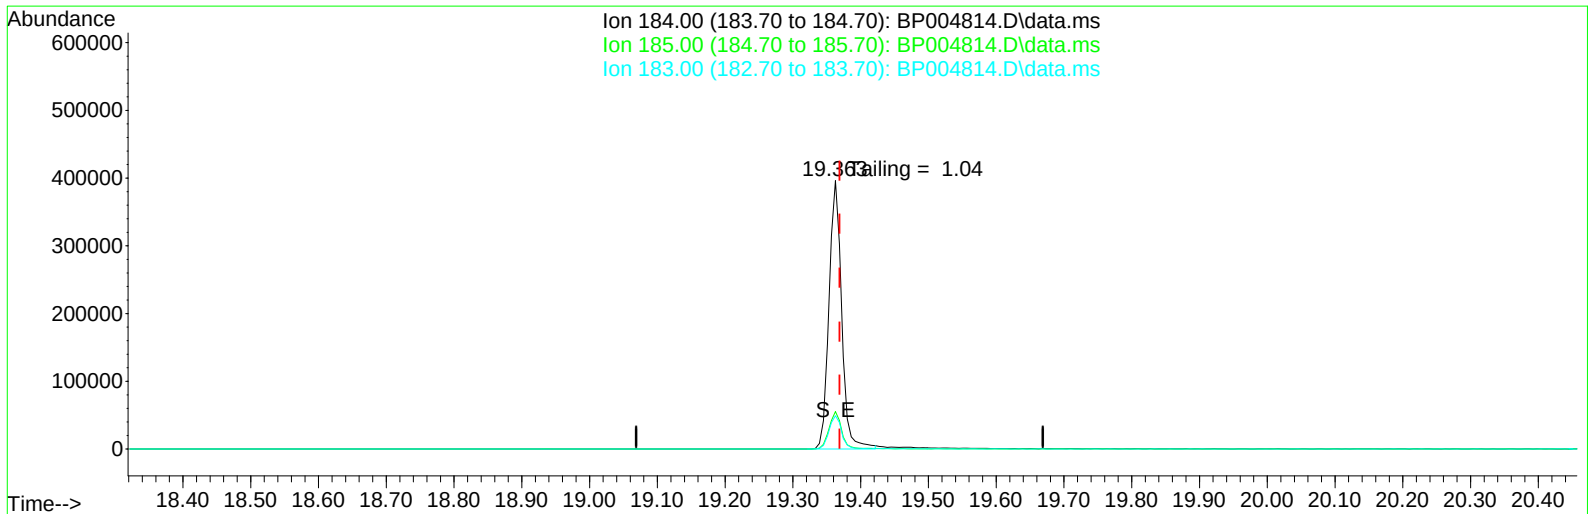

TIC: BP004814.D\data.ms

(77) Benzidine

19.363min (-0.006) 142991.84 ng

response 521431

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.97
183.00	12.00	12.42
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/19/2021	BNA_P	BP004814.D
Compound Name	Response	Retention Time
DDT	345831	20.56
DDD	1511	20.13
DDE	451	19.64
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1962	347793	0.56

Instrument :
BNA_P
ClientSampleId :
DFTPP