
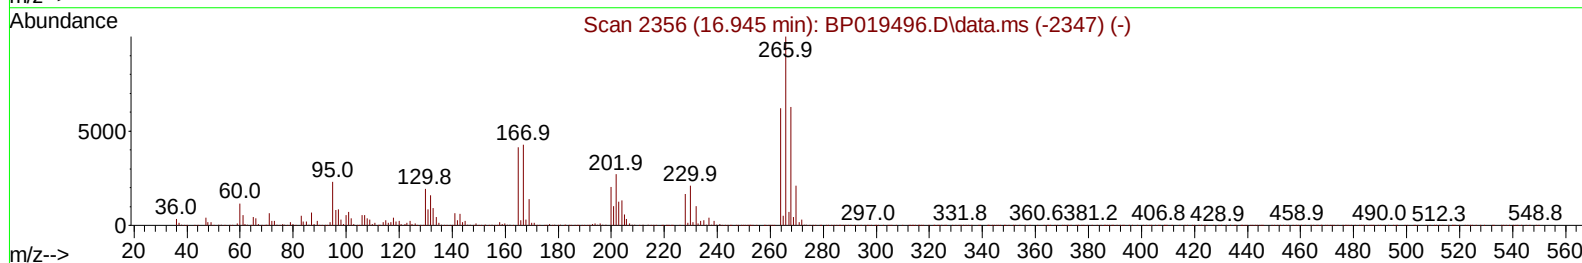
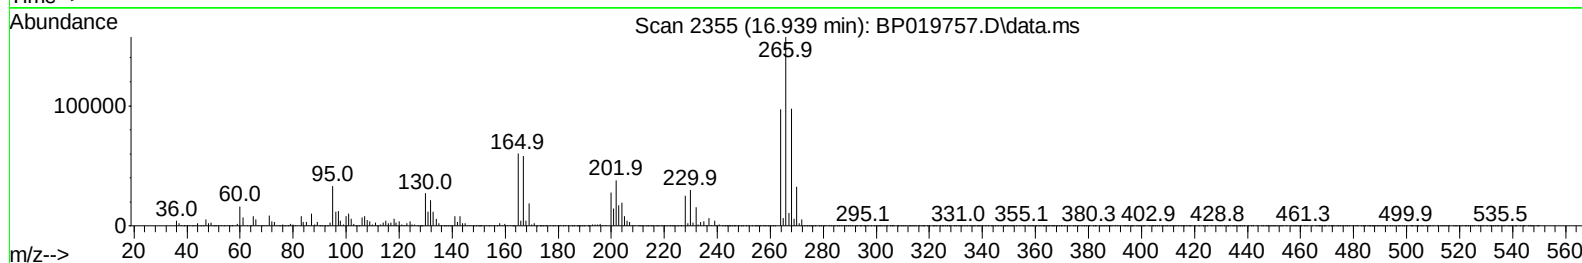


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP021924\  
Data File : BP019757.D  
Acq On : 19 Feb 2024 10:24  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 20 00:28:14 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP013124.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Feb 19 23:35:42 2024  
Response via : Initial Calibration

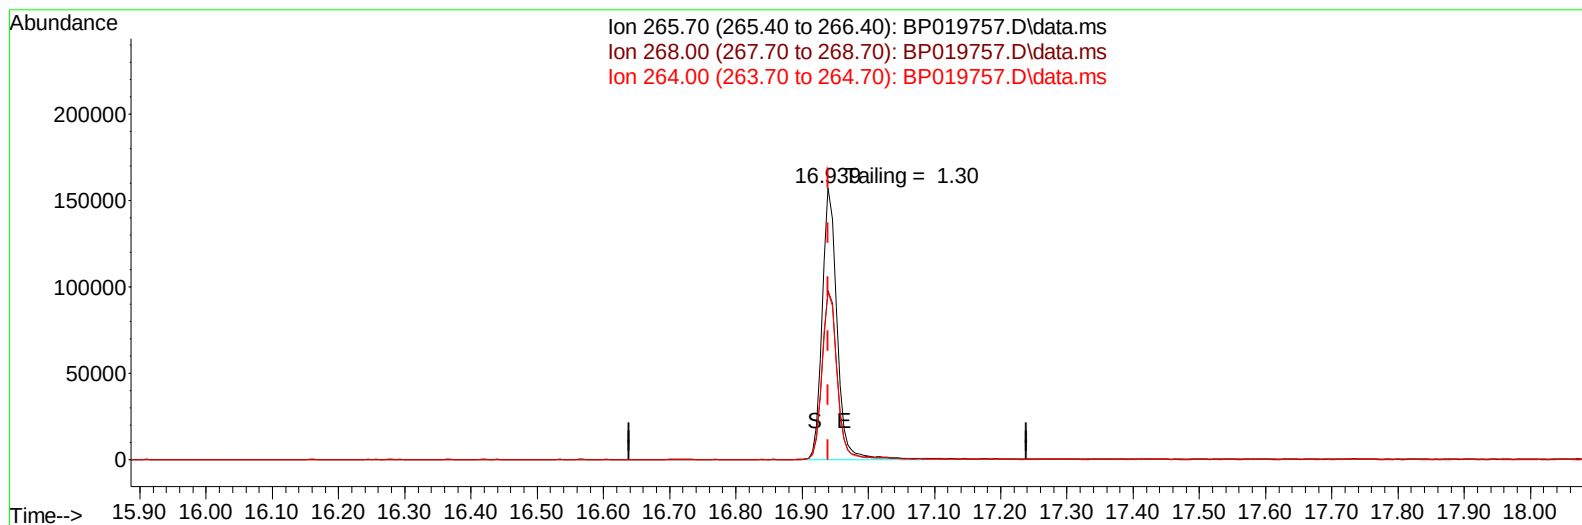

TIC: BP019757.D\data.ms

**(70) Pentachlorophenol (C)**




**16.939min (+ 0.000) 129804.61 ng**

**response 240736**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.90  | 62.19  |
| 264.00 | 62.10  | 61.79  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP021924\  
Data File : BP019757.D  
Acq On : 19 Feb 2024 10:24  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 20 00:28:14 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP013124.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Feb 19 23:35:42 2024  
Response via : Initial Calibration

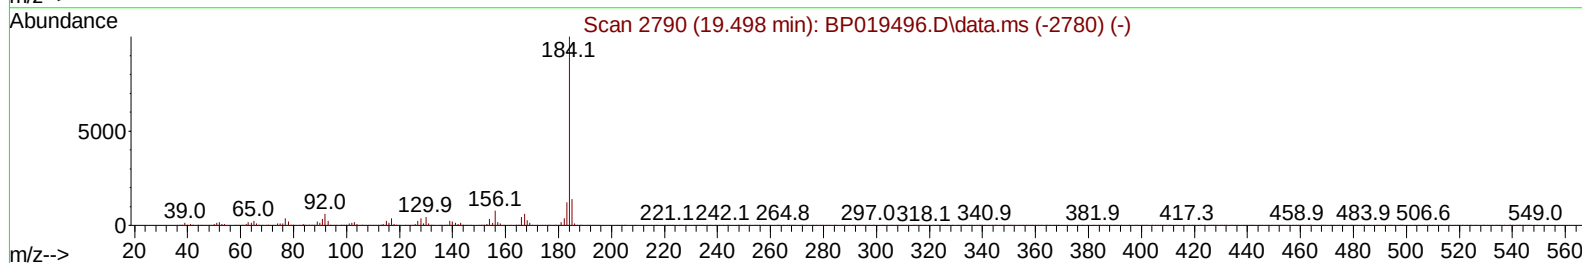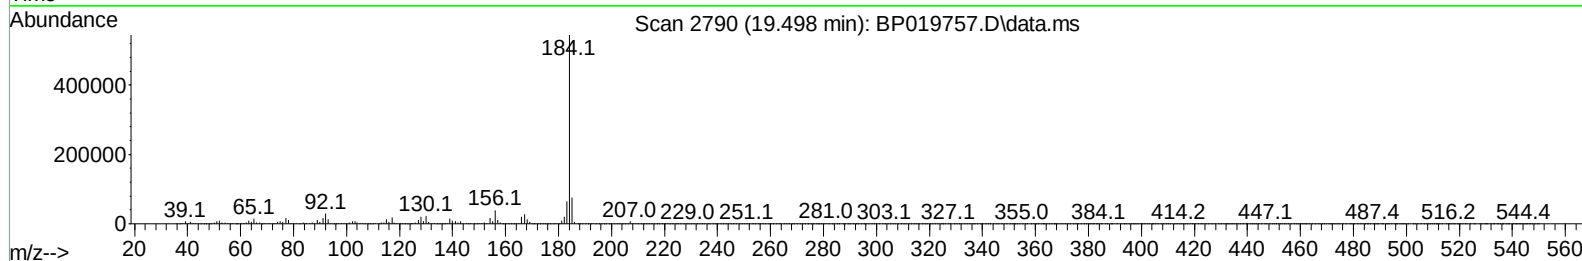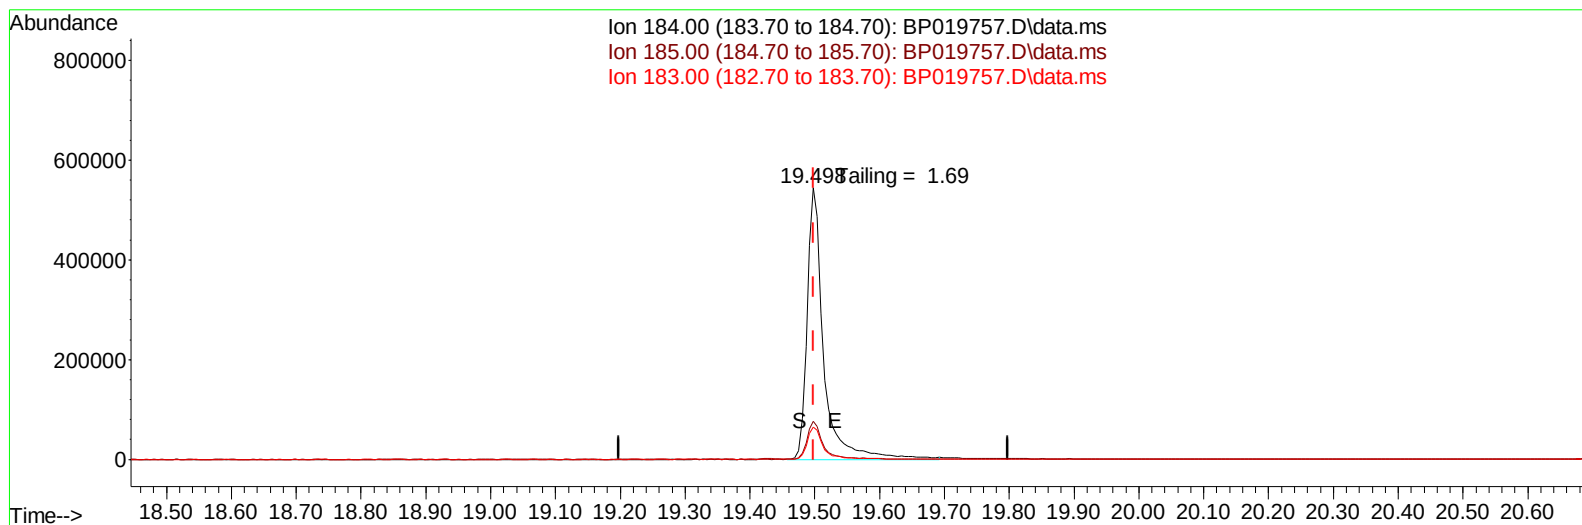

TIC: BP019757.D\data.ms

**(77) Benzidine**

**19.498min (+ 0.000) 34669.41 ng**

**response 977785**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.90  | 13.96  |
| 183.00 | 12.10  | 11.87  |
| 0.00   | 0.00   | 0.00   |