

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021924\
 Data File : BP019759.D
 Acq On : 19 Feb 2024 12:50
 Operator : MA/JU
 Sample : PB159072BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB159072BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP019759.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.017	323	328	335	rBV	40872	62490	1.11%	0.286%
2	5.475	398	406	420	rBV	1299687	1964142	34.99%	8.998%
3	7.069	670	677	690	rBV	1126276	1912563	34.07%	8.761%
4	7.899	811	818	828	rBV	267822	432152	7.70%	1.980%
5	9.069	1007	1017	1035	rBV	760667	1303175	23.21%	5.970%
6	10.699	1286	1294	1307	rBV	309400	552196	9.84%	2.530%
7	13.163	1703	1713	1742	rBV	1951142	3073474	54.75%	14.079%
8	14.534	1939	1946	1954	rBV	447350	717503	12.78%	3.287%
9	16.034	2192	2201	2230	rBV	1690317	2792313	49.74%	12.791%
10	17.292	2409	2415	2429	rBV	612479	972729	17.33%	4.456%
11	18.187	2563	2567	2576	rBV3	33138	61753	1.10%	0.283%
12	19.575	2799	2803	2810	rVB	62360	81182	1.45%	0.372%
13	19.863	2846	2852	2866	rBV	4370035	5613598	100.00%	25.716%
14	20.592	2973	2976	2982	rBV3	49521	69746	1.24%	0.320%
15	21.386	3106	3111	3121	rBV	799760	1161530	20.69%	5.321%
16	23.810	3517	3523	3533	rVB	465079	1059048	18.87%	4.851%




Sum of corrected areas: 21829594

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021924\
Data File : BP019759.D
Acq On : 19 Feb 2024 12:50
Operator : MA/JU
Sample : PB159072BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB159072BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

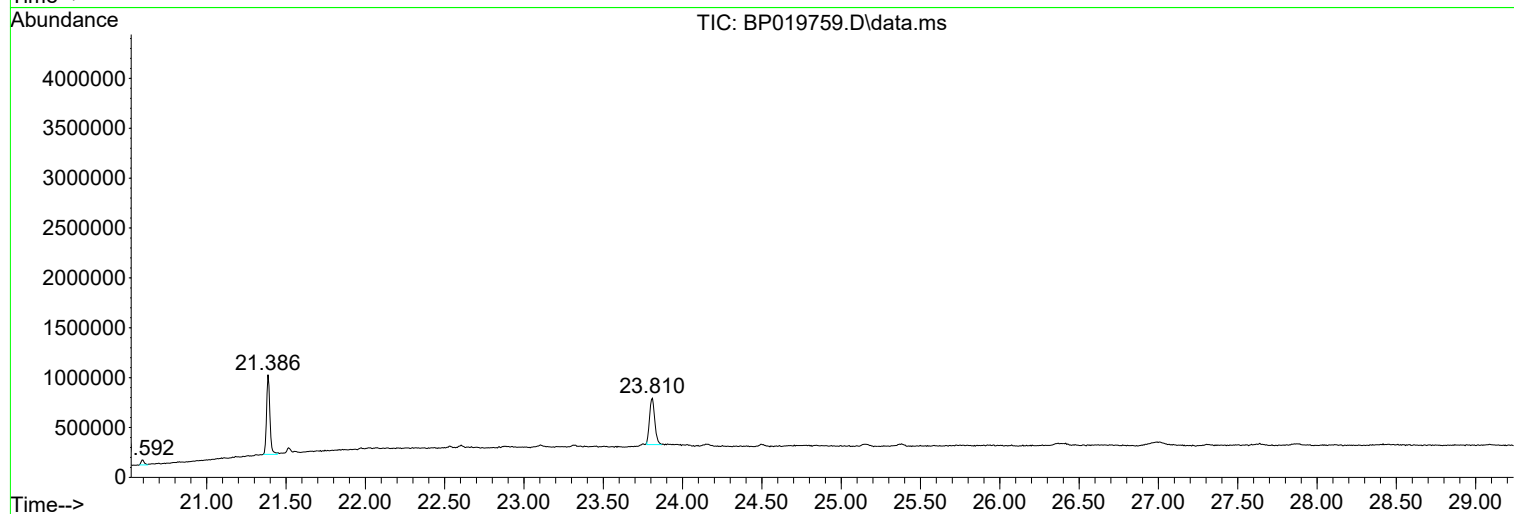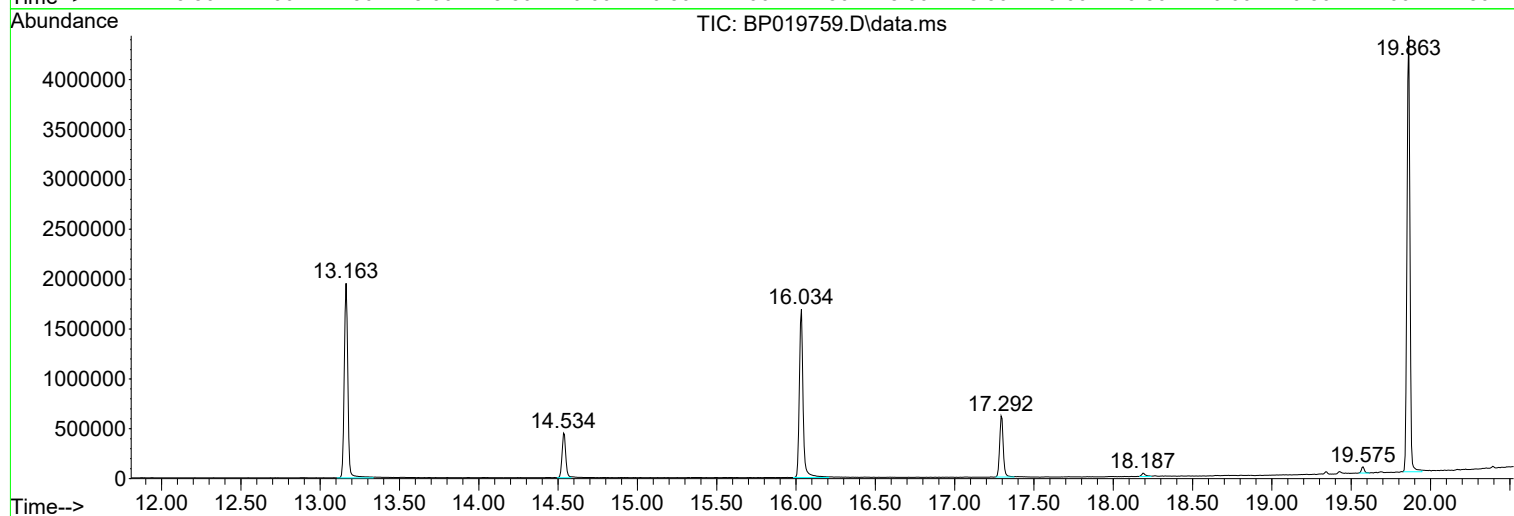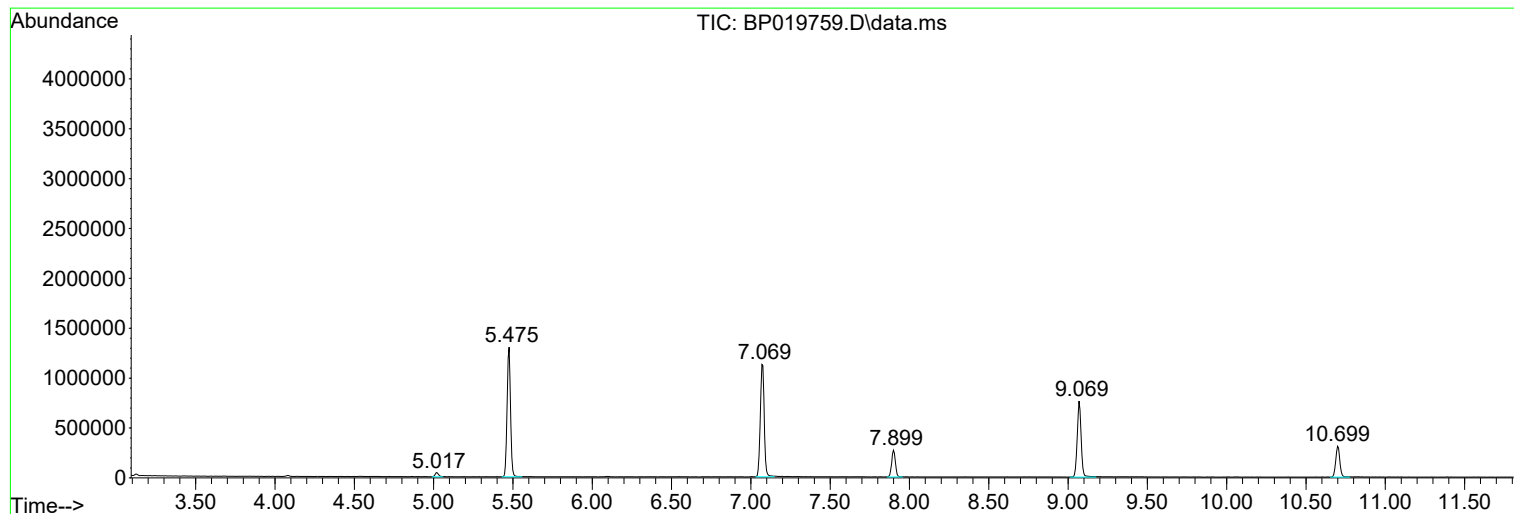

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021924\
Data File : BP019759.D
Acq On : 19 Feb 2024 12:50
Operator : MA/JU
Sample : PB159072BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB159072BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown5.017 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.017	2.89 ng	62490	1,4-Dichlorobenzene-d4	7.899

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Hydrazine, 1,1-bis(1-methylethyl)-	116	C6H16N2	000921-14-2	47
2			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	45
3			2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	35
4			Succinic acid, heptyl 2-methoxye...	274	C14H26O5	1000325-80-7	28
5			Silane, trimethyl-	74	C3H10Si	000993-07-7	17

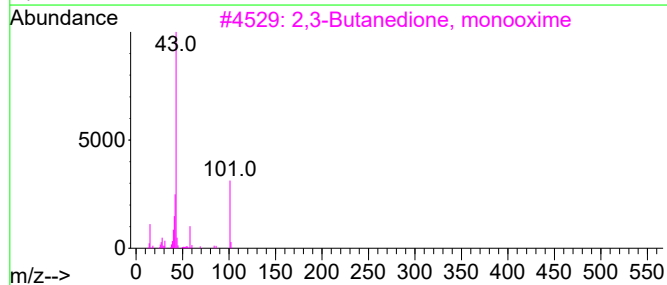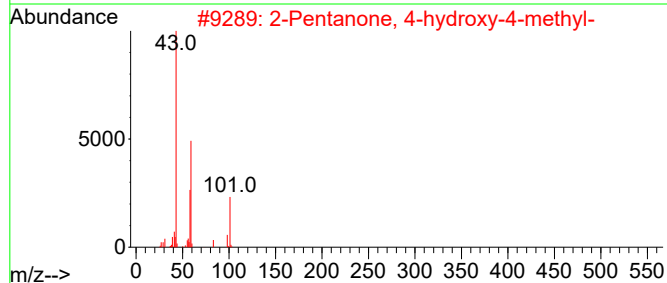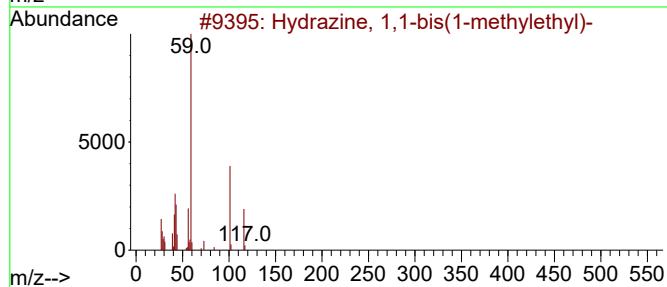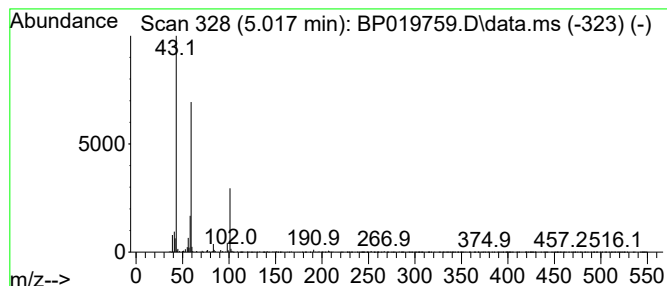

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021924\
Data File : BP019759.D
Acq On : 19 Feb 2024 12:50
Operator : MA/JU
Sample : PB159072BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB159072BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown5.017	5.017	2.9	ng	62490	1	7.899	432152	20.0