

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021924\
Data File : BP019761.D
Acq On : 19 Feb 2024 13:57
Operator : MA/JU
Sample : PB159068BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB159068BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP019761.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.475	399	406	415	rBV	1393980	2065293	34.22%	9.269%
2	7.075	670	678	692	rBV	1214286	2028290	33.61%	9.103%
3	7.899	811	818	826	rBV	274111	439815	7.29%	1.974%
4	9.069	1009	1017	1034	rBV	815057	1419238	23.52%	6.370%
5	10.699	1284	1294	1308	rBV	304965	555921	9.21%	2.495%
6	13.163	1704	1713	1728	rBV	2067741	3204996	53.11%	14.385%
7	14.534	1938	1946	1955	rBV	424556	710780	11.78%	3.190%
8	16.034	2193	2201	2228	rBV	1495610	2634441	43.65%	11.824%
9	17.292	2408	2415	2428	rBV	573415	942657	15.62%	4.231%
10	19.857	2845	2851	2867	rBV	4505610	6035160	100.00%	27.087%
11	21.386	3106	3111	3123	rBV	784916	1152509	19.10%	5.173%
12	23.810	3516	3523	3536	rVB	480316	1091525	18.09%	4.899%




Sum of corrected areas: 22280625

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021924\
Data File : BP019761.D
Acq On : 19 Feb 2024 13:57
Operator : MA/JU
Sample : PB159068BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB159068BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

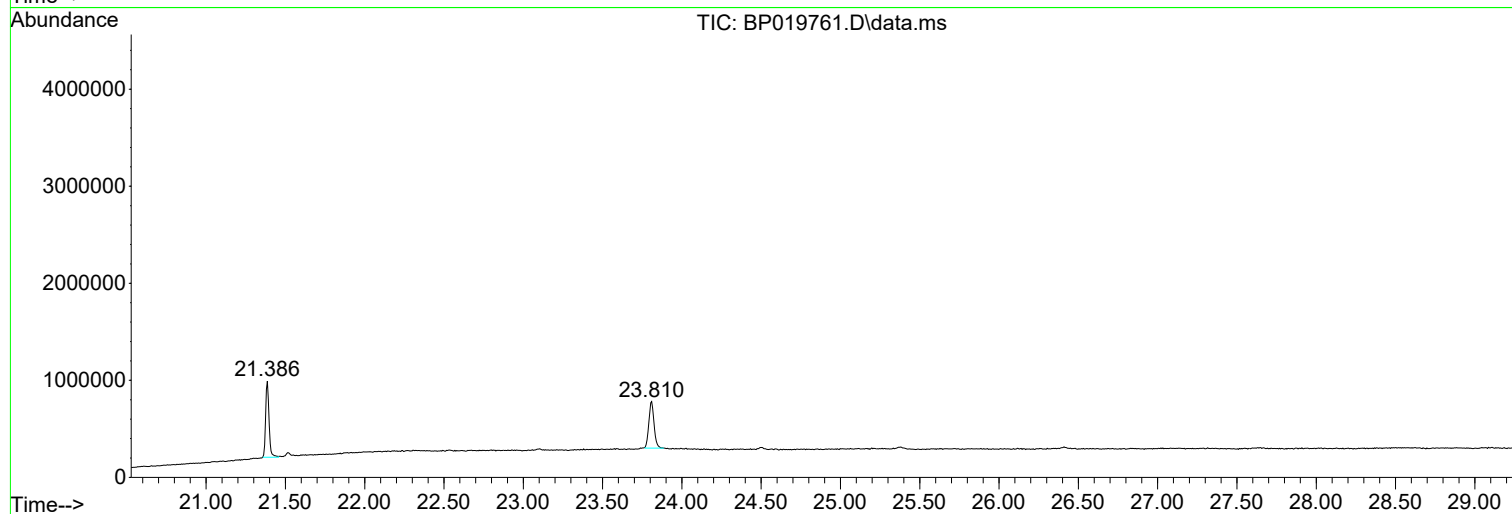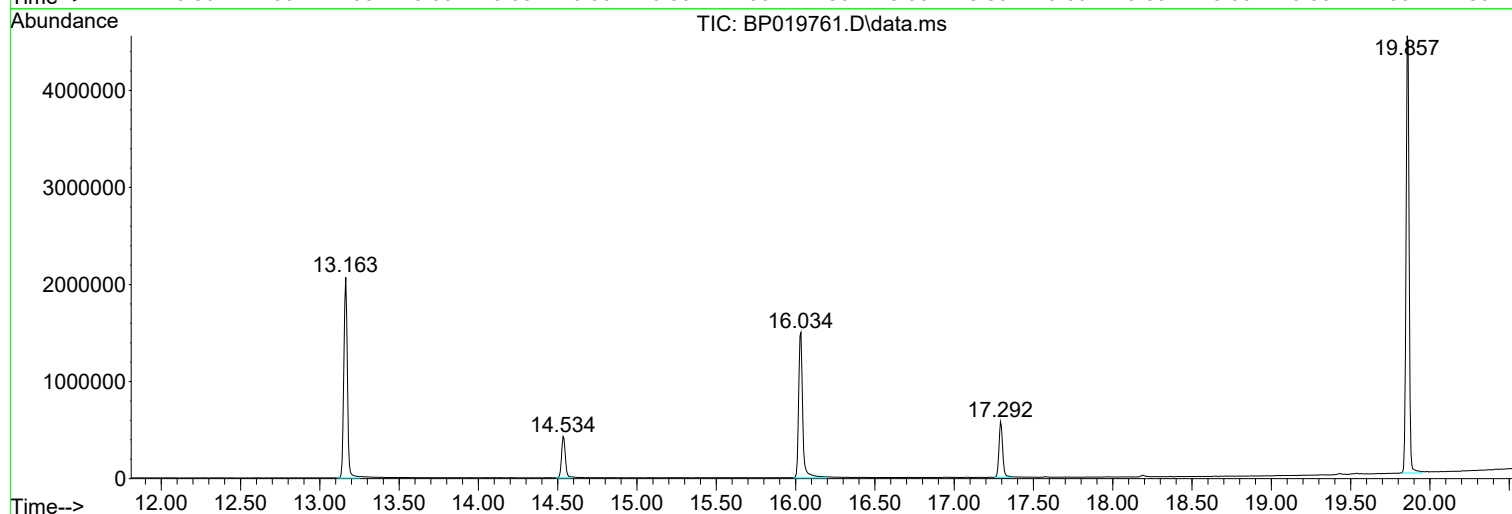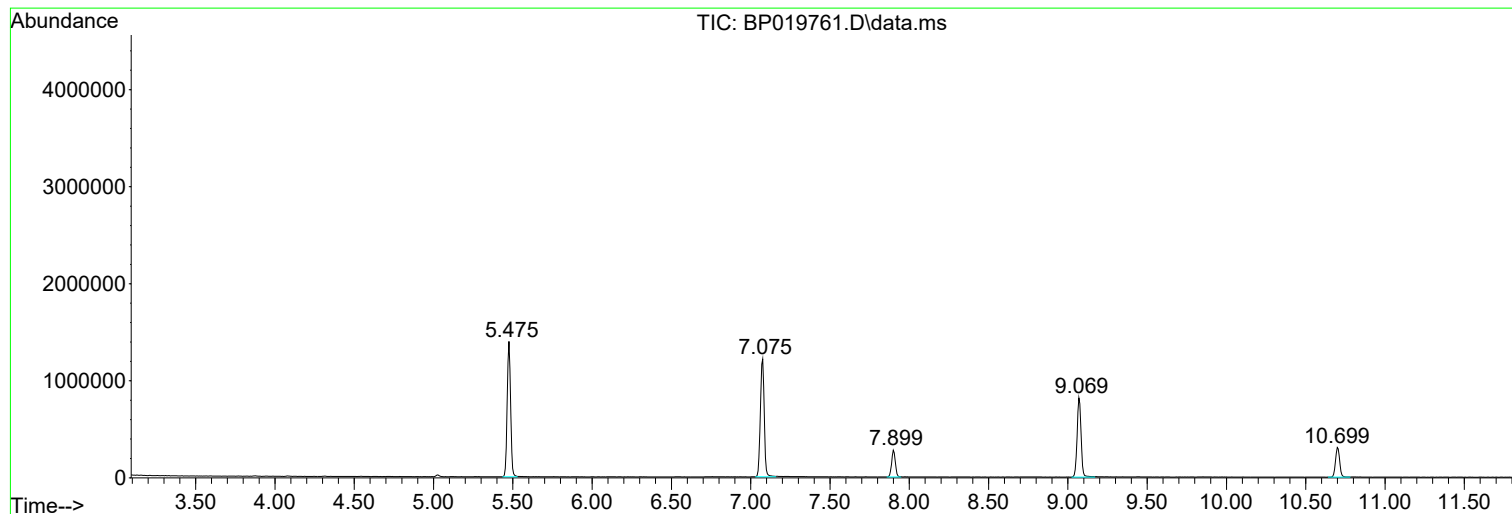

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021924\
Data File : BP019761.D
Acq On : 19 Feb 2024 13:57
Operator : MA/JU
Sample : PB159068BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB159068BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021924\
Data File : BP019761.D
Acq On : 19 Feb 2024 13:57
Operator : MA/JU
Sample : PB159068BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB159068BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------