


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021924\
Data File : BP019757.D
Acq On : 19 Feb 2024 10:24
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Feb 19 23:35:42 2024

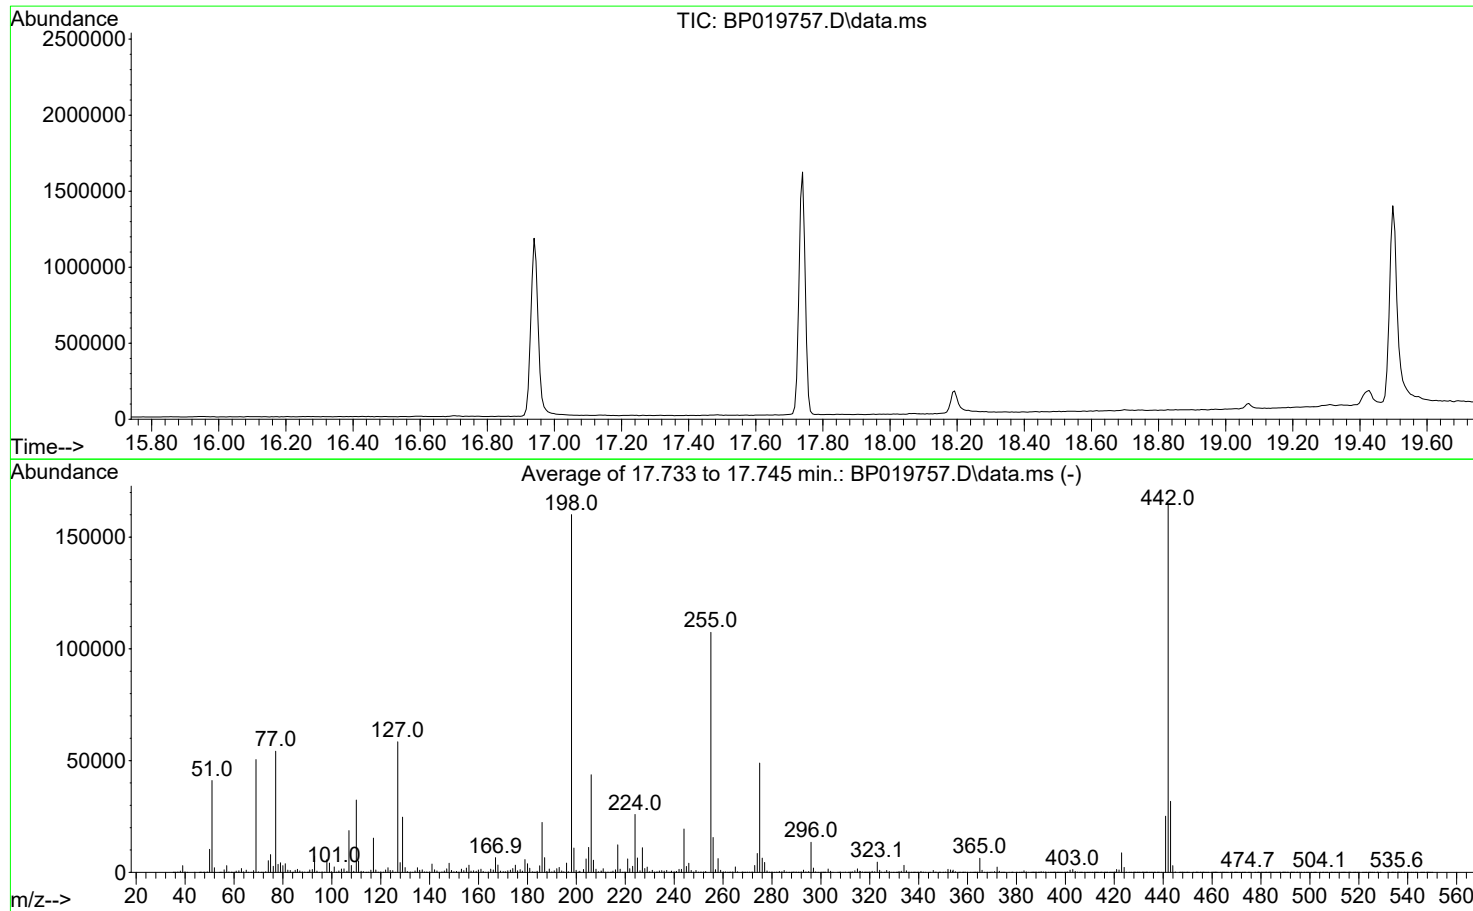




AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.7	41121	PASS
68	69	0.00	2	1.6	795	PASS
69	198	0.00	100	31.5	50467	PASS
70	69	0.00	2	0.4	217	PASS
127	198	10	80	36.5	58449	PASS
197	198	0.00	2	0.2	258	PASS
198	198	100	100	100.0	160092	PASS
199	198	5	9	6.8	10920	PASS
275	198	10	60	30.5	48875	PASS
365	198	1	100	3.9	6274	PASS
441	198	0.01	100	15.7	25149	PASS
442	442	100	100	100.0	164605	PASS
443	442	15	24	19.3	31784	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021924\
Data File : BP019757.D
Acq On : 19 Feb 2024 10:24
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 20 00:28:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 19 23:35:42 2024
Response via : Initial Calibration

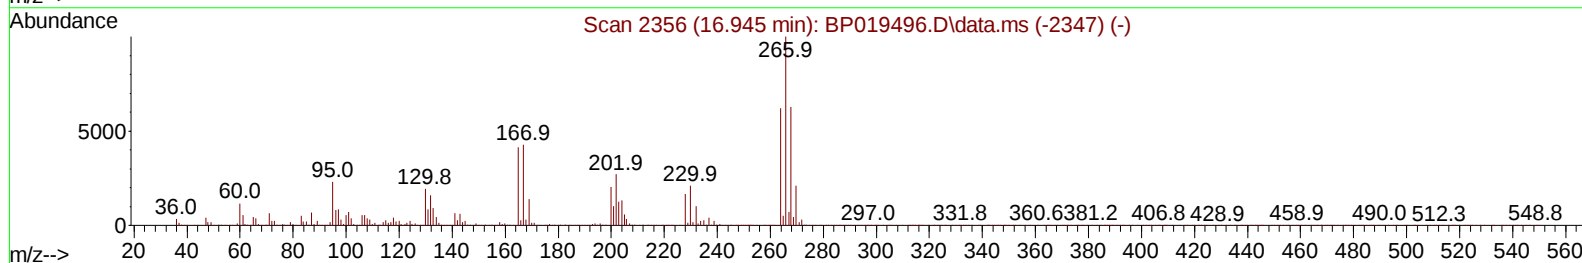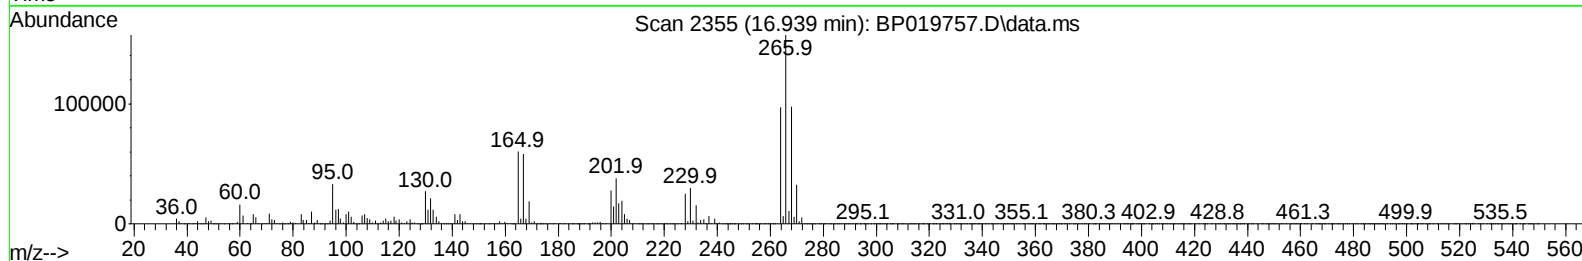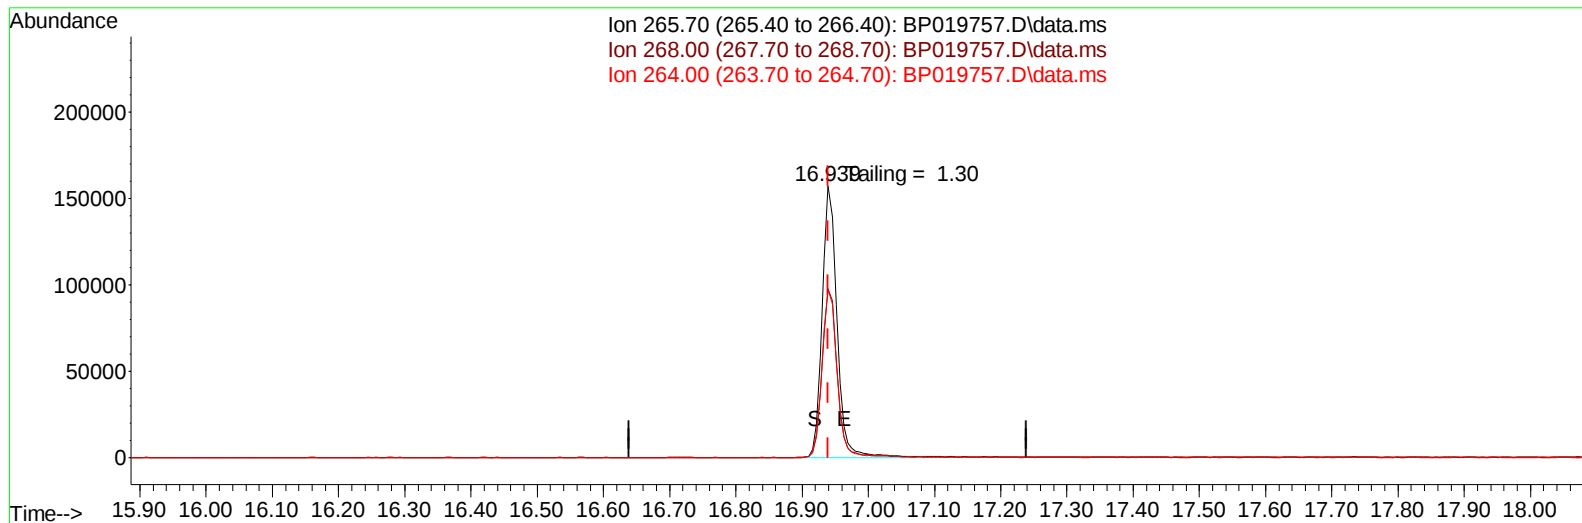

TIC: BP019757.D\data.ms

(70) Pentachlorophenol (C)

16.939min (+ 0.000) 129804.61 ng




response 240736

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	62.19
264.00	62.10	61.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021924\
Data File : BP019757.D
Acq On : 19 Feb 2024 10:24
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 20 00:28:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 19 23:35:42 2024
Response via : Initial Calibration

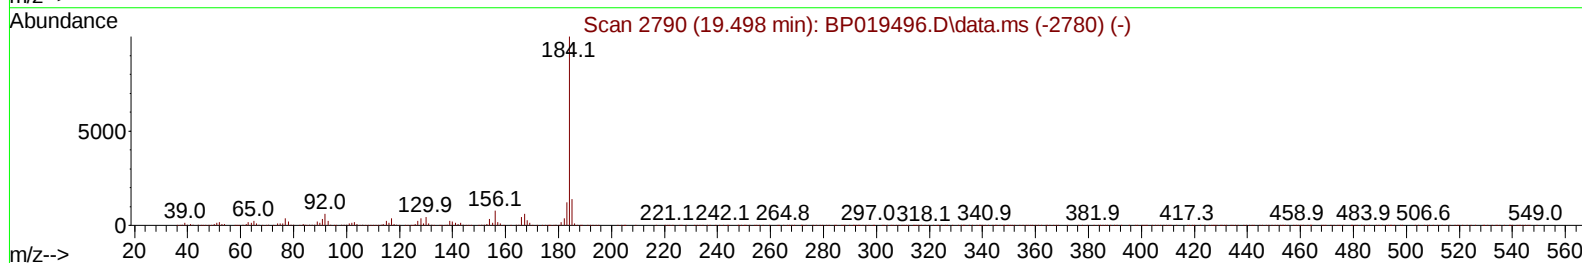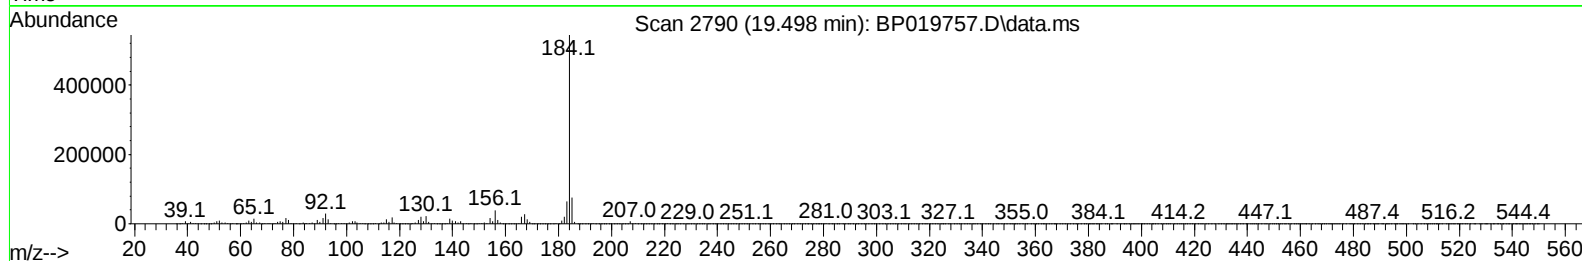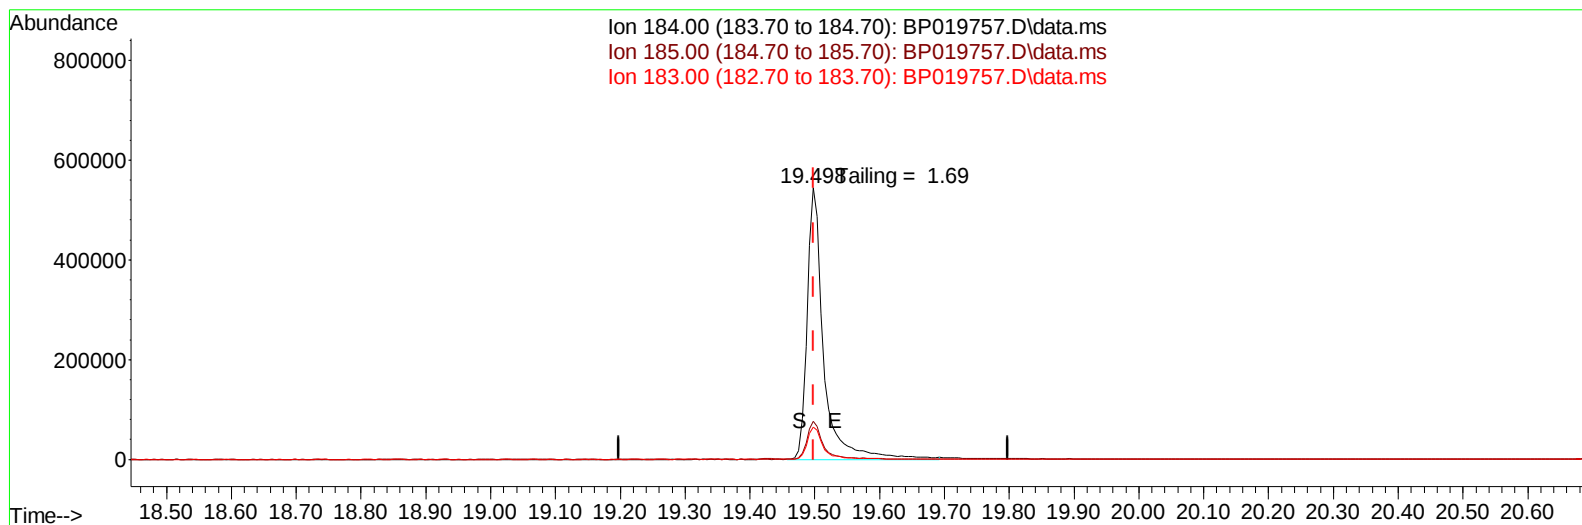

TIC: BP019757.D\data.ms

(77) Benzidine

19.498min (+ 0.000) 34669.41 ng

response 977785

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.96
183.00	12.10	11.87
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/19/2024	BNA_P	<u>BP019757.D</u>
Compound Name	Response	Retention Time
DDT	587658	22.692
DDD	22320	20.269
DDE	1890	19.763
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24210	611868	3.96

Instrument :
BNA_P
ClientSampleId :
DFTPP