
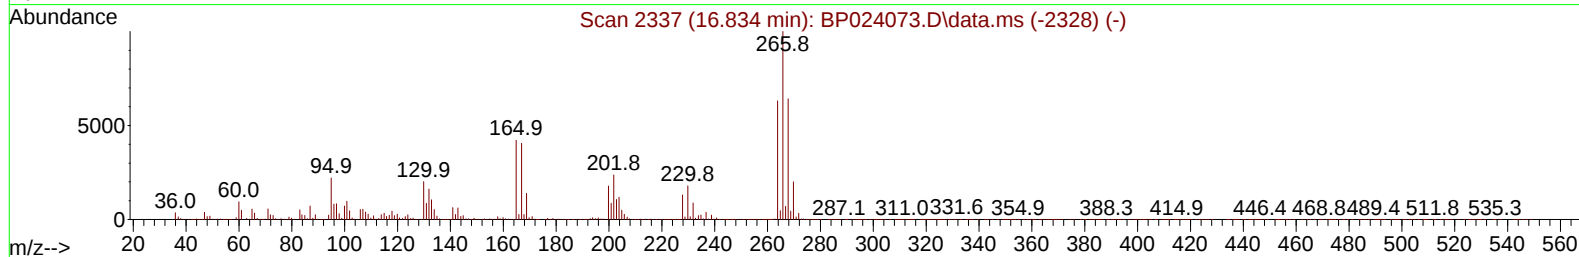
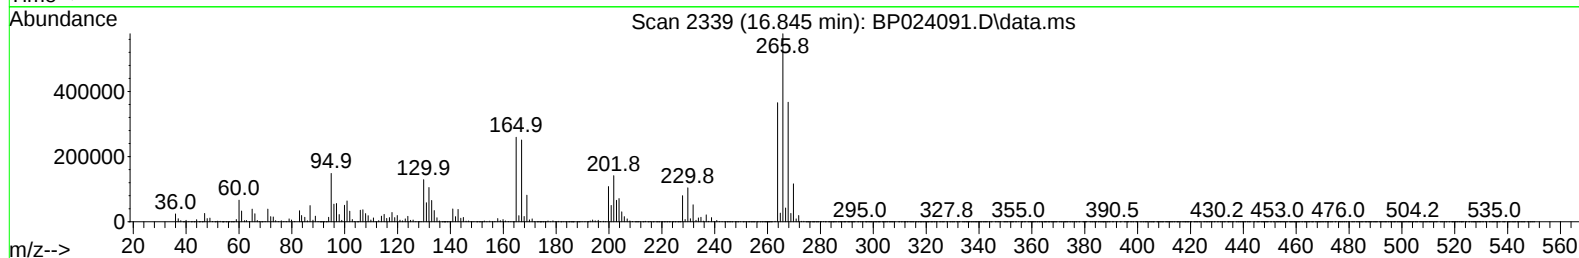


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021925\
Data File : BP024091.D
Acq On : 19 Feb 2025 09:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 19 10:37:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 18 02:25:07 2025
Response via : Initial Calibration

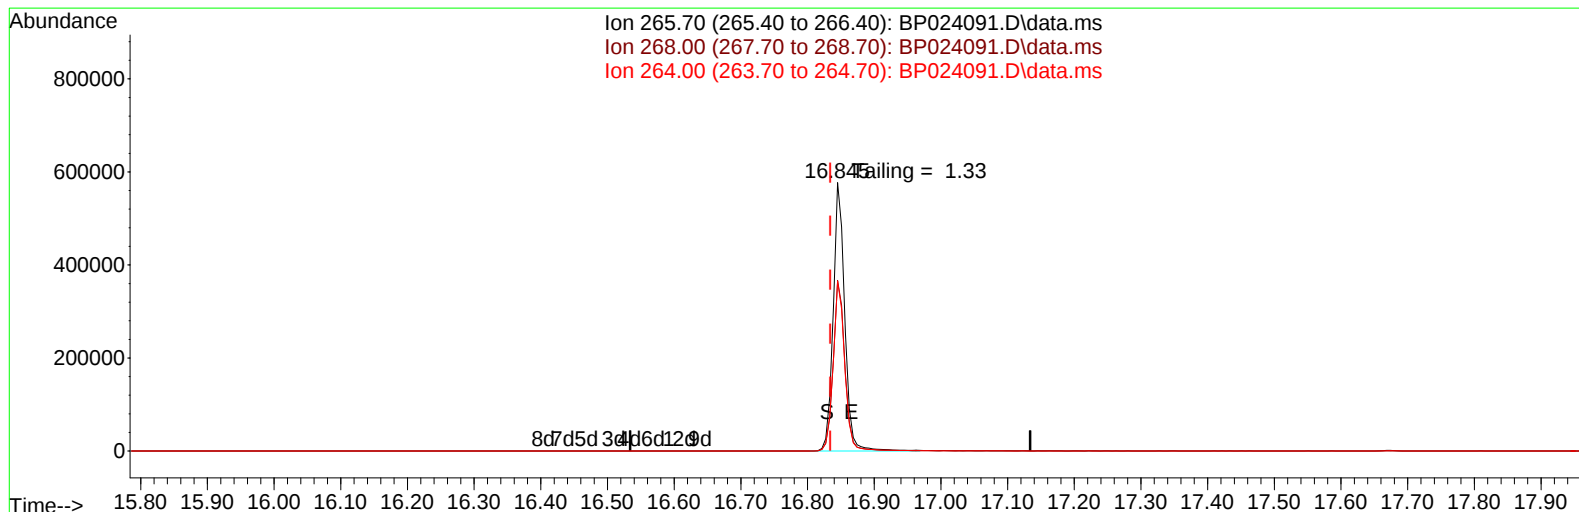

TIC: BP024091.D\data.ms

(70) Pentachlorophenol (C)




16.845min (+ 0.011) 178595.77 ng m

response 692785

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	63.59
264.00	63.10	63.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021925\
Data File : BP024091.D
Acq On : 19 Feb 2025 09:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 19 10:37:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 18 02:25:07 2025
Response via : Initial Calibration

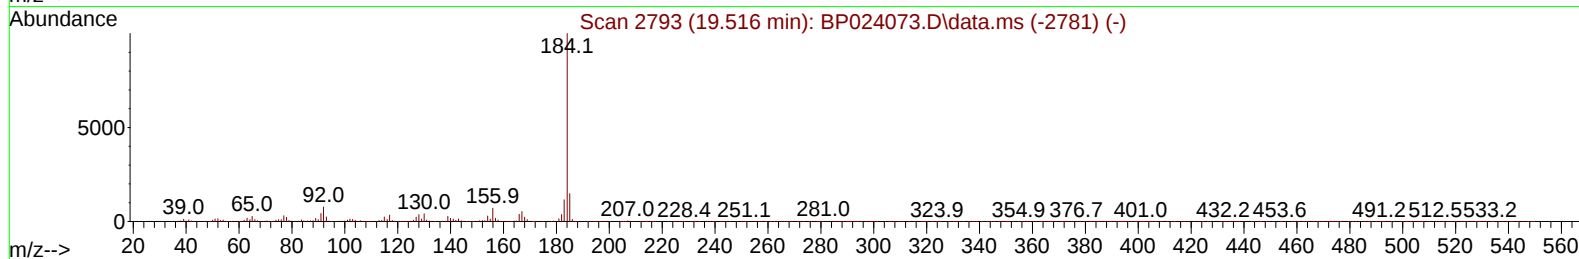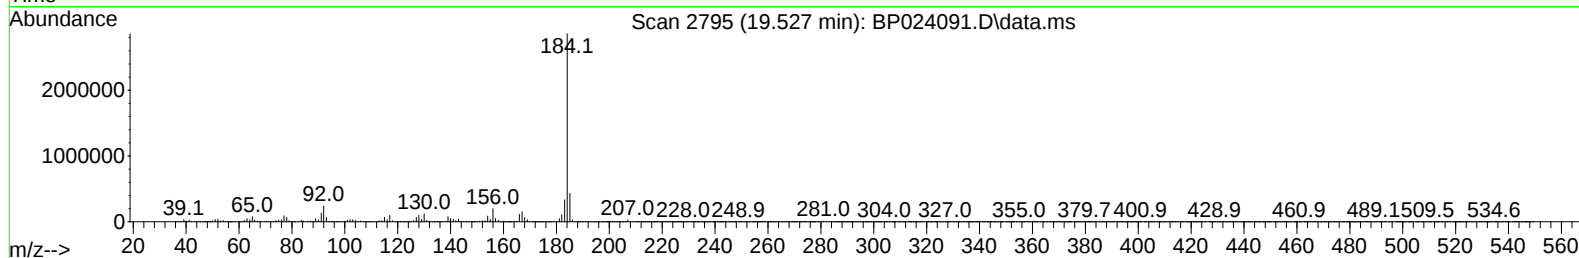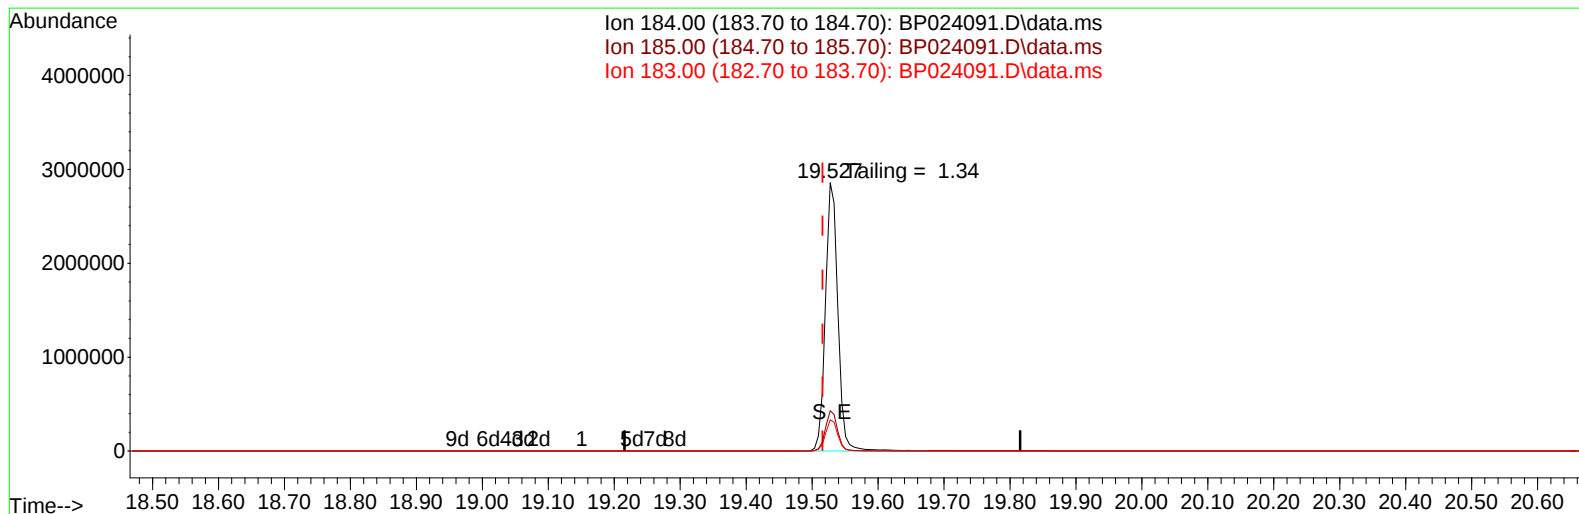

TIC: BP024091.D\data.ms

(77) Benzidine

19.527min (+ 0.011) 11418388.63 ng m

response 3756766

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	15.07
183.00	11.60	11.62
0.00	0.00	0.00