

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021925\
Data File : BP024093.D
Acq On : 19 Feb 2025 10:32
Operator : RC/JU
Sample : PB166339BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB166339BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP024093.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.358	380	386	405	rBV	7471676	10312793	49.42%	10.960%
2	6.922	643	652	673	rBV	6621747	10095226	48.38%	10.728%
3	7.746	783	792	801	rBV	1561869	2415984	11.58%	2.567%
4	8.893	978	987	1003	rBV	3968596	6443801	30.88%	6.848%
5	10.522	1254	1264	1281	rBV	1831882	3183910	15.26%	3.384%
6	12.987	1675	1683	1700	rBV	10177382	14655718	70.23%	15.575%
7	14.375	1912	1919	1930	rBV	2414704	3746724	17.95%	3.982%
8	15.893	2170	2177	2203	rBV	7247766	9432731	45.20%	10.024%
9	17.187	2389	2397	2408	rBV	2877455	4147871	19.88%	4.408%
10	19.910	2854	2860	2872	rBV	17663879	20868151	100.00%	22.177%
11	21.639	3148	3154	3168	rVB	2946877	4401035	21.09%	4.677%
12	25.021	3720	3729	3744	rVB	1720906	4394907	21.06%	4.671%




Sum of corrected areas: 94098851

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021925\
Data File : BP024093.D
Acq On : 19 Feb 2025 10:32
Operator : RC/JU
Sample : PB166339BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB166339BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

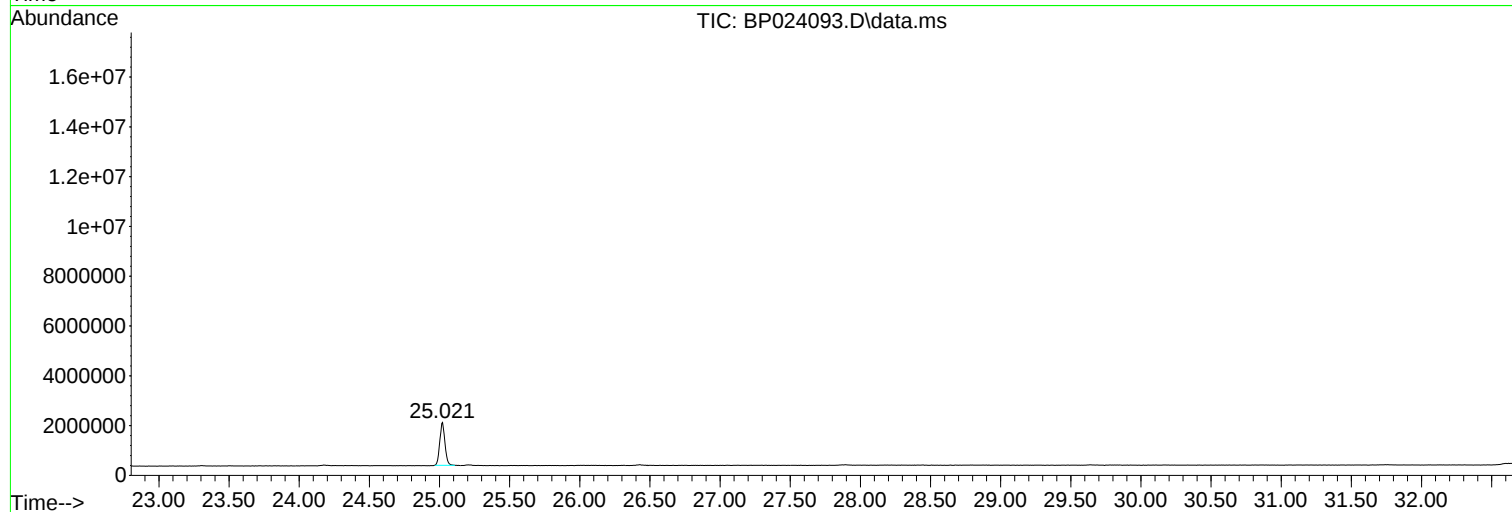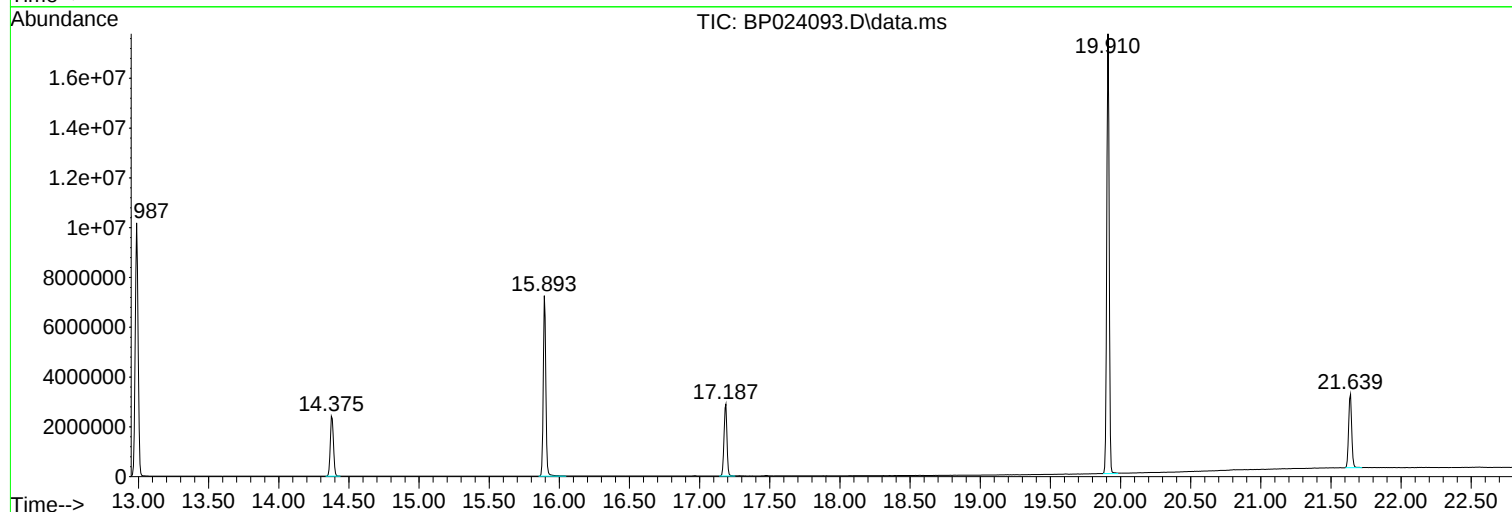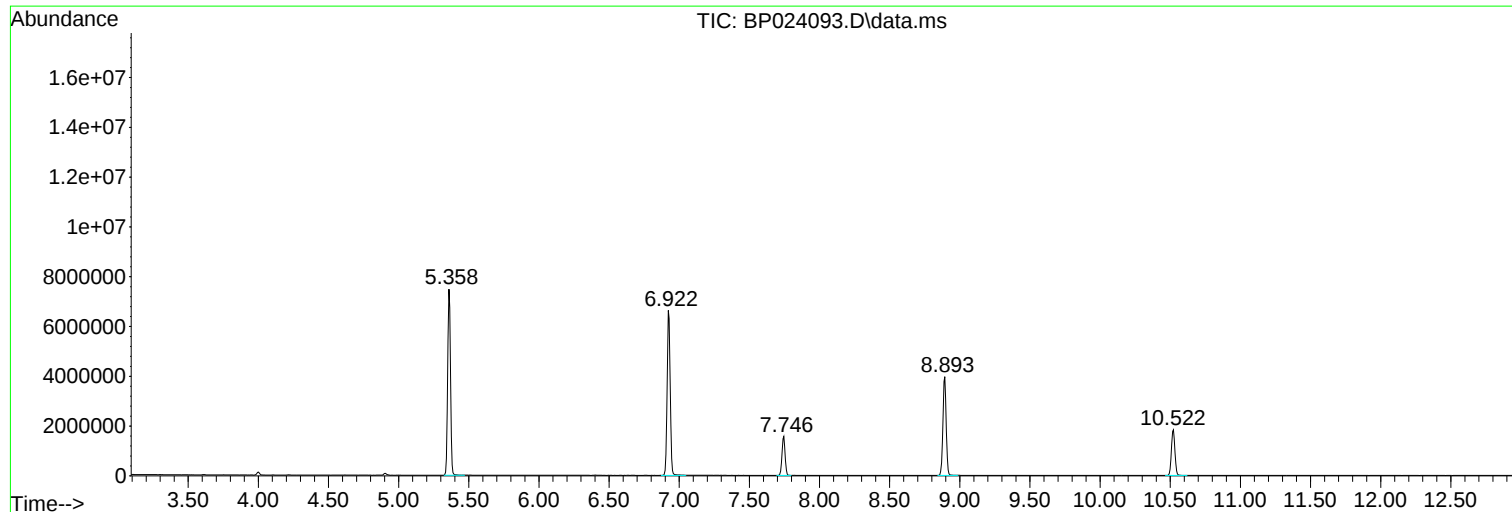

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021925\
Data File : BP024093.D
Acq On : 19 Feb 2025 10:32
Operator : RC/JU
Sample : PB166339BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB166339BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021925\
Data File : BP024093.D
Acq On : 19 Feb 2025 10:32
Operator : RC/JU
Sample : PB166339BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB166339BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------