
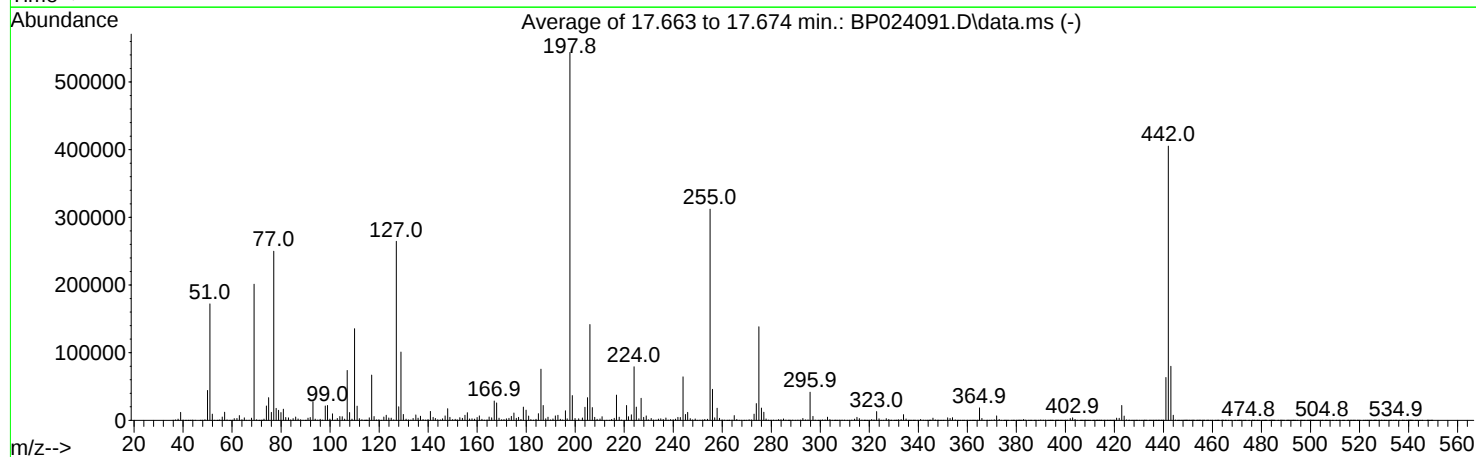


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021925\
Data File : BP024091.D
Acq On : 19 Feb 2025 09:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Feb 18 02:25:07 2025

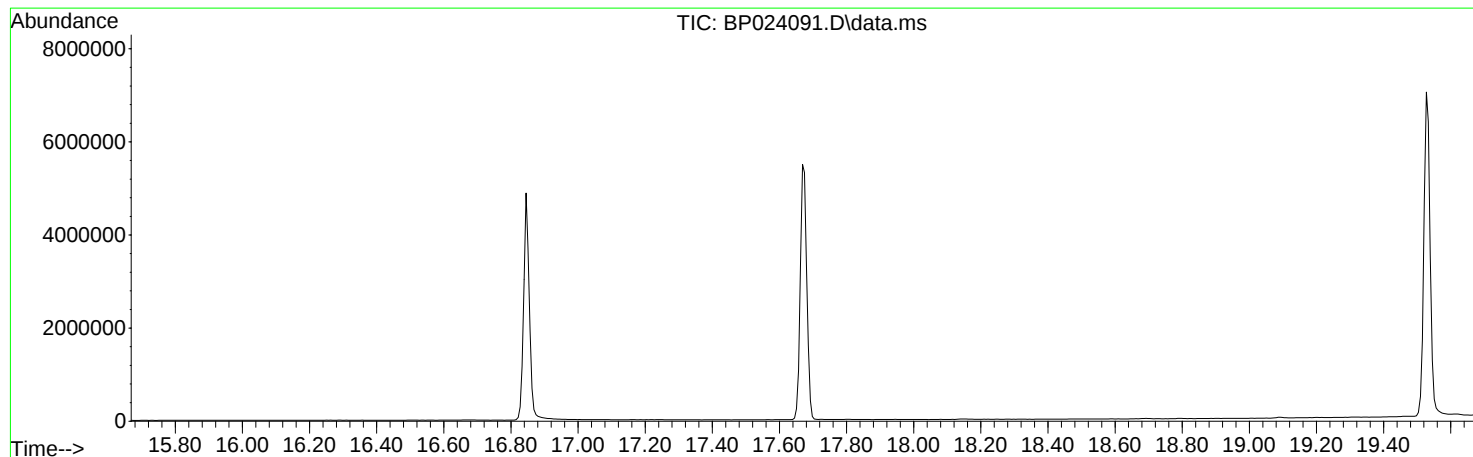

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.7	172152	PASS
68	69	0.00	2	1.7	3323	PASS
69	198	0.00	100	37.0	201329	PASS
70	69	0.00	2	0.5	1084	PASS
127	198	10	80	48.7	264545	PASS
197	198	0.00	2	0.4	2310	PASS
198	198	100	100	100.0	543574	PASS
199	198	5	9	6.7	36642	PASS
275	198	10	60	25.5	138435	PASS
365	198	1	100	3.4	18382	PASS
441	198	0.01	100	11.7	63347	PASS
442	442	100	100	100.0	405227	PASS
443	442	15	24	19.7	79930	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/19/2025	BNA_P	<u>BP024091.D</u>
Compound Name	Response	Retention Time
DDT	1883483	20.821
DDD	18354	20.41
DDE	628	19.833
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18982	1902465	1.00

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021925\
Data File : BP024091.D
Acq On : 19 Feb 2025 09:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 19 10:37:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 18 02:25:07 2025
Response via : Initial Calibration

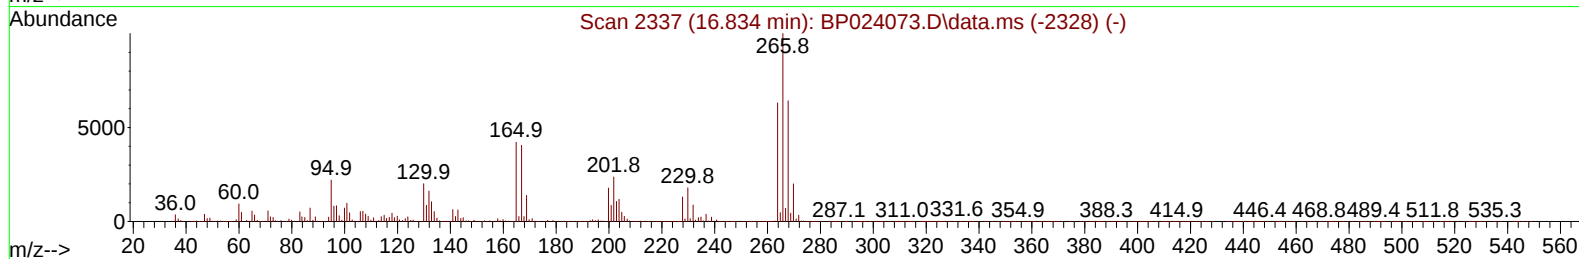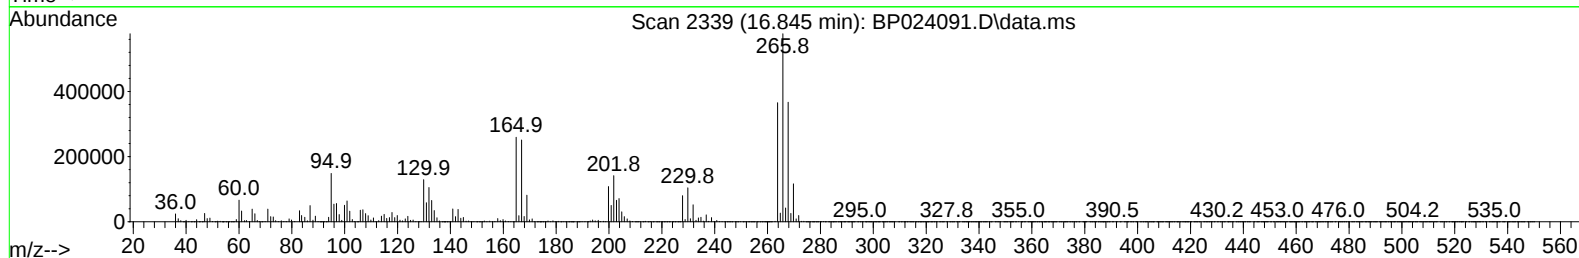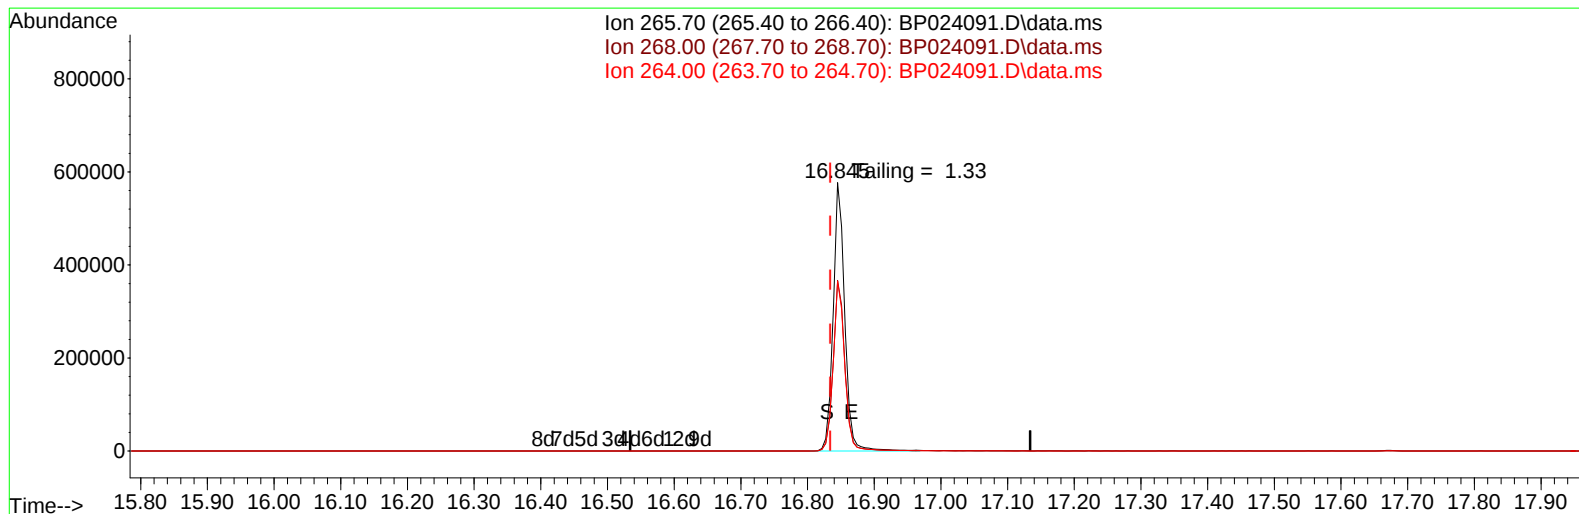

TIC: BP024091.D\data.ms

(70) Pentachlorophenol (C)

16.845min (+ 0.011) 178595.77 ng m




response 692785

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	63.59
264.00	63.10	63.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021925\
Data File : BP024091.D
Acq On : 19 Feb 2025 09:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 19 10:37:31 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 18 02:25:07 2025
Response via : Initial Calibration

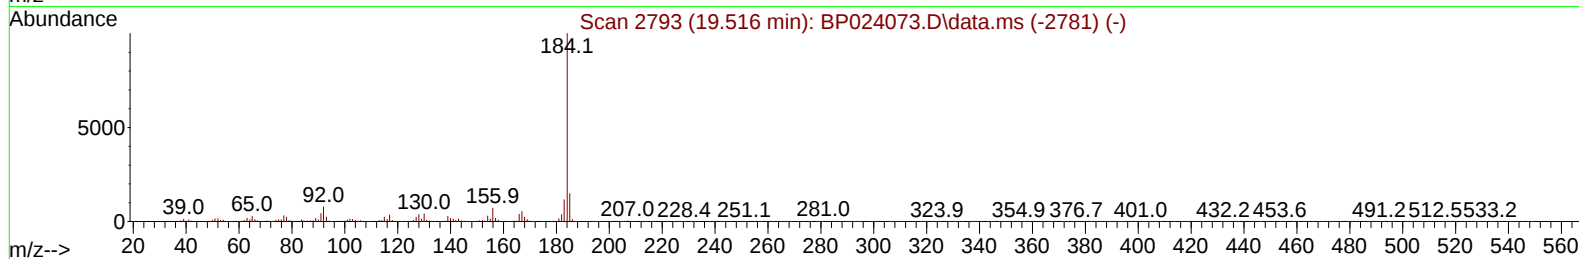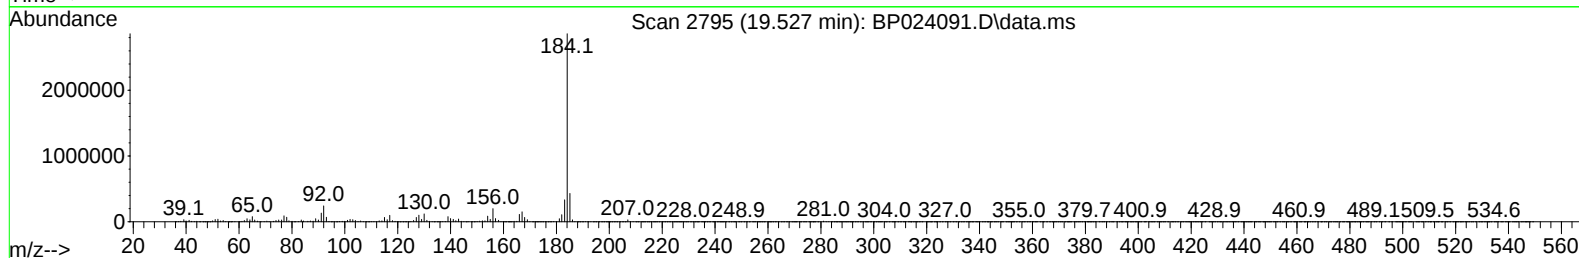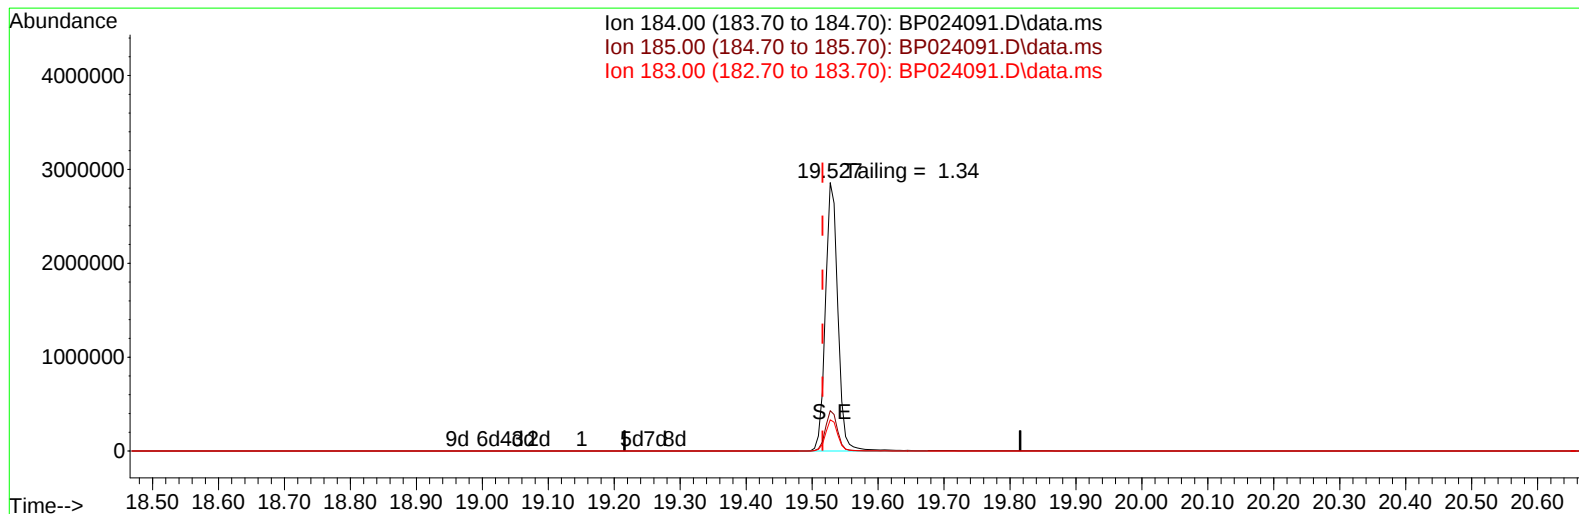

TIC: BP024091.D\data.ms

(77) Benzidine

19.527min (+ 0.011) 11418388.63 ng m

response 3756766

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	15.07
183.00	11.60	11.62
0.00	0.00	0.00