

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022020\
 Data File : BP001798.D
 Acq On : 20 Feb 2020 12:48
 Operator : CG/JU
 Sample : L1418-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C5AT2

Quant Time: Feb 21 06:39:54 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 21 06:37:37 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	353880	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	1470448	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	899788	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.05	188	1947395	20.00	ng/ul	0.00
78) Chrysene-d12	21.13	240	2018520	20.00	ng/ul	0.00
86) Perylene-d12	23.35	264	2166161	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.18	96	40913	4.80	ng/uL	0.00
5) Phenol-d5	6.83	99	717351	26.83	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	434213	27.95	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	634073	29.34	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	558206	26.32	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	292033	29.34	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	292499	32.49	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	595670	27.83	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	633111	25.00	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	1753583	27.77	ng/ul	0.00
47) Acenaphthylene-d8	13.98	160	2227229	28.65	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	222461	20.23	ng/ul	0.00
58) Fluorene-d10	15.29	176	1625168	28.62	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	128085	16.68	ng/ul	0.00
71) Anthracene-d10	17.14	188	2410342	28.10	ng/ul	0.00
79) Pyrene-d10	19.39	212	2753089	26.58	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.21	264	2930025	28.01	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.75	163	226158	3.403	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP022020\
Data File : BP001798.D
Acq On : 20 Feb 2020 12:48
Operator : CG/JU
Sample : L1418-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C5AT2

Quant Time: Feb 21 06:39:54 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 21 06:37:37 2020
Response via : Initial Calibration

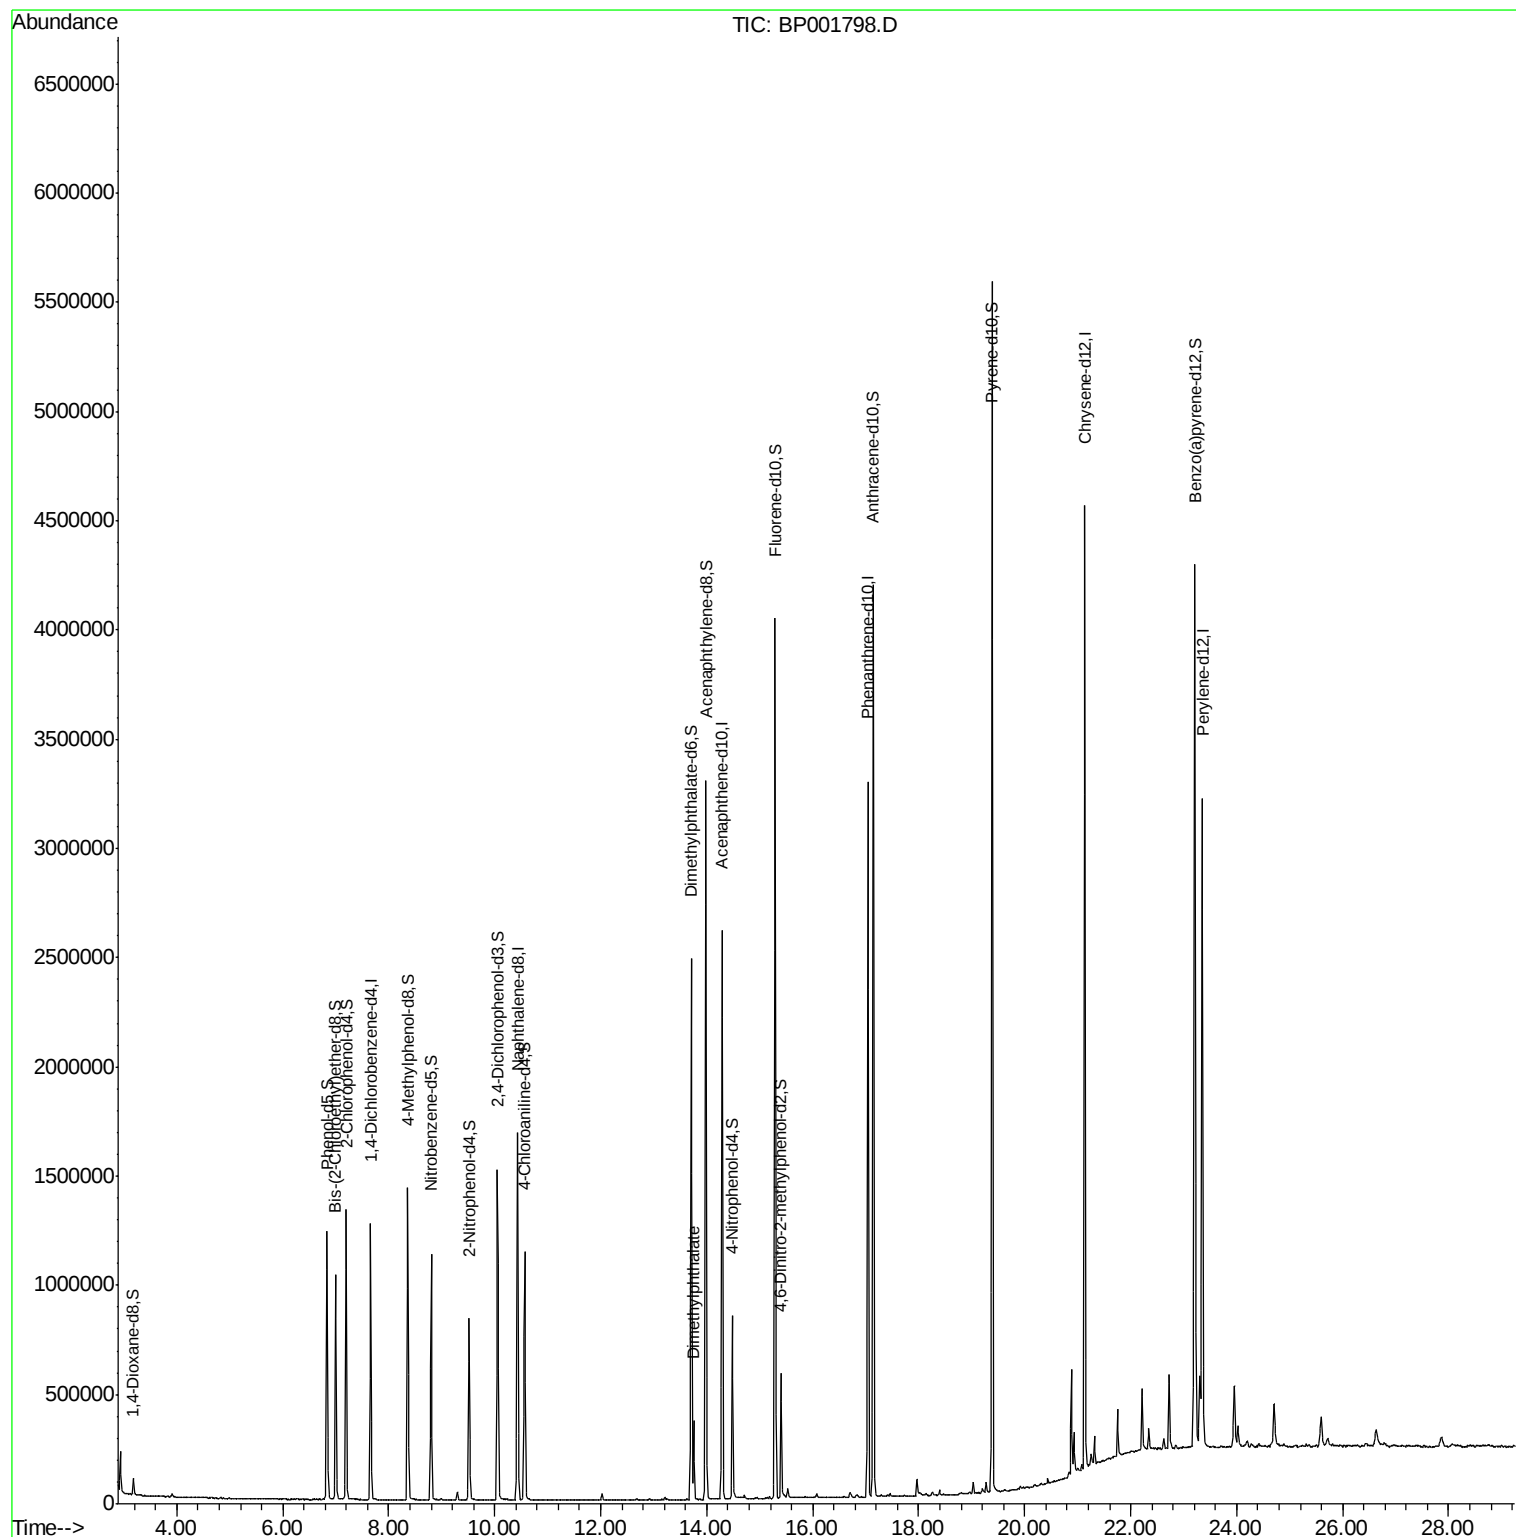

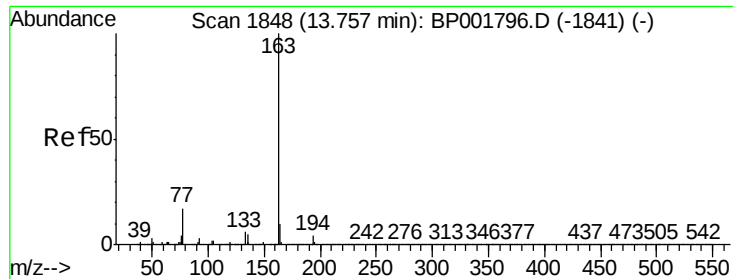

#45

Dimethylphthalate

Concen: 3.403 ng/ul

RT: 13.75 min Scan# 1847

Delta R.T. -0.01 min

Lab File: BP001798.D

Acq: 20 Feb 2020 12:48

Instrument :

BNA_P

ClientSampleId :

C5AT2


Tot Ion:163 Resp: 226158

Ion Ratio Lower Upper

163 100

194 4.3 3.5 5.3

164 10.7 8.0 12.0

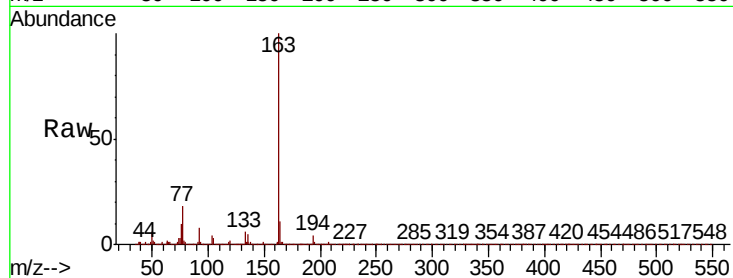

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

