

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022020\
 Data File : BP001800.D
 Acq On : 20 Feb 2020 13:55
 Operator : CG/JU
 Sample : L1418-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C5AT4

Quant Time: Feb 21 06:54:06 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 21 06:37:37 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	374825	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	1553066	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	948084	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.05	188	2068322	20.00	ng/ul	0.00
78) Chrysene-d12	21.13	240	2130077	20.00	ng/ul	0.00
86) Perylene-d12	23.35	264	2262741	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.18	96	21469	2.38	ng/uL	0.00
5) Phenol-d5	6.83	99	407492	14.39	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	264956	16.10	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	370546	16.19	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	238817	10.63	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	176283	16.77	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	158312	16.65	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	336203	14.87	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	125171	4.68	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	1071393	16.10	ng/ul	0.00
47) Acenaphthylene-d8	13.98	160	1385545	16.91	ng/ul	0.00
52) 4-Nitrophenol-d4	14.48	143	87939	7.59	ng/ul	0.00
58) Fluorene-d10	15.29	176	1032417	17.26	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	58611	7.19	ng/ul	0.00
71) Anthracene-d10	17.14	188	1599026	17.55	ng/ul	0.00
79) Pyrene-d10	19.39	212	1920357	17.57	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.21	264	1990082	18.21	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.75	163	131298	1.875	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP022020\
Data File : BP001800.D
Acq On : 20 Feb 2020 13:55
Operator : CG/JU
Sample : L1418-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C5AT4

Quant Time: Feb 21 06:54:06 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 21 06:37:37 2020
Response via : Initial Calibration

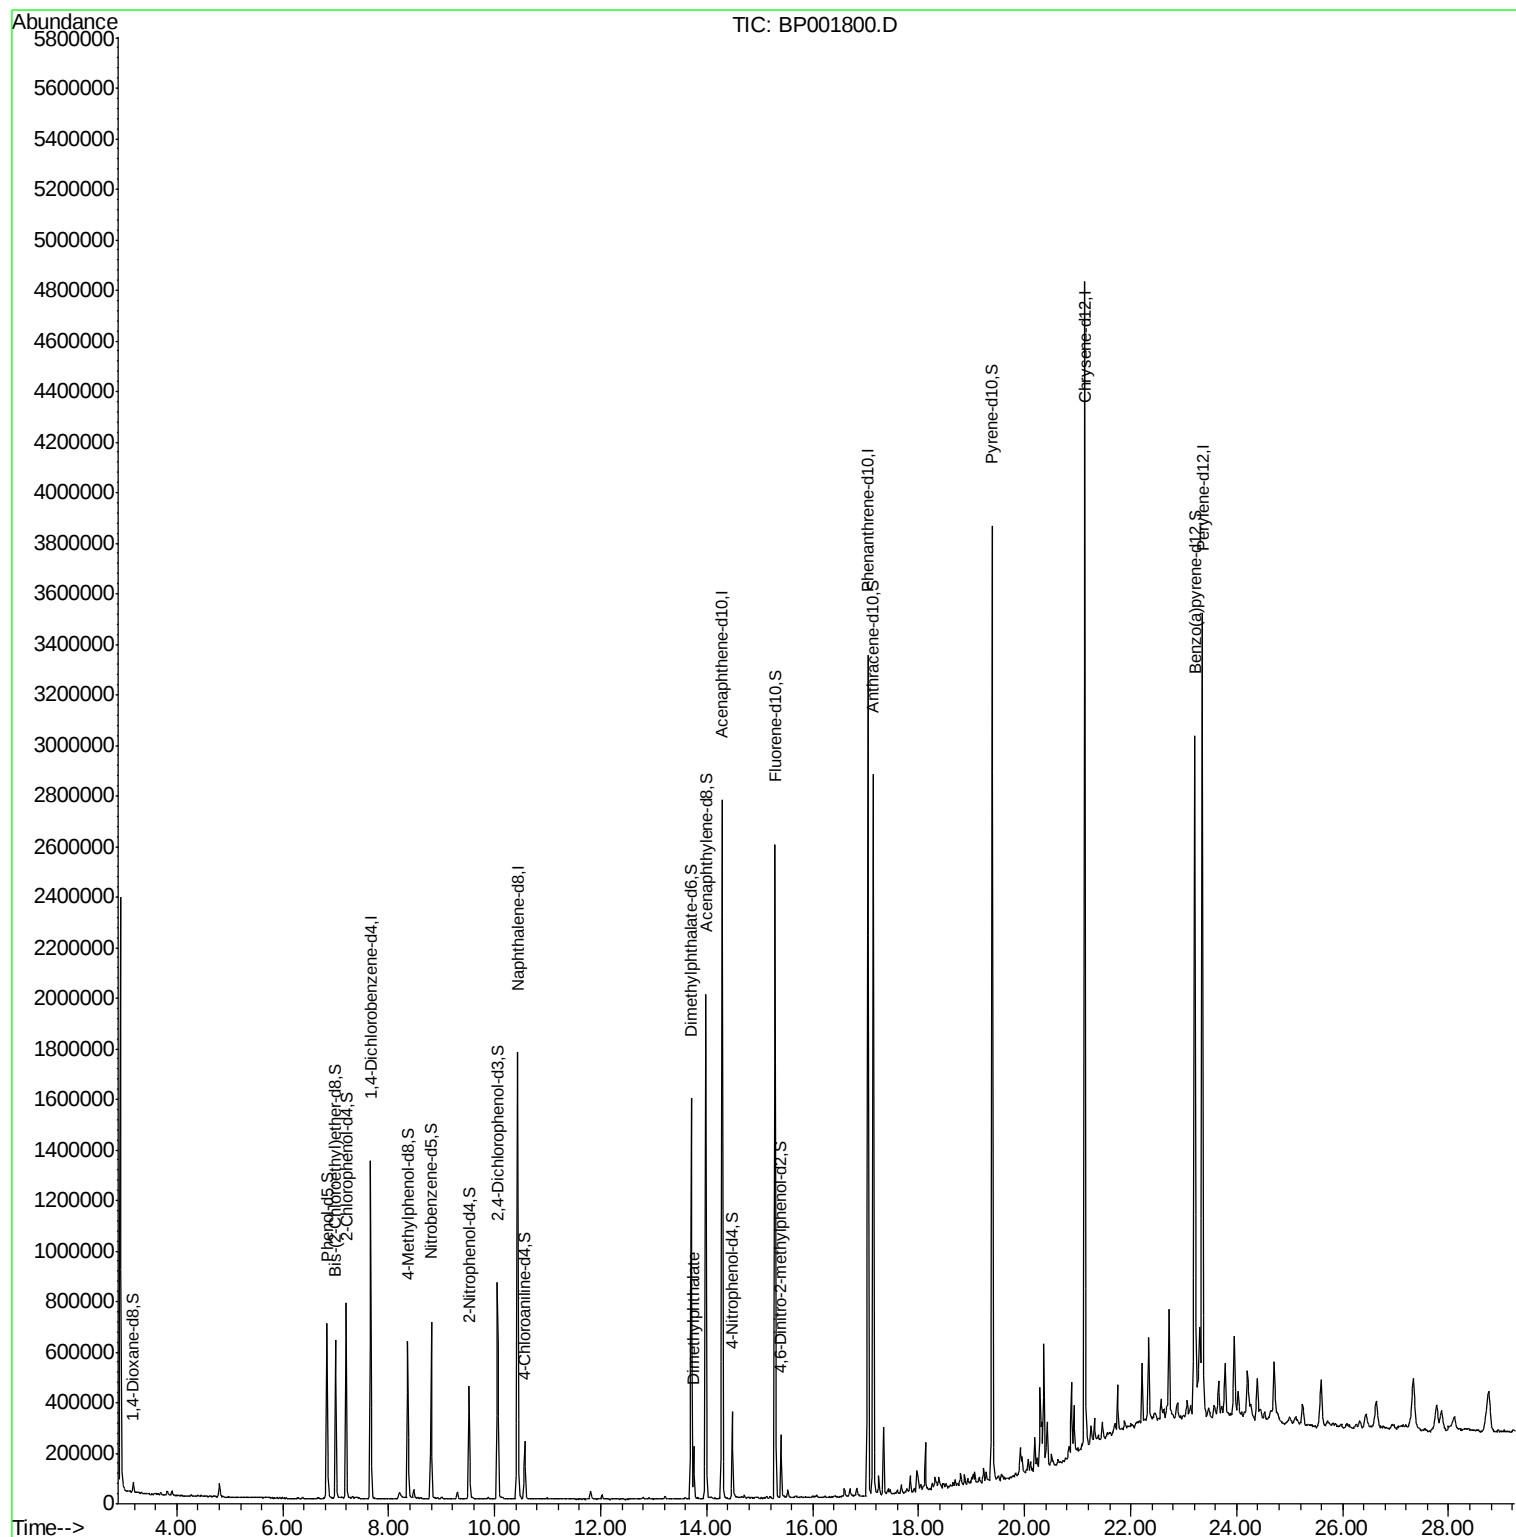

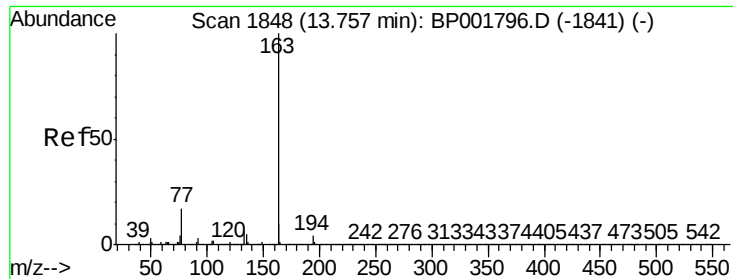

#45

Dimethylphthalate

Concen: 1.875 ng/ul

RT: 13.75 min Scan# 1847

Delta R.T. -0.01 min

Lab File: BP001800.D

Acq: 20 Feb 2020 13:55

Instrument :

BNA_P

ClientSampleId :

C5AT4

Tot Ion:163 Resp: 131298

Ion Ratio Lower Upper

163 100

194 4.6 3.5 5.3

164 10.6 8.0 12.0

