

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022020\
 Data File : BP001801.D
 Acq On : 20 Feb 2020 14:29
 Operator : CG/JU
 Sample : L1418-09
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C5AT8

Quant Time: Feb 21 06:40:23 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 21 06:37:37 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	376789	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	1556398	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	956774	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	2106370	20.00	ng/ul	0.00
78) Chrysene-d12	21.13	240	2213598	20.00	ng/ul	0.00
86) Perylene-d12	23.35	264	2376302	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.18	96	23133	2.55	ng/uL	0.00
5) Phenol-d5	6.83	99	409522	14.38	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	249407	15.08	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	360517	15.67	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	282645	12.52	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	161863	15.36	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	155151	16.28	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	332443	14.67	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	464014	17.31	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	1057583	15.75	ng/ul	0.00
47) Acenaphthylene-d8	13.98	160	1283138	15.52	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	118870	10.17	ng/ul	0.00
58) Fluorene-d10	15.29	176	973309	16.12	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	71212	8.58	ng/ul	0.00
71) Anthracene-d10	17.14	188	1488384	16.04	ng/ul	0.00
79) Pyrene-d10	19.39	212	1841002	16.21	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.21	264	2009496	17.51	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.75	163	170157	2.408	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP022020\
Data File : BP001801.D
Acq On : 20 Feb 2020 14:29
Operator : CG/JU
Sample : L1418-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C5AT8

Quant Time: Feb 21 06:40:23 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 21 06:37:37 2020
Response via : Initial Calibration

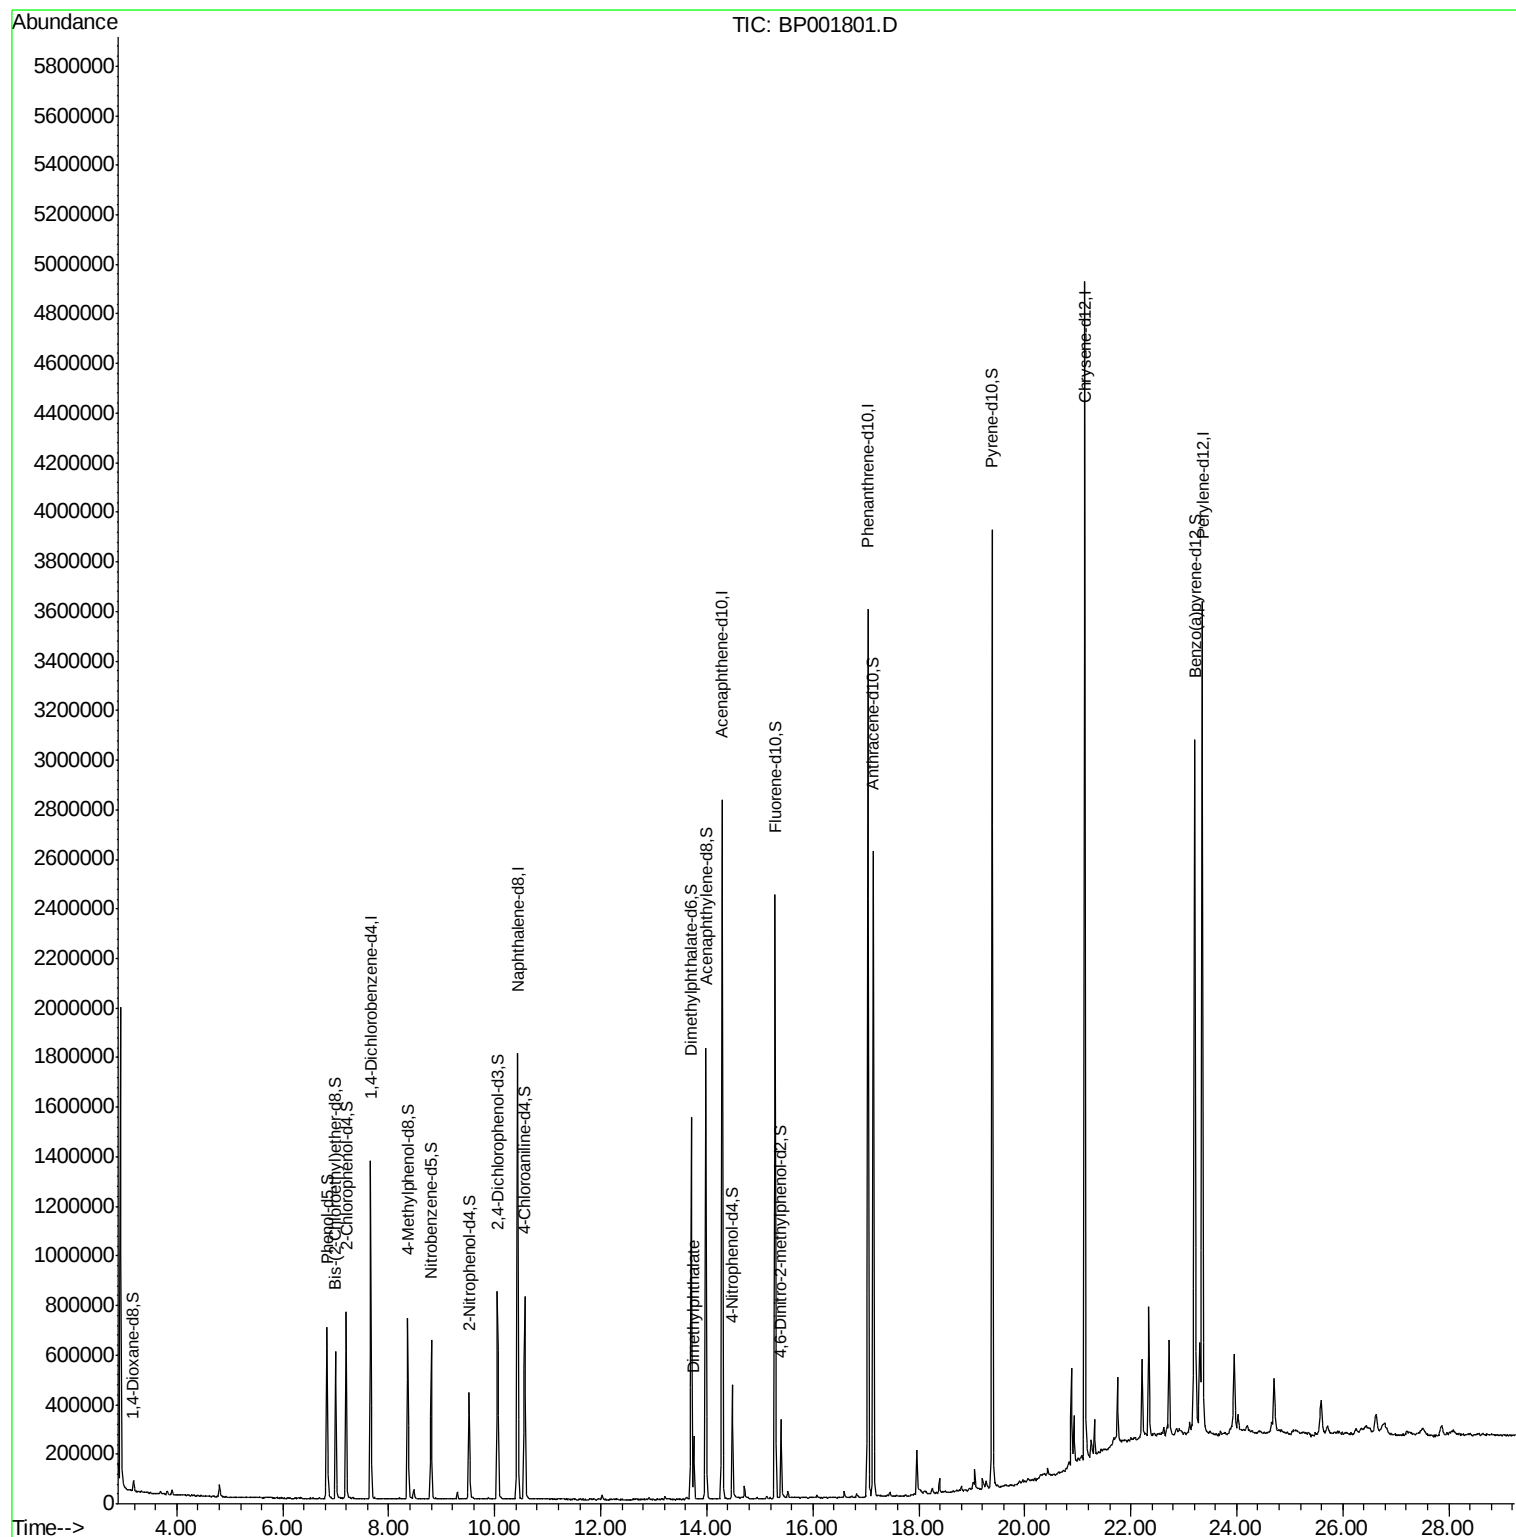

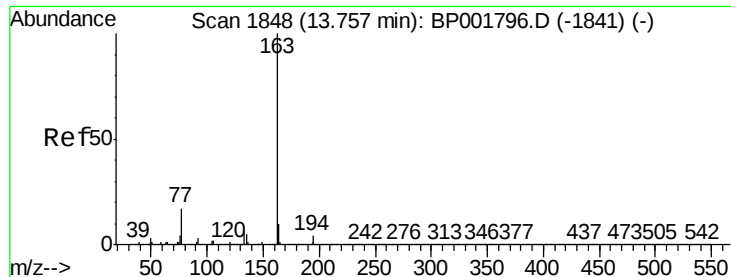

#45

Dimethylphthalate

Concen: 2.408 ng/ul

RT: 13.75 min Scan# 1847

Delta R.T. -0.01 min

Lab File: BP001801.D

Acq: 20 Feb 2020 14:29

Instrument :

BNA_P

ClientSampleId :

C5AT8


Tot Ion:163 Resp: 170157

Ion Ratio Lower Upper

163 100

194 4.5 3.5 5.3

164 10.5 8.0 12.0

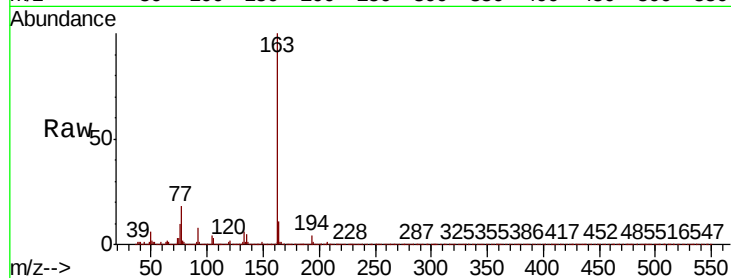

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

