
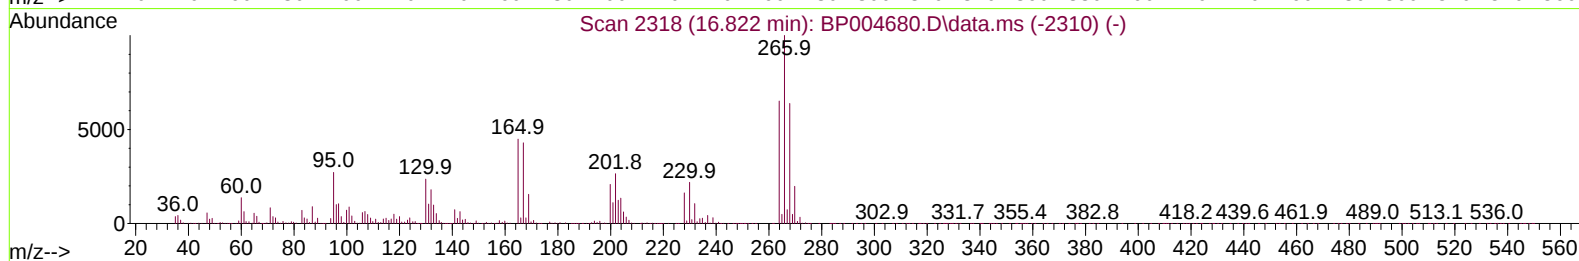
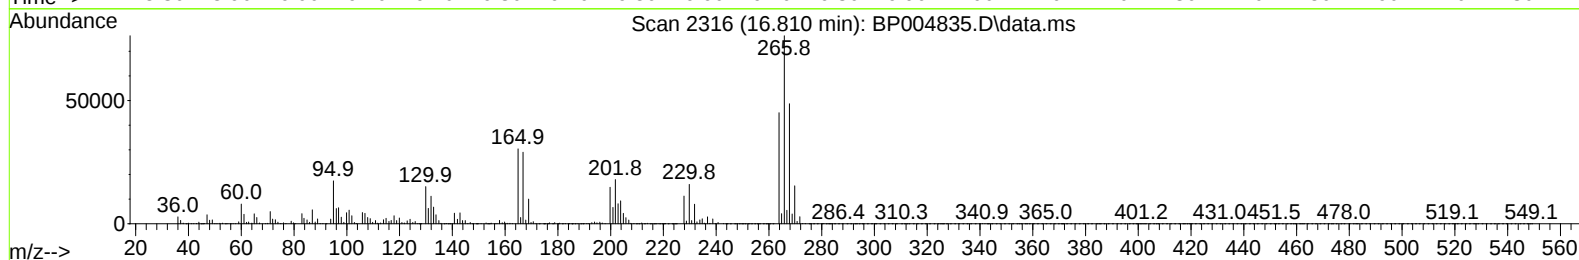


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022021\
Data File : BP004835.D
Acq On : 20 Feb 2021 10:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 22 05:14:29 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 19 12:04:44 2021
Response via : Initial Calibration

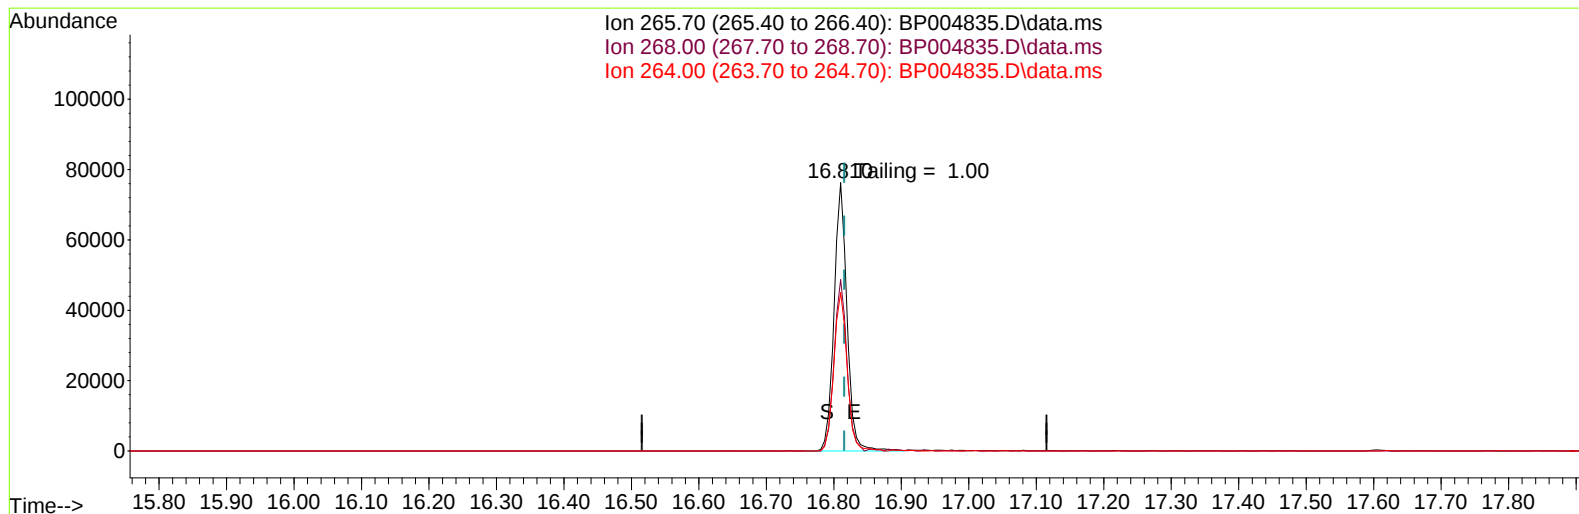

TIC: BP004835.D\data.ms

(70) Pentachlorophenol (C)




16.810min (-0.006) 295106.07 ng

response 101934

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	63.84
264.00	63.30	59.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022021\
 Data File : BP004835.D
 Acq On : 20 Feb 2021 10:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 22 05:14:29 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 19 12:04:44 2021
 Response via : Initial Calibration

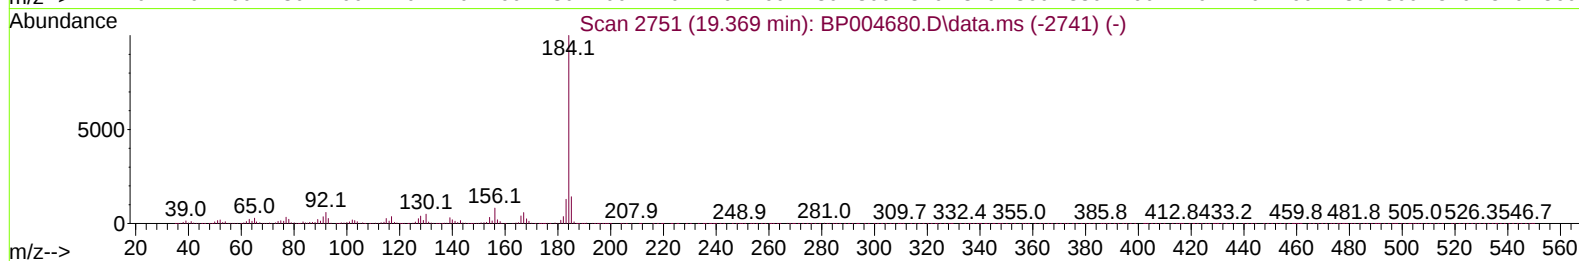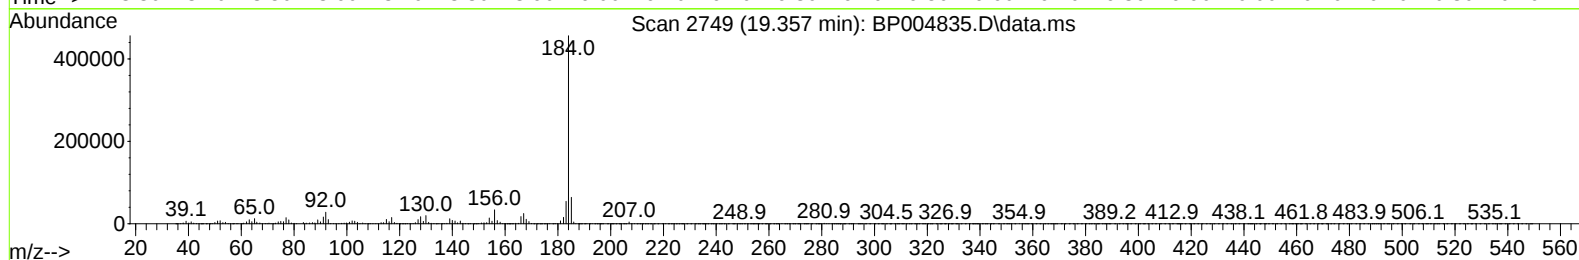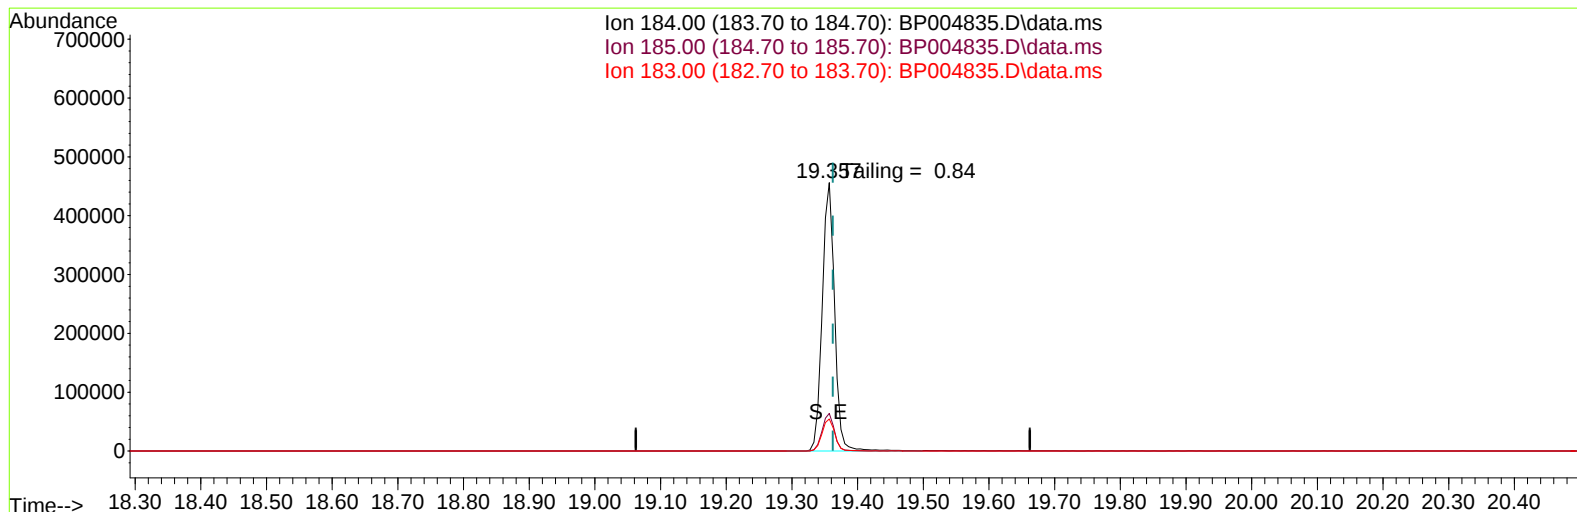

TIC: BP004835.D\data.ms

(77) Benzidine**19.357min (-0.006) 514943.18 ng****response 594637**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.04
183.00	12.00	11.93
0.00	0.00	0.00