

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022021\
 Data File : BP004843.D
 Acq On : 20 Feb 2021 15:34
 Operator : CG/JU
 Sample : M1425-13
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 41061

Manual Integrations
 APPROVED

mohammad
 2/22/2021 2:11:38 PM

Quant Time: Feb 22 04:31:37 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 19 12:04:44 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.757	152	58090	20.00	ng	0.00
21) Naphthalene-d8	10.551	136	228696	20.00	ng	# 0.00
39) Acenaphthene-d10	14.410	164	143998	20.00	ng	0.00
64) Phenanthrene-d10	17.163	188	306333	20.00	ng	0.00
76) Chrysene-d12	21.245	240	309527	20.00	ng	0.00
86) Perylene-d12	23.545	264	311786	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.357	112	233097	61.96	ng	0.00
7) Phenol-d6	6.951	99	181153	35.01	ng	0.00
23) Nitrobenzene-d5	8.916	82	357490	68.11	ng	0.00
42) 2,4,6-Tribromophenol	15.910	330	232992	121.78	ng	0.00
45) 2-Fluorobiphenyl	13.028	172	788987	66.97	ng	0.00
79) Terphenyl-d14	19.727	244	968083	52.54	ng	0.00
Target Compounds						Qvalue
6) Aniline	7.093	93	68768	11.92	ng	# 91
9) Benzaldehyde	6.904	77	5427	2.50	ng	# 82
10) Phenol	6.981	94	396471	79.16	ng	83
15) Benzyl Alcohol	8.004	79	12942	3.33	ng	# 81
17) 2-Methylphenol	8.216	107	12605	3.72	ng	# 85
20) 3+4-Methylphenols	8.598	107	2843123m	632.99	ng	
27) 2,4-Dimethylphenol	9.804	122	59401m	18.58	ng	
59) 2,3,4,6-Tetrachlorophenol	15.045	232	9845	3.02	ng	# 89
60) Diethylphthalate	15.239	149	29613	2.33	ng	# 93
70) Pentachlorophenol	16.821	266	30064	12.50	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022021\
Data File : BP004843.D
Acq On : 20 Feb 2021 15:34
Operator : CG/JU
Sample : M1425-13
Misc :
ALS Vial : 9 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
41061

Manual Integrations
APPROVED

mohammad
2/22/2021 2:11:38 PM

Quant Time: Feb 22 04:31:37 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 19 12:04:44 2021
Response via : Initial Calibration

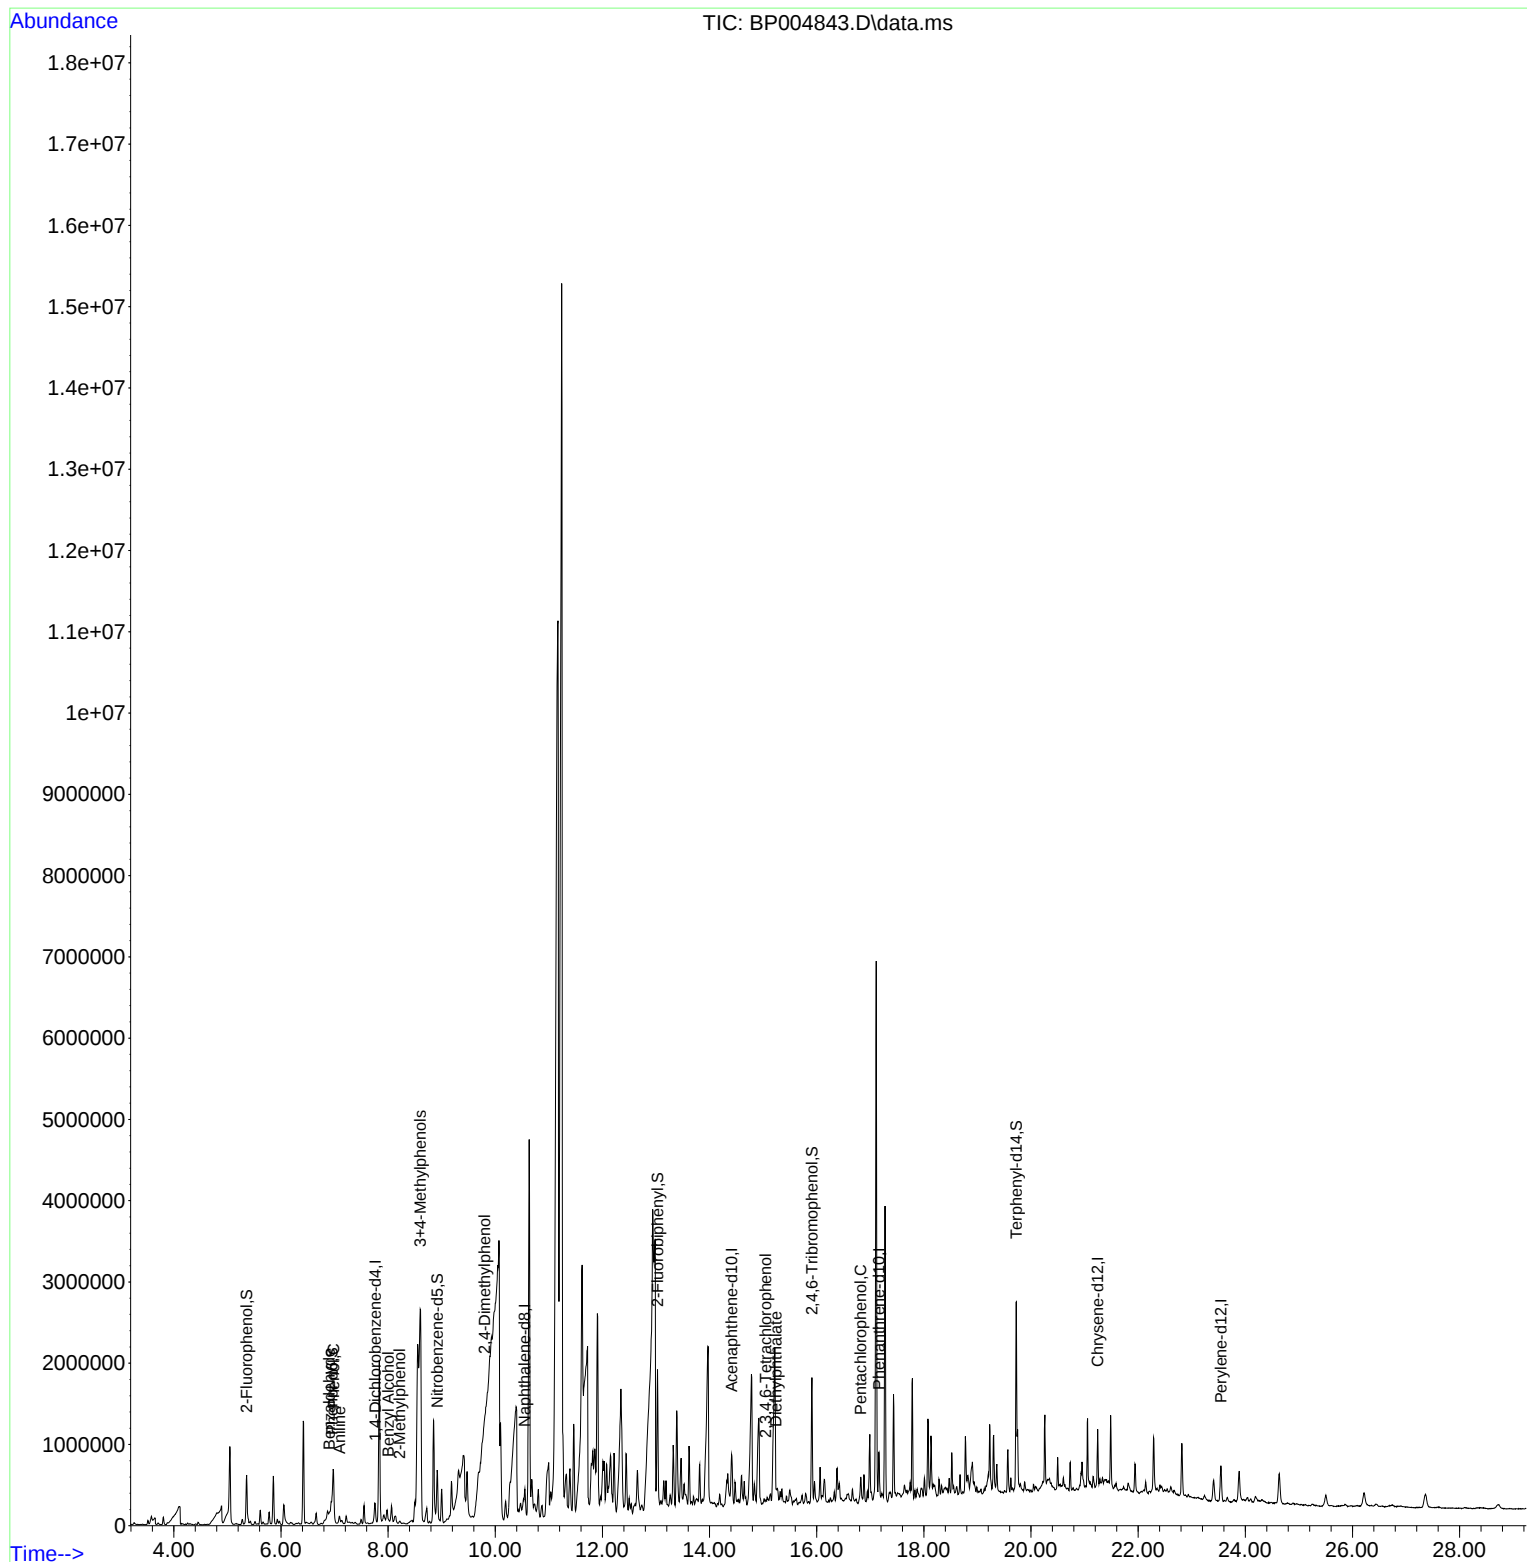







#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.757 min Scan# 777
Delta R.T. -0.006 min
Lab File: BP004843.D
Acq: 20 Feb 2021 15:34

Tgt Ion:152 Resp: 58090
Ion Ratio Lower Upper
152 100
150 157.2 123.8 185.6
115 63.6 43.8 65.6

Instrument :
BNA_P
ClientSampled :
41061




Manual Integrations
APPROVED


mohammad
2/22/2021 2:11:38 PM

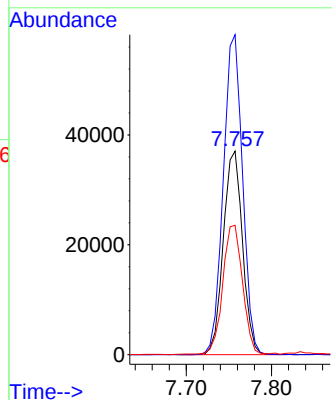

#5
2-Fluorophenol
Concen: 61.96 ng
RT: 5.357 min Scan# 369
Delta R.T. 0.006 min
Lab File: BP004843.D
Acq: 20 Feb 2021 15:34


Tgt Ion:112 Resp: 233097
Ion Ratio Lower Upper
112 100
64 52.9 32.8 49.2#
63 30.0 17.0 25.4#

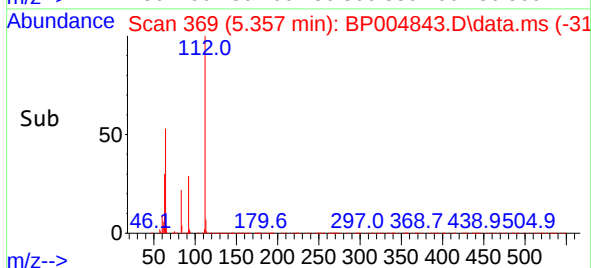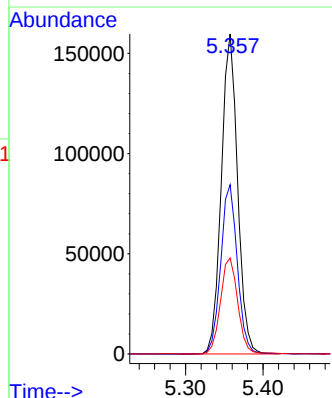



#6
Aniline
Concen: 11.92 ng
RT: 7.093 min Scan# 664
Delta R.T. -0.000 min
Lab File: BP004843.D
Acq: 20 Feb 2021 15:34




Instrument :
BNA_P
ClientSampleId :
41061




Tgt Ion: 93 Resp: 68768
Ion Ratio Lower Upper
93 100
66 36.8 25.4 38.0
65 18.8 12.5 18.7#

Manual Integrations
APPROVED



mohammad
2/22/2021 2:11:38 PM

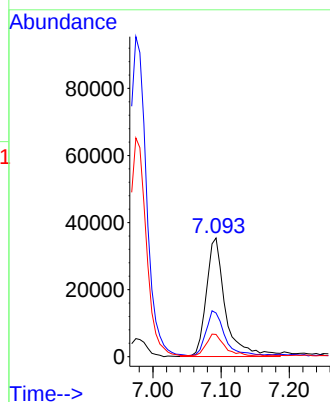


#7
Phenol-d6
Concen: 35.01 ng
RT: 6.951 min Scan# 640
Delta R.T. 0.006 min
Lab File: BP004843.D
Acq: 20 Feb 2021 15:34



Tgt Ion: 99 Resp: 181153
Ion Ratio Lower Upper
99 100
42 18.6 8.6 13.0#
71 42.2 23.4 35.2#

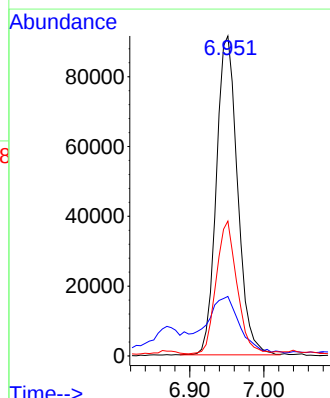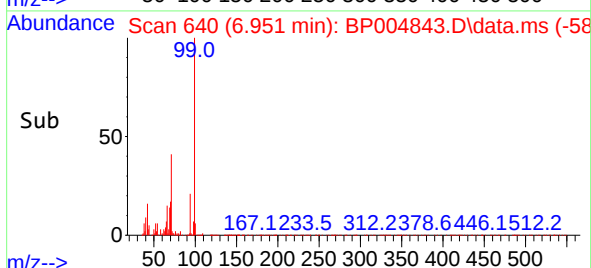

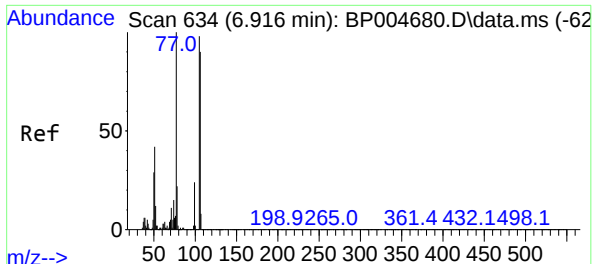





#9
Benzaldehyde
Concen: 2.50 ng
RT: 6.904 min Scan# 632
Delta R.T. -0.000 min
Lab File: BP004843.D
Acq: 20 Feb 2021 15:34

Instrument :
BNA_P
ClientSampleId :
41061

Manual Integrations
APPROVED




mohammad
2/22/2021 2:11:38 PM


Tgt Ion: 77 Resp: 5427
Ion Ratio Lower Upper
77 100
105 100.3 97.1 137.1
106 90.5 93.7 133.7#

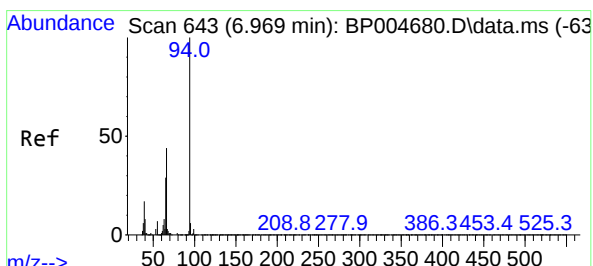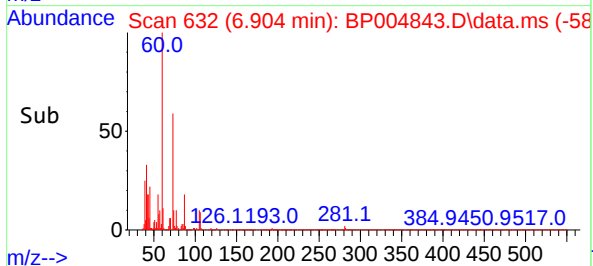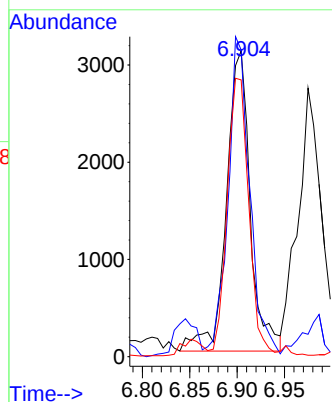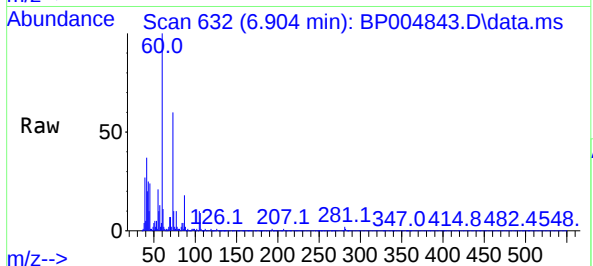

#10
Phenol
Concen: 79.16 ng
RT: 6.981 min Scan# 645
Delta R.T. 0.012 min
Lab File: BP004843.D
Acq: 20 Feb 2021 15:34


Tgt Ion: 94 Resp: 396471
Ion Ratio Lower Upper
94 100
65 28.7 2.3 42.3
66 41.7 10.9 50.9

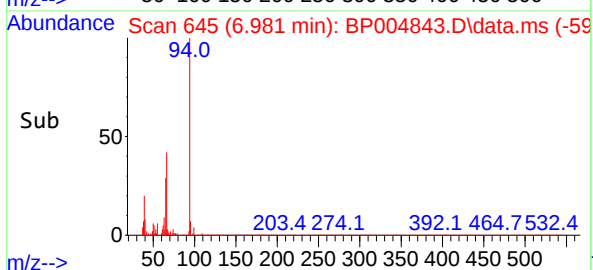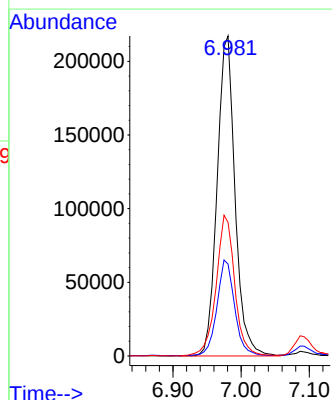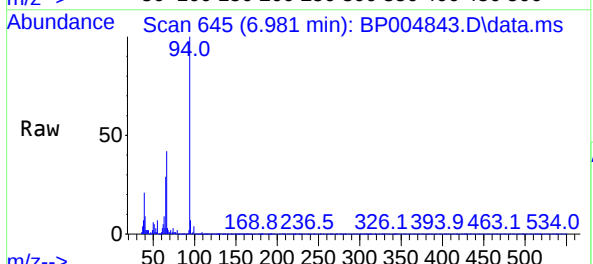



#15
Benzyl Alcohol
Concen: 3.33 ng
RT: 8.004 min Scan# 819
Delta R.T. -0.000 min
Lab File: BP004843.D
Acq: 20 Feb 2021 15:34




Instrument :
BNA_P
ClientSampled :
41061




Tgt Ion: 79 Resp: 12942
Ion Ratio Lower Upper
79 100
108 62.8 73.5 110.3#
77 63.9 50.3 75.5

Manual Integrations
APPROVED



mohammad
2/22/2021 2:11:38 PM

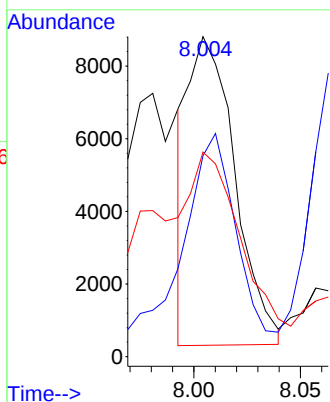


#17
2-Methylphenol
Concen: 3.72 ng
RT: 8.216 min Scan# 855
Delta R.T. 0.006 min
Lab File: BP004843.D
Acq: 20 Feb 2021 15:34




Tgt Ion: 107 Resp: 12605
Ion Ratio Lower Upper
107 100
108 126.3 89.6 134.4
77 54.5 31.8 47.6#
79 46.5 31.1 46.7

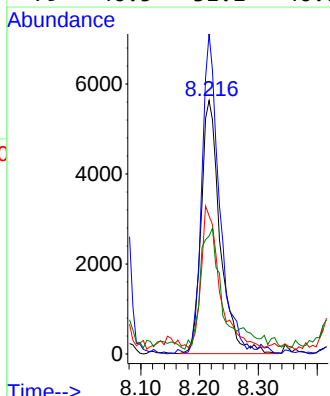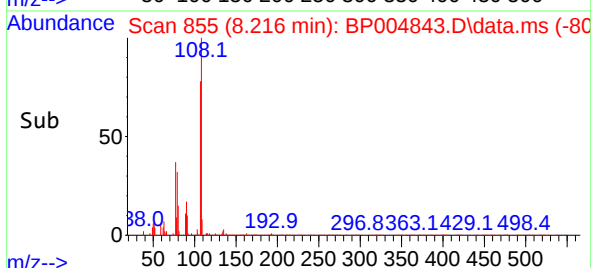



#20
3+4-Methylphenols
Concen: 632.99 ng m
RT: 8.598 min Scan# 920
Delta R.T. 0.059 min
Lab File: BP004843.D
Acq: 20 Feb 2021 15:34




Instrument :
BNA_P
ClientSampled :
41061




Tgt Ion:107 Resp: 2843123
Ion Ratio Lower Upper
107 100
108 78.1 69.0 109.0
77 32.6 8.5 48.5
79 23.8 4.8 44.8

Manual Integrations
APPROVED



mohammad
2/22/2021 2:11:38 PM

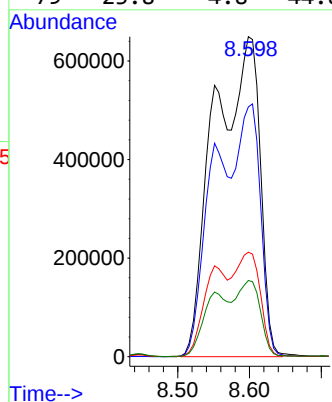


#21
Naphthalene-d8
Concen: 20.00 ng
RT: 10.551 min Scan# 1252
Delta R.T. -0.006 min
Lab File: BP004843.D
Acq: 20 Feb 2021 15:34




Tgt Ion:136 Resp: 228696
Ion Ratio Lower Upper
136 100
137 11.2 8.6 13.0
54 6.5 3.6 5.4#
68 5.7 3.3 4.9#

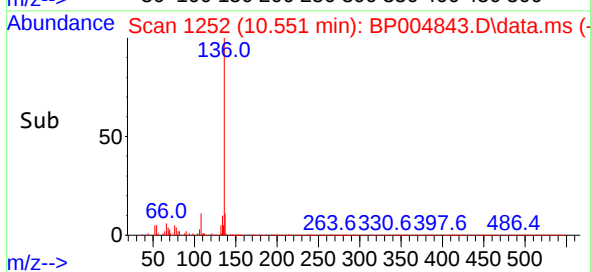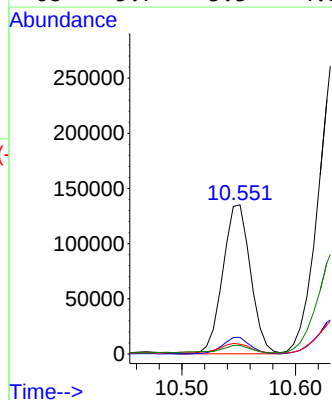



#23
Nitrobenzene-d5
Concen: 68.11 ng
RT: 8.916 min Scan# 974
Delta R.T. -0.006 min
Lab File: BP004843.D
Acq: 20 Feb 2021 15:34




Instrument :
BNA_P
ClientSampleId :
41061




Tgt Ion: 82 Resp: 357490
Ion Ratio Lower Upper
82 100
128 41.4 45.6 68.4#
54 44.9 30.1 45.1

Manual Integrations
APPROVED



mohammad
2/22/2021 2:11:38 PM

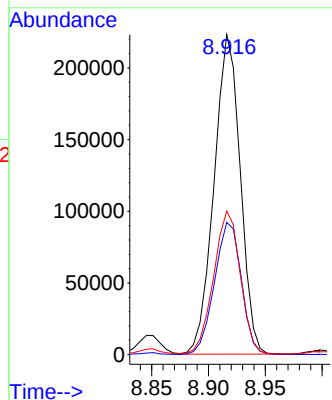


#27
2,4-Dimethylphenol
Concen: 18.58 ng m
RT: 9.804 min Scan# 1125
Delta R.T. 0.065 min
Lab File: BP004843.D
Acq: 20 Feb 2021 15:34




Tgt Ion: 122 Resp: 59401
Ion Ratio Lower Upper
122 100
107 125.1 87.3 130.9
121 51.2 47.3 70.9

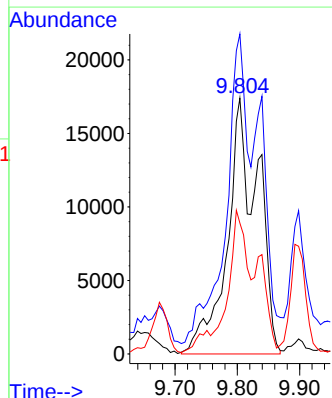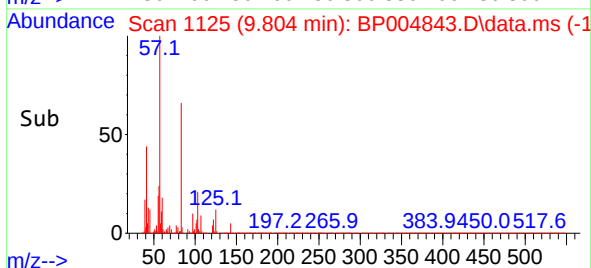



#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.410 min Scan# 1908
Delta R.T. -0.000 min
Lab File: BP004843.D
Acq: 20 Feb 2021 15:34




Instrument :
BNA_P
ClientSampled :
41061

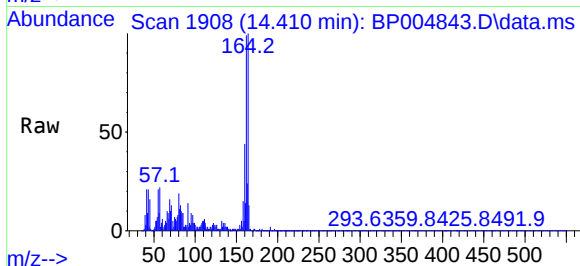

Tgt Ion:164 Resp: 143998
Ion Ratio Lower Upper
164 100
162 99.3 79.4 119.2
160 43.5 36.1 54.1




Manual Integrations
APPROVED


mohammad
2/22/2021 2:11:38 PM

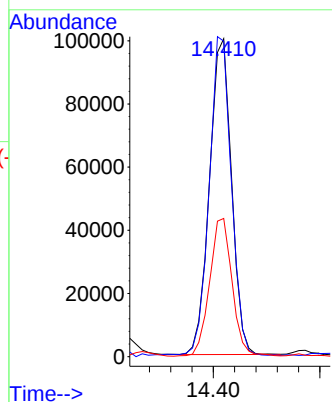

#42
2,4,6-Tribromophenol
Concen: 121.78 ng
RT: 15.910 min Scan# 2163
Delta R.T. -0.000 min
Lab File: BP004843.D
Acq: 20 Feb 2021 15:34


Tgt Ion:330 Resp: 232992
Ion Ratio Lower Upper
330 100
332 97.7 77.1 115.7
141 38.7 23.4 35.2#

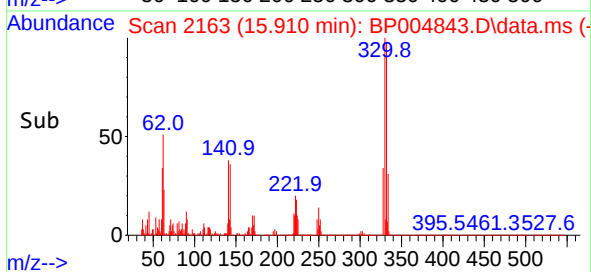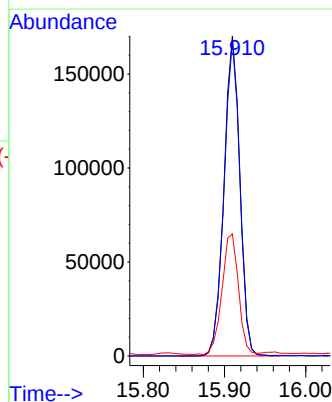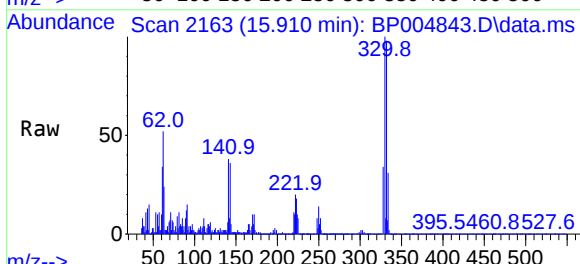



#45
2-Fluorobiphenyl
Concen: 66.97 ng
RT: 13.028 min Scan# 1673
Delta R.T. -0.000 min
Lab File: BP004843.D
Acq: 20 Feb 2021 15:34




Instrument :
BNA_P
ClientSampled :
41061

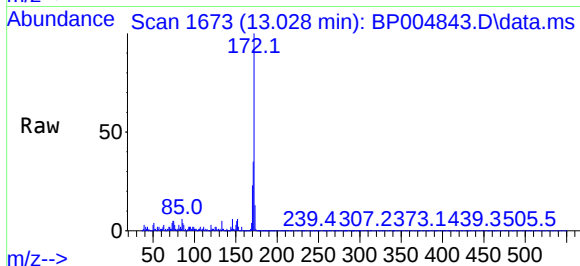


Tgt Ion:172 Resp: 788987
Ion Ratio Lower Upper
172 100
171 35.0 28.5 42.7
170 23.3 19.2 28.8

Manual Integrations
APPROVED



mohammad
2/22/2021 2:11:38 PM

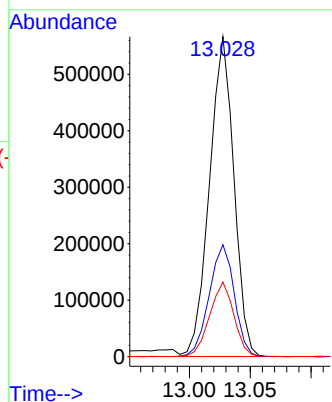


#59
2,3,4,6-Tetrachlorophenol
Concen: 3.02 ng
RT: 15.045 min Scan# 2016
Delta R.T. 0.006 min
Lab File: BP004843.D
Acq: 20 Feb 2021 15:34

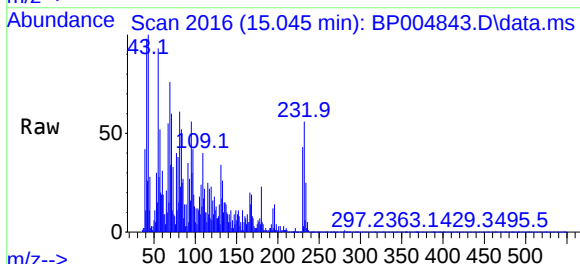


Tgt Ion:232 Resp: 9845
Ion Ratio Lower Upper
232 100
131 54.6 34.1 51.1#
130 0.0 1.8 2.8#
166 31.0 24.6 36.8

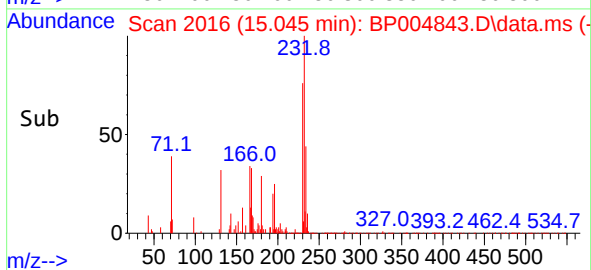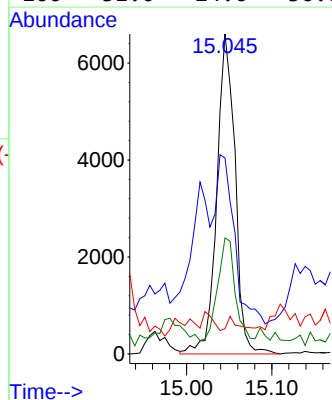



#60
Diethylphthalate
Concen: 2.33 ng
RT: 15.239 min Scan# 2049
Delta R.T. -0.000 min
Lab File: BP004843.D
Acq: 20 Feb 2021 15:34




Instrument :
BNA_P
ClientSampled :
41061

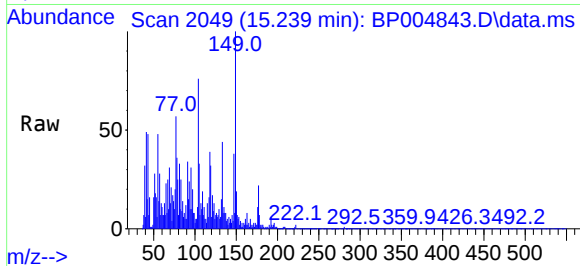


Tgt Ion:149 Resp: 29613
Ion Ratio Lower Upper
149 100
177 21.7 18.0 27.0
150 19.3 10.0 15.0#

Manual Integrations
APPROVED



mohammad
2/22/2021 2:11:38 PM

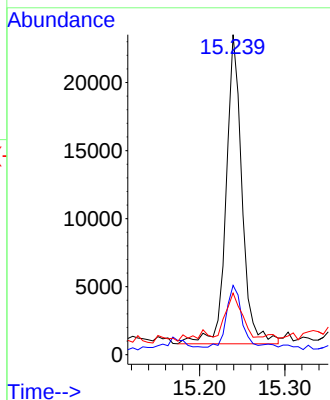


#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.163 min Scan# 2376
Delta R.T. -0.000 min
Lab File: BP004843.D
Acq: 20 Feb 2021 15:34

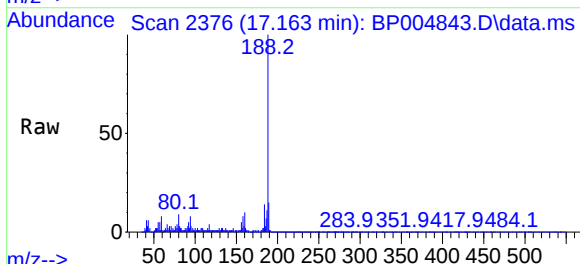


Tgt Ion:188 Resp: 306333
Ion Ratio Lower Upper
188 100
94 7.6 6.2 9.2
80 9.1 6.2 9.2

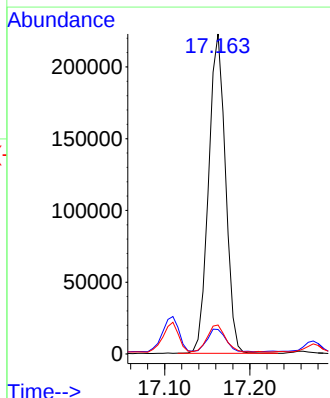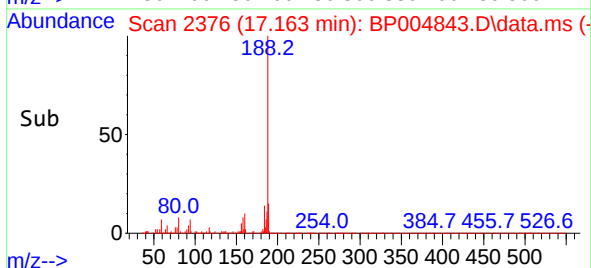



#70
Pentachlorophenol
Concen: 12.50 ng
RT: 16.821 min Scan# 2318
Delta R.T. 0.006 min
Lab File: BP004843.D
Acq: 20 Feb 2021 15:34




Instrument :
BNA_P
ClientSampled :
41061




Tgt Ion:266 Resp: 30064
Ion Ratio Lower Upper
266 100
268 67.0 51.1 76.7
264 63.8 50.6 76.0

Manual Integrations
APPROVED



mohammad
2/22/2021 2:11:38 PM

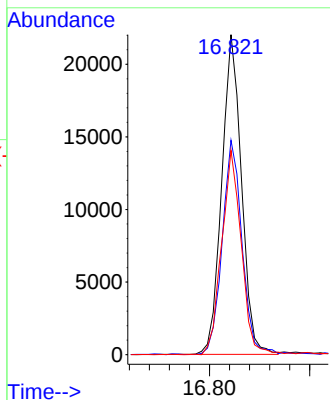


#76
Chrysene-d12
Concen: 20.00 ng
RT: 21.245 min Scan# 3070
Delta R.T. -0.006 min
Lab File: BP004843.D
Acq: 20 Feb 2021 15:34




Tgt Ion:240 Resp: 309527
Ion Ratio Lower Upper
240 100
120 8.2 7.8 11.6
236 25.4 20.8 31.2


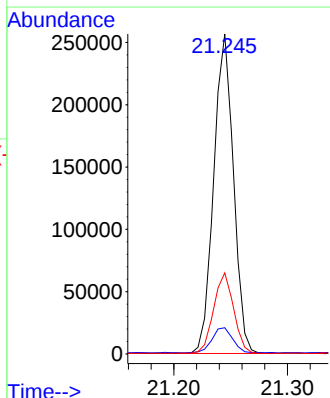
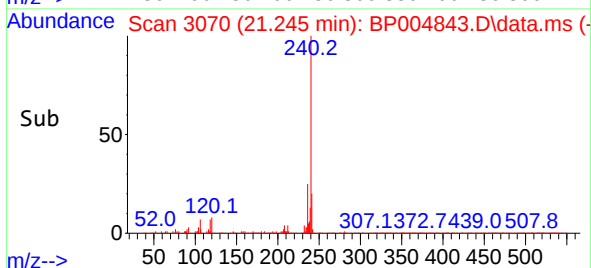





#79
Terphenyl-d14
Concen: 52.54 ng
RT: 19.727 min Scan# 2812
Delta R.T. -0.006 min
Lab File: BP004843.D
Acq: 20 Feb 2021 15:34





Tgt Ion: 244 Resp: 968083
Ion Ratio Lower Upper
244 100
212 7.2 5.8 8.6
122 8.6 7.8 11.8

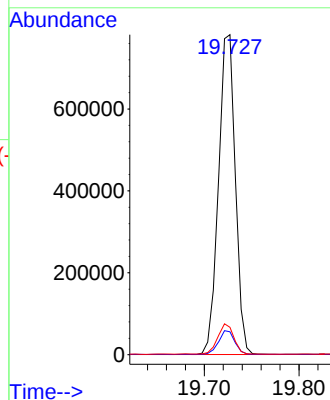

#86
Perylene-d12
Concen: 20.00 ng
RT: 23.545 min Scan# 3461
Delta R.T. -0.012 min
Lab File: BP004843.D
Acq: 20 Feb 2021 15:34



Tgt Ion: 264 Resp: 311786
Ion Ratio Lower Upper
264 100
260 23.2 18.8 28.2
265 21.5 17.4 26.2

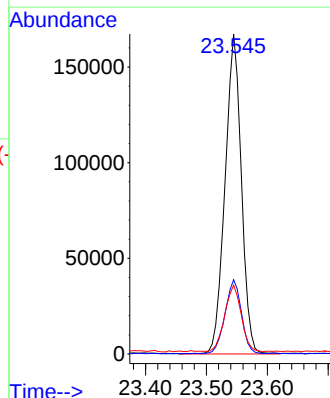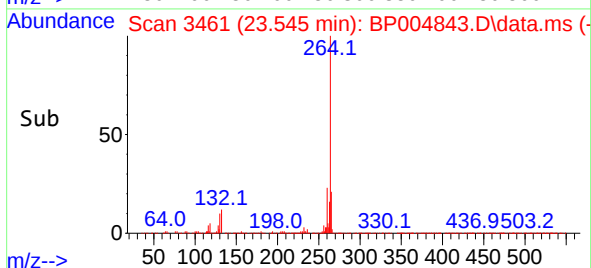

Instrument :
BNA_P
ClientSampled :
41061

Manual Integrations
APPROVED

mohammad
2/22/2021 2:11:38 PM