
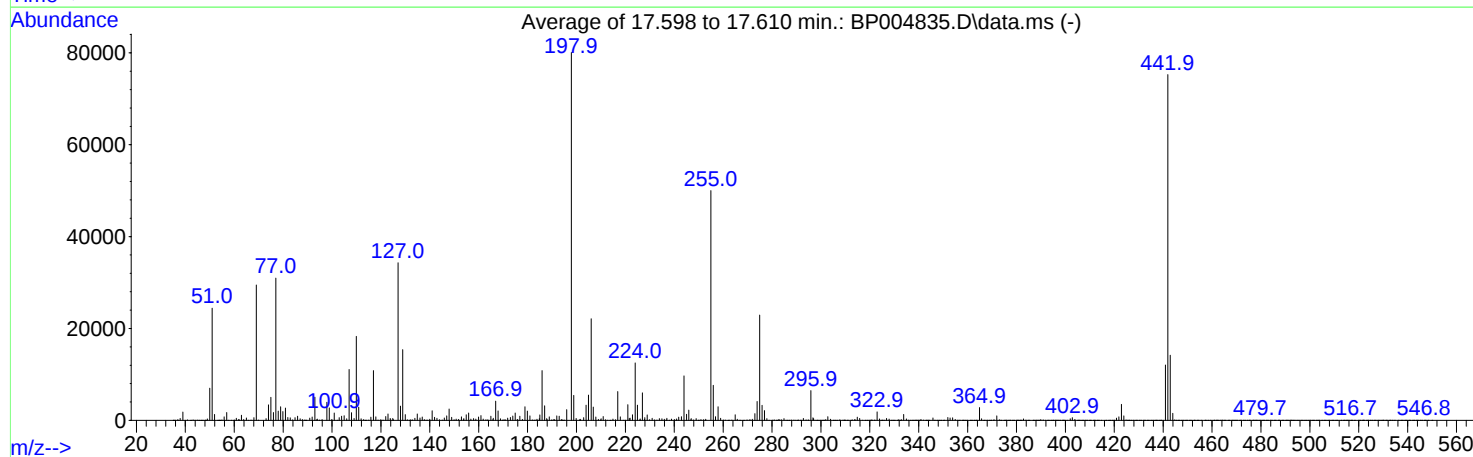


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022021\
 Data File : BP004835.D
 Acq On : 20 Feb 2021 10:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 19 12:04:44 2021

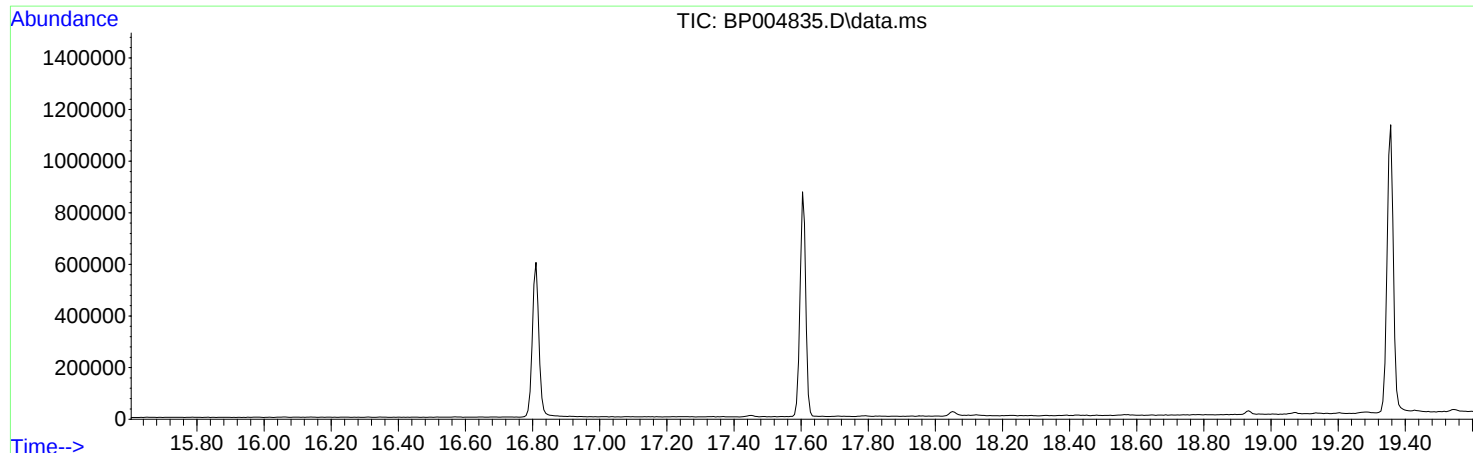




AutoFind: Scans 2450, 2451, 2452; Background Corrected with Scan 2441

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.5	24426	PASS
68	69	0.00	2	2.0	579	PASS
69	198	0.00	100	36.8	29470	PASS
70	69	0.00	2	0.2	65	PASS
127	198	10	80	42.8	34304	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	80077	PASS
199	198	5	9	6.8	5455	PASS
275	198	10	60	28.6	22930	PASS
365	198	1	100	3.5	2788	PASS
441	198	0.01	100	15.1	12068	PASS
442	442	100	100	100.0	75283	PASS
443	442	15	24	18.8	14162	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022021\
 Data File : BP004835.D
 Acq On : 20 Feb 2021 10:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Feb 22 05:14:29 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 19 12:04:44 2021
 Response via : Initial Calibration

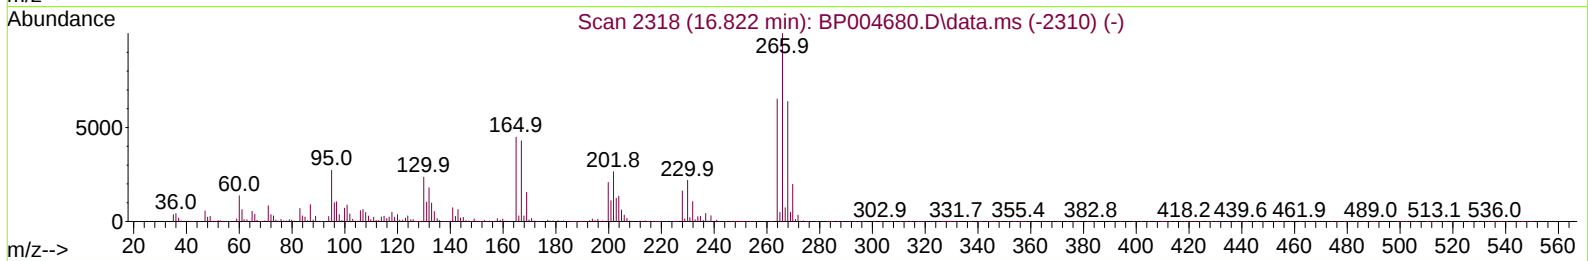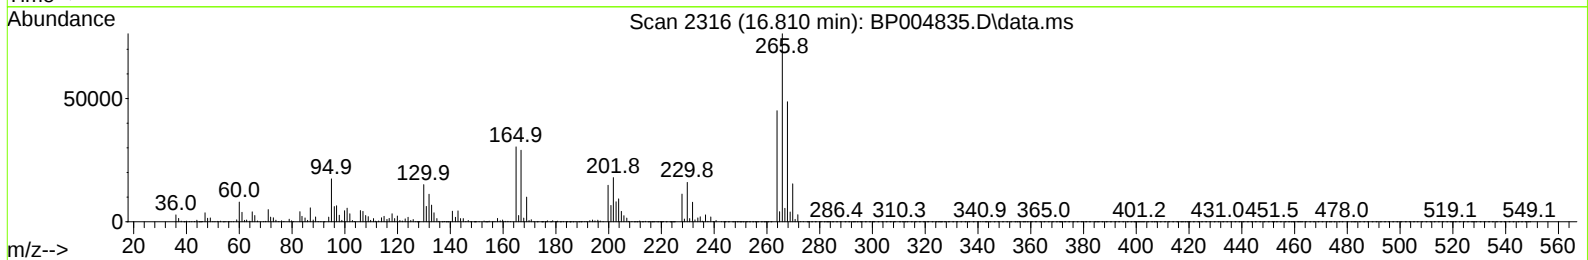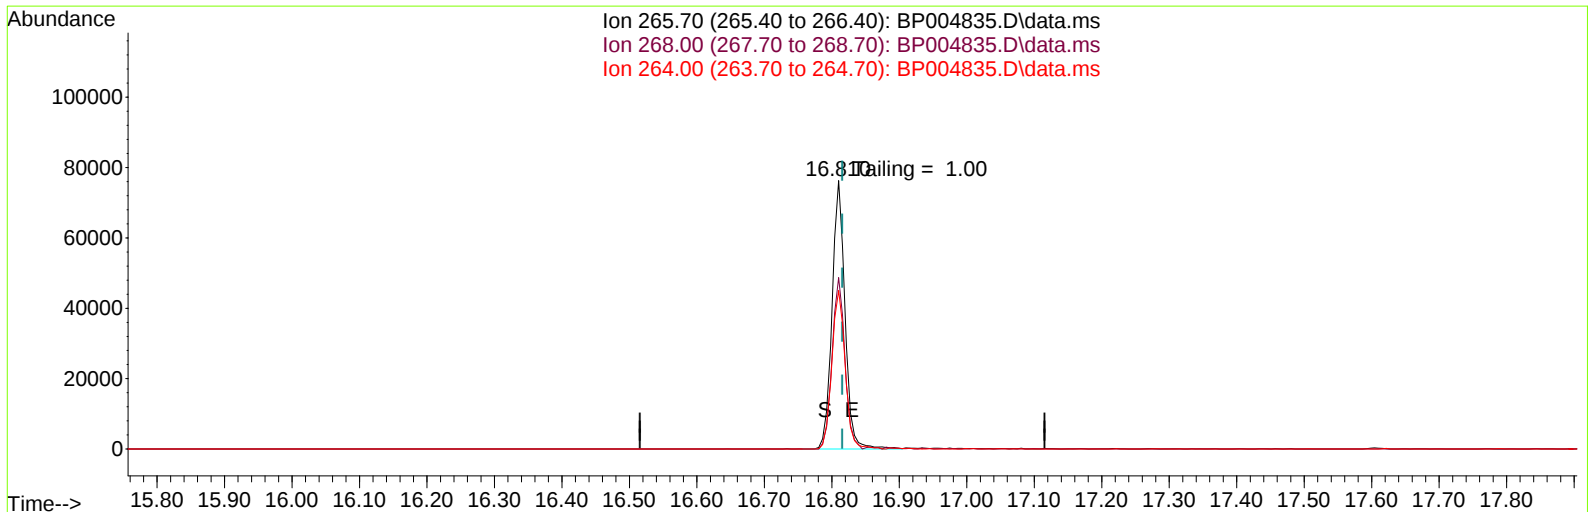

TIC: BP004835.D\data.ms

(70) Pentachlorophenol (C)

16.810min (-0.006) 295106.07 ng




response 101934

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	63.84
264.00	63.30	59.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022021\
 Data File : BP004835.D
 Acq On : 20 Feb 2021 10:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Feb 22 05:14:29 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 19 12:04:44 2021
 Response via : Initial Calibration

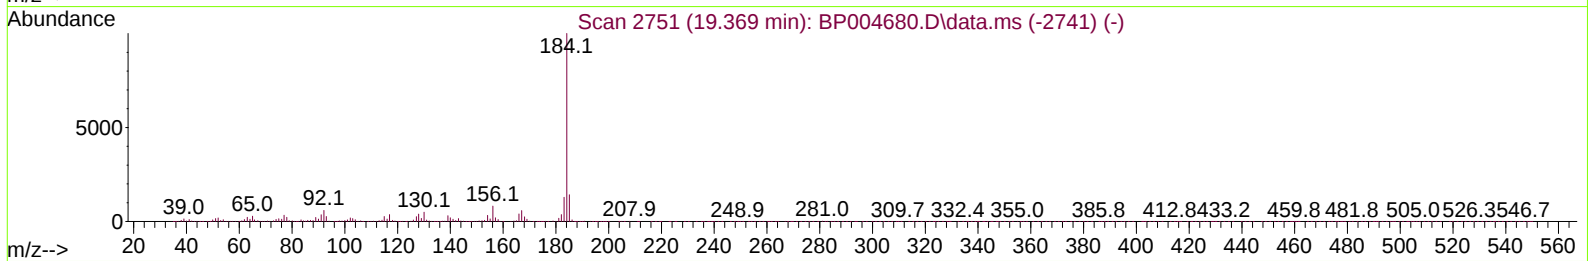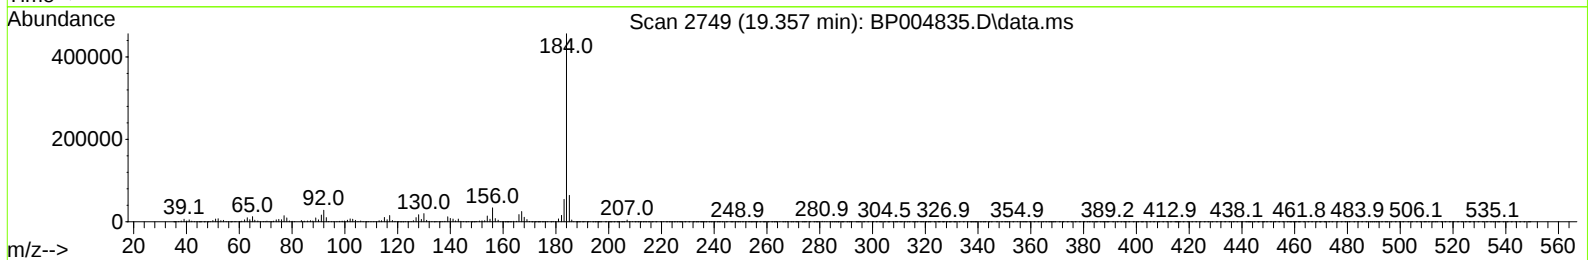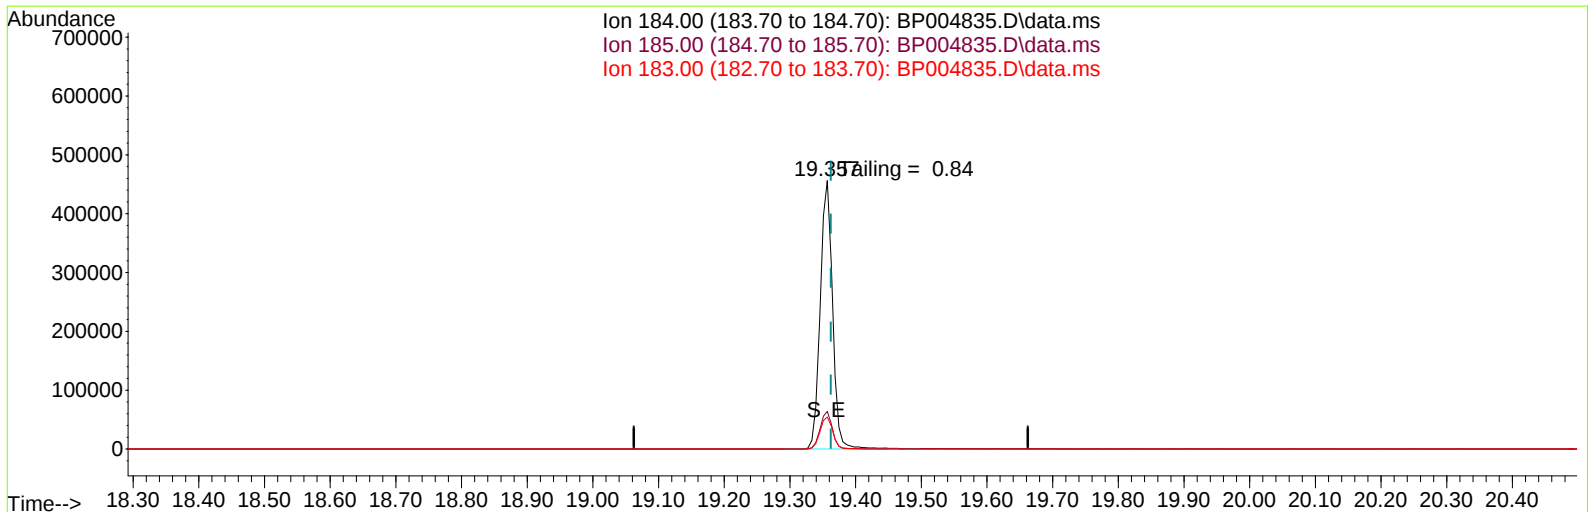

TIC: BP004835.D\data.ms

(77) Benzidine

19.357min (-0.006) 514943.18 ng

response 594637

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.04
183.00	12.00	11.93
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_P
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
02/20/2021	BNA_P	BP004835.D
Compound Name	Response	Retention Time
DDT	320591	20.551
DDD	3418	20.127
DDE	473	19.627
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3891	324482	1.20