
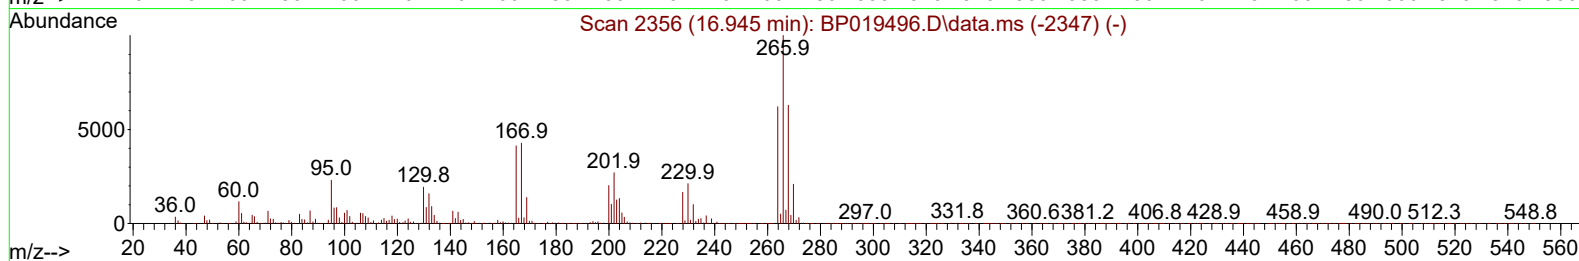
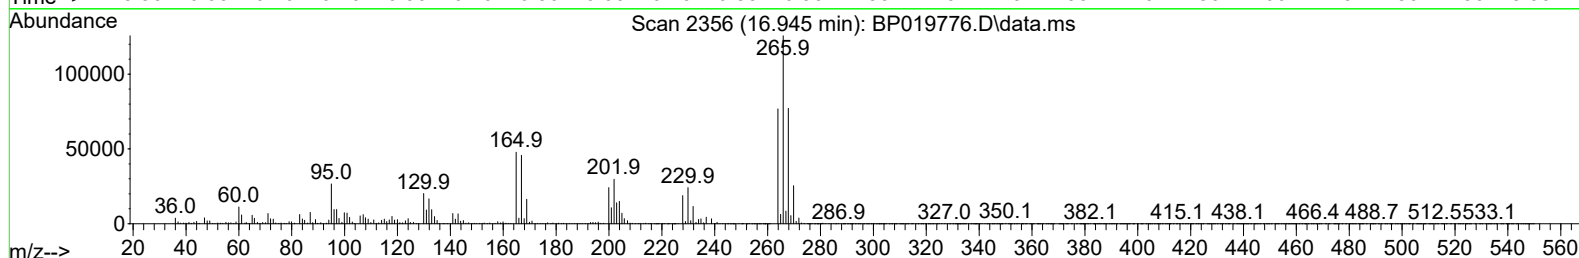


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022024\
Data File : BP019776.D
Acq On : 20 Feb 2024 09:36
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 20 10:36:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 19 23:35:42 2024
Response via : Initial Calibration

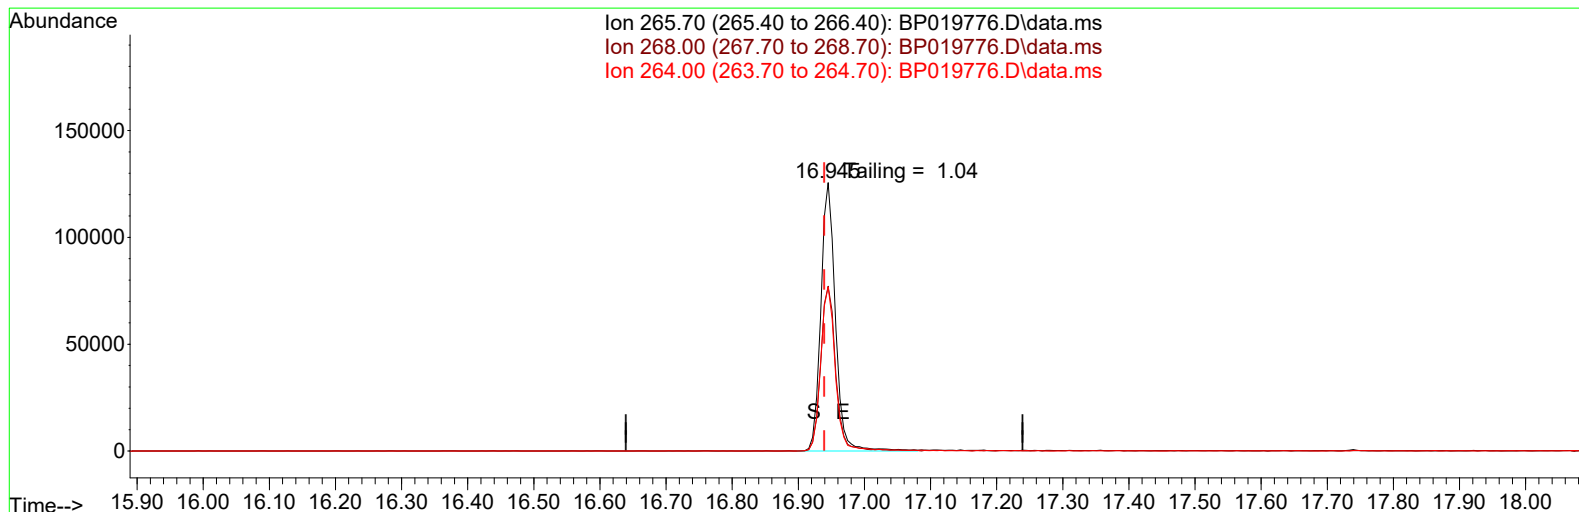

TIC: BP019776.D\data.ms

(70) Pentachlorophenol (C)




16.945min (+ 0.006) 133831.05 ng

response 192236

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	61.39
264.00	62.10	61.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022024\
Data File : BP019776.D
Acq On : 20 Feb 2024 09:36
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 20 10:36:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 19 23:35:42 2024
Response via : Initial Calibration

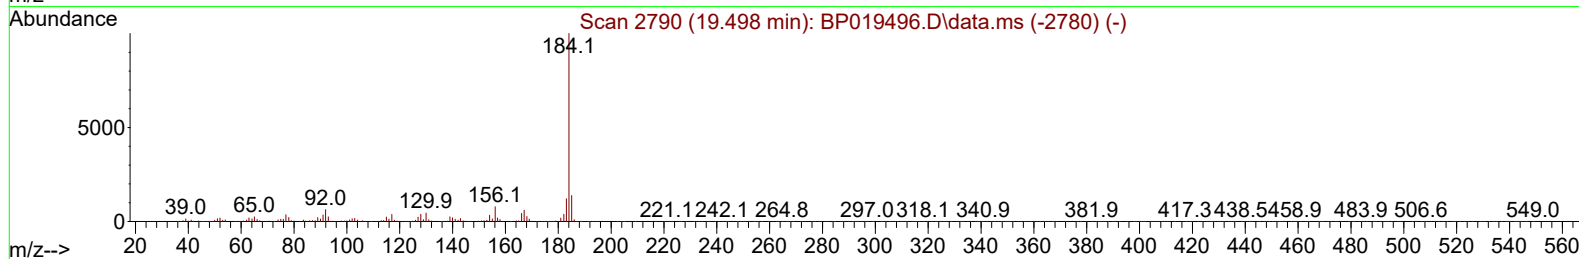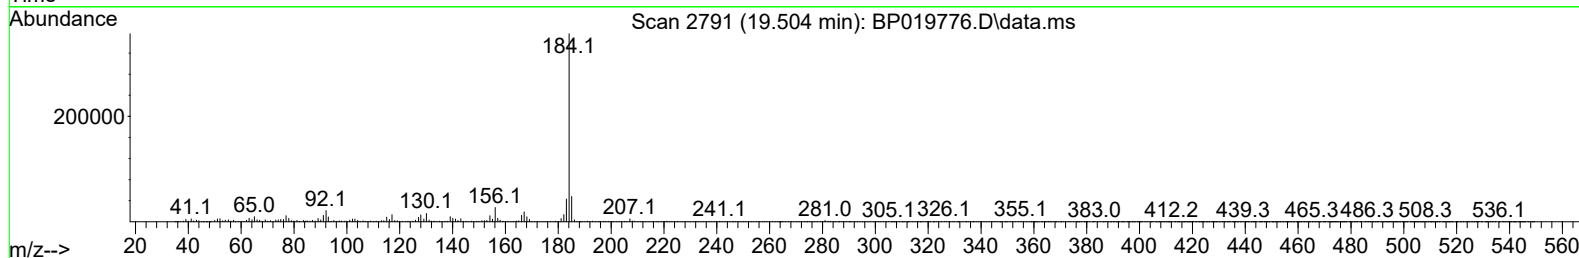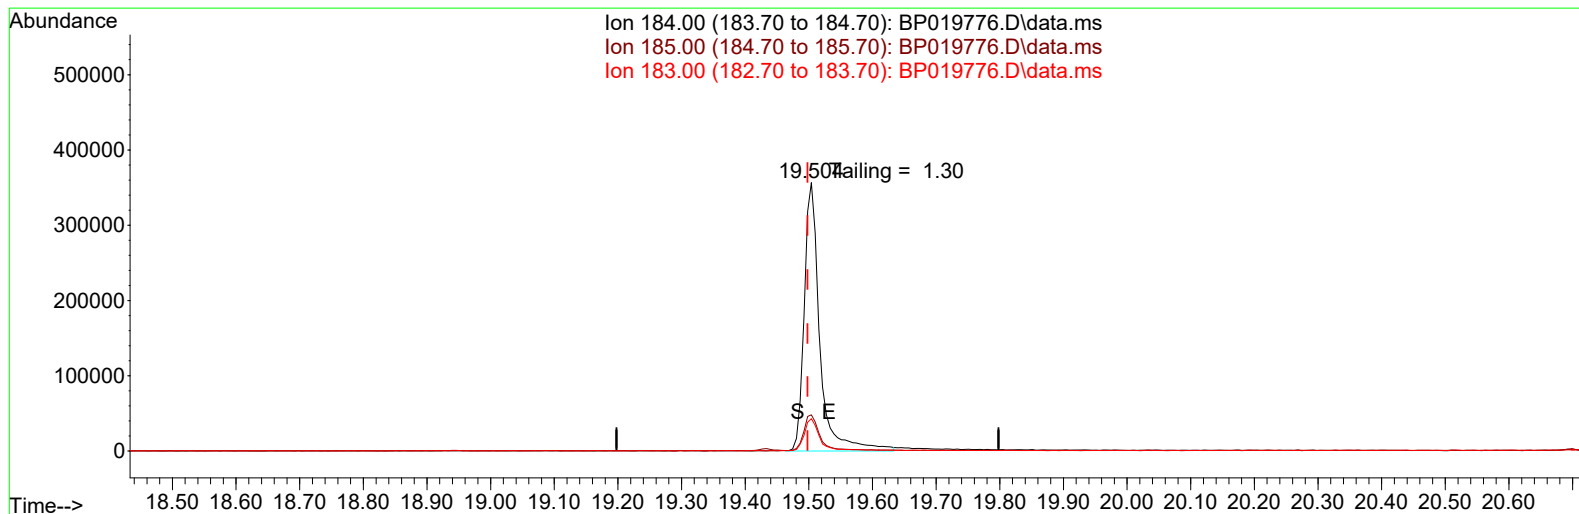

TIC: BP019776.D\data.ms

(77) Benzidine**19.504min (+ 0.006) 54622.56 ng****response 621235**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.49
183.00	12.10	12.07
0.00	0.00	0.00