

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022024\
 Data File : BP019794.D
 Acq On : 20 Feb 2024 19:52
 Operator : MA/JU
 Sample : P1523-07
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 20240767-AMENDED-COMP-39N-N-3-02

Quant Time: Feb 20 23:55:33 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 19 23:35:42 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.893	152	63064	20.000	ng	0.00
21) Naphthalene-d8	10.699	136	227689	20.000	ng	0.00
39) Acenaphthene-d10	14.528	164	161885	20.000	ng	-0.01
64) Phenanthrene-d10	17.287	188	391560	20.000	ng	0.00
76) Chrysene-d12	21.380	240	442373	20.000	ng	#-0.01
86) Perylene-d12	23.798	264	499270	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.469	112	190417	48.671	ng	0.00
7) Phenol-d6	7.069	99	310647	58.887	ng	0.00
23) Nitrobenzene-d5	9.063	82	285909	54.411	ng	0.00
42) 2,4,6-Tribromophenol	16.028	330	108390	45.857	ng	0.00
45) 2-Fluorobiphenyl	13.157	172	630942	48.182	ng	0.00
79) Terphenyl-d14	19.857	244	1411867	52.487	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022024\
Data File : BP019794.D
Acq On : 20 Feb 2024 19:52
Operator : MA/JU
Sample : P1523-07
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
20240767-AMENDED-COMP-39N-N-3-02

Quant Time: Feb 20 23:55:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 19 23:35:42 2024
Response via : Initial Calibration




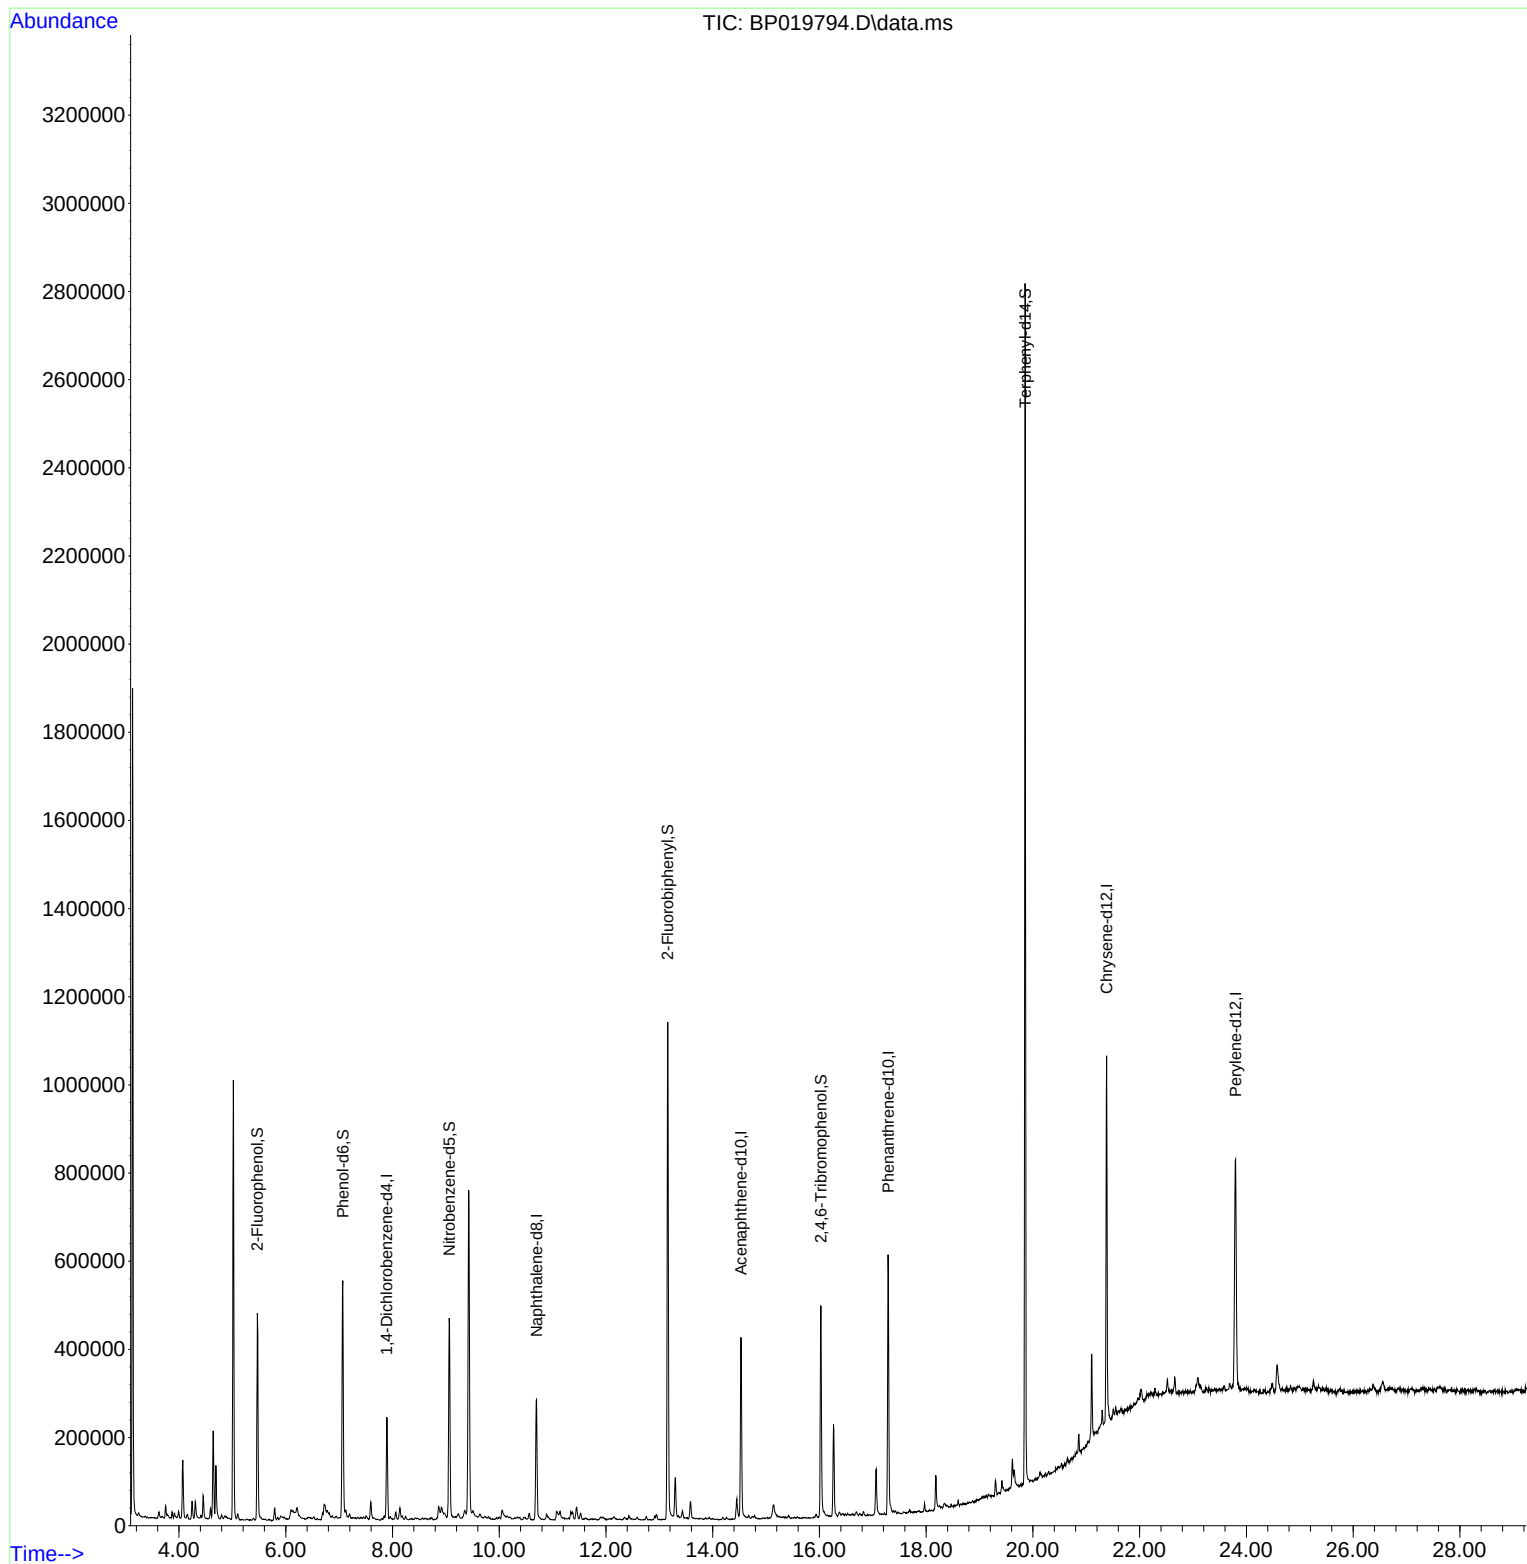




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.893 min Scan# 81
Delta R.T. -0.006 min
Lab File: BP019794.D
Acq: 20 Feb 2024 19:52




Instrument :
BNA_P
ClientSampleId :
20240767-AMENDED-COMP-39N-N-3-02


Tgt Ion:152 Resp: 63064
Ion Ratio Lower Upper
152 100
150 156.1 121.8 182.8
115 61.8 49.9 74.9

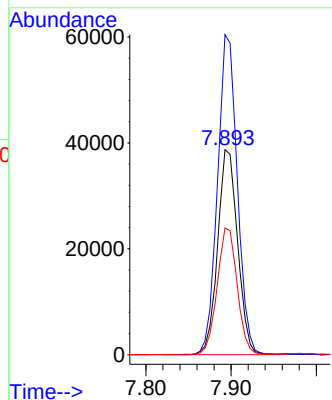

#5
2-Fluorophenol
Concen: 48.671 ng
RT: 5.469 min Scan# 405
Delta R.T. -0.006 min
Lab File: BP019794.D
Acq: 20 Feb 2024 19:52

Tgt Ion:112 Resp: 190417
Ion Ratio Lower Upper
112 100
64 61.0 47.4 71.0
63 33.9 27.0 40.6


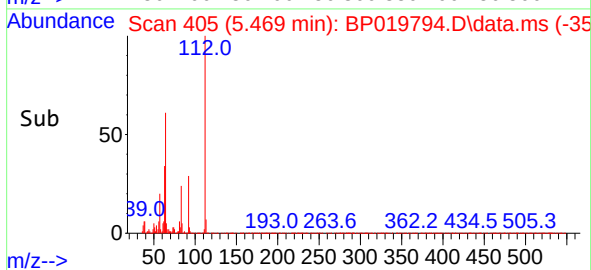
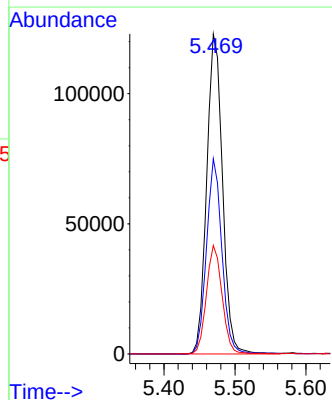





#7
Phenol-d6
Concen: 58.887 ng
RT: 7.069 min Scan# 61
Delta R.T. 0.000 min
Lab File: BP019794.D
Acq: 20 Feb 2024 19:52




Instrument :
BNA_P
ClientSampleId :
20240767-AMENDED-COMP-39N-N-3-02


Tgt Ion: 99 Resp: 310647
Ion Ratio Lower Upper
99 100
42 17.5 14.7 22.1
71 42.7 34.8 52.2

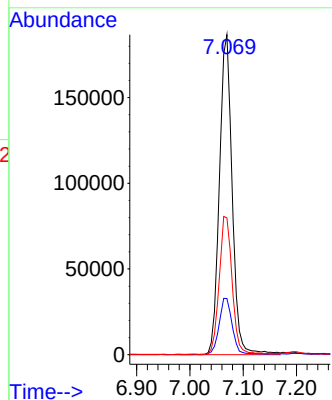

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.699 min Scan# 1294
Delta R.T. 0.000 min
Lab File: BP019794.D
Acq: 20 Feb 2024 19:52

Tgt Ion:136 Resp: 227689
Ion Ratio Lower Upper
136 100
137 11.5 8.8 13.2
54 7.1 5.3 7.9
68 4.8 4.1 6.1

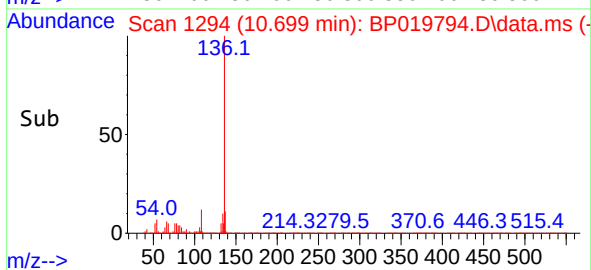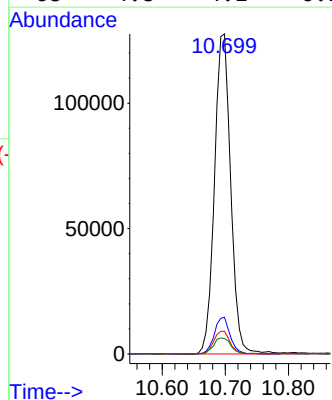



#23

Nitrobenzene-d5

Concen: 54.411 ng

RT: 9.063 min Scan# 1016

Delta R.T. -0.006 min

Lab File: BP019794.D


Acq: 20 Feb 2024 19:52

Instrument :

BNA_P

ClientSampleId :

20240767-AMENDED-COMP-39N-N-3-02

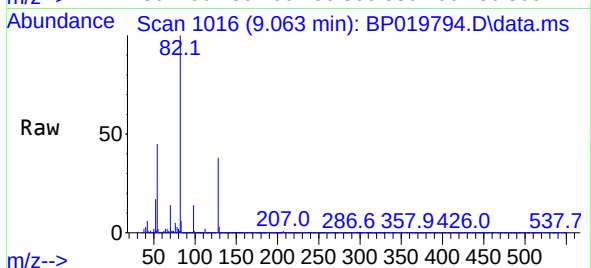




Tgt Ion: 82 Resp: 285909

Ion Ratio Lower Upper

82 100

128 38.2 29.7 44.5

54 44.5 36.8 55.2

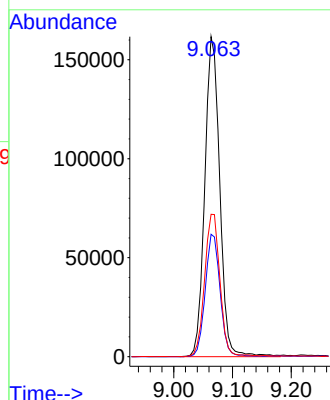

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.528 min Scan# 1945

Delta R.T. -0.012 min

Lab File: BP019794.D

Acq: 20 Feb 2024 19:52




Tgt Ion: 164 Resp: 161885


Ion Ratio Lower Upper

164 100

162 101.2 81.2 121.8

160 43.2 35.1 52.7


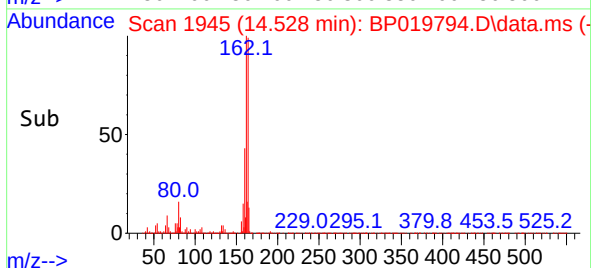
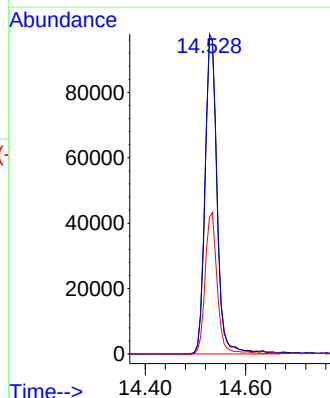





#42
2,4,6-Tribromophenol
Concen: 45.857 ng
RT: 16.028 min Scan# 21
Delta R.T. -0.006 min
Lab File: BP019794.D
Acq: 20 Feb 2024 19:52




Instrument :
BNA_P
ClientSampleId :
20240767-AMENDED-COMP-39N-N-3-02


Tgt Ion:330 Resp: 108390
Ion Ratio Lower Upper
330 100
332 97.3 77.2 115.8
141 29.7 27.0 40.4

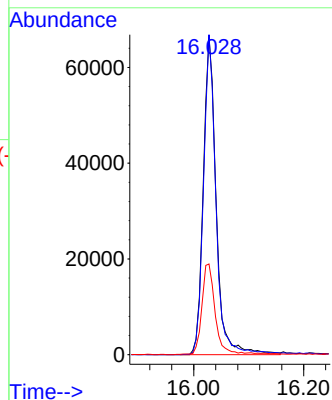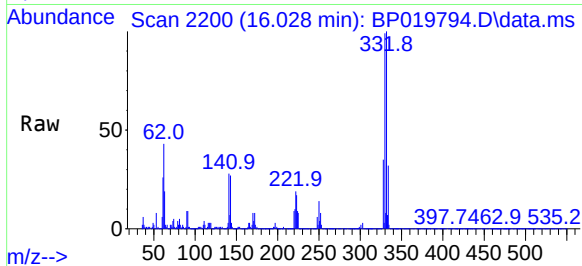

#45
2-Fluorobiphenyl
Concen: 48.182 ng
RT: 13.157 min Scan# 1712
Delta R.T. -0.006 min
Lab File: BP019794.D
Acq: 20 Feb 2024 19:52

Tgt Ion:172 Resp: 630942
Ion Ratio Lower Upper
172 100
171 35.5 28.2 42.4
170 22.5 18.9 28.3


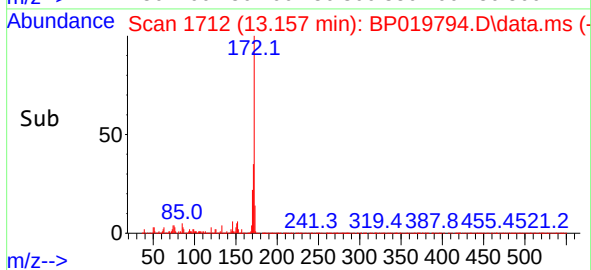
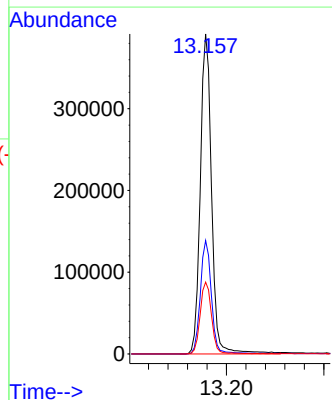
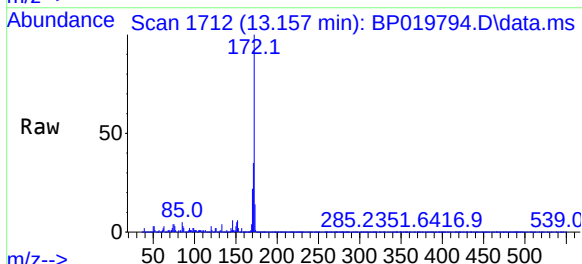




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.287 min Scan# 2417
Delta R.T. -0.006 min
Lab File: BP019794.D
Acq: 20 Feb 2024 19:52




Instrument :
BNA_P
ClientSampleId :
20240767-AMENDED-COMP-39N-N-3-02


Tgt Ion:188 Resp: 391560
Ion Ratio Lower Upper
188 100
94 6.8 5.4 8.2
80 7.7 6.3 9.5

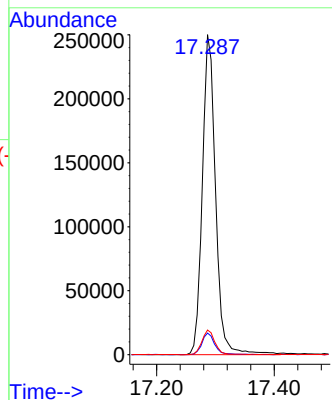

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.380 min Scan# 3110
Delta R.T. -0.012 min
Lab File: BP019794.D
Acq: 20 Feb 2024 19:52

Tgt Ion:240 Resp: 442373
Ion Ratio Lower Upper
240 100
120 5.8 6.1 9.1#
236 25.2 20.7 31.1


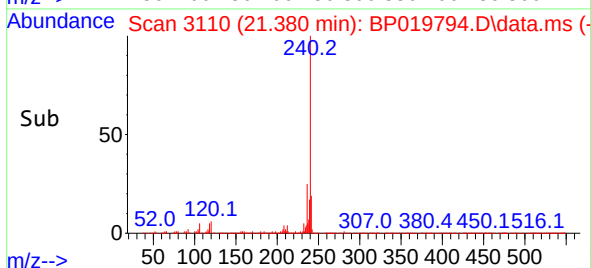
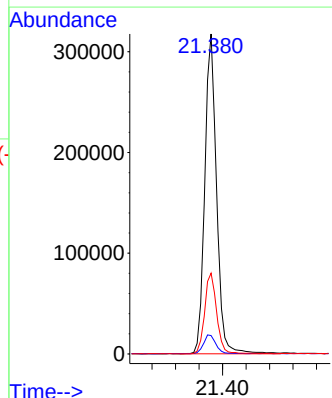





#79
Terphenyl-d14
Concen: 52.487 ng
RT: 19.857 min Scan# 21
Delta R.T. -0.006 min
Lab File: BP019794.D
Acq: 20 Feb 2024 19:52

Instrument :
BNA_P
ClientSampleId :
20240767-AMENDED-COMP-39N-N-3-02

Tgt Ion:244 Resp: 1411867
Ion Ratio Lower Upper
244 100
212 7.1 6.1 9.1
122 6.4 5.9 8.9

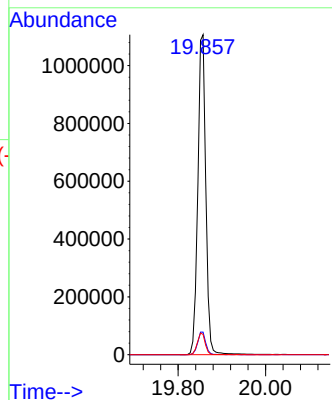

#86
Perylene-d12
Concen: 20.000 ng
RT: 23.798 min Scan# 3521
Delta R.T. -0.012 min
Lab File: BP019794.D
Acq: 20 Feb 2024 19:52

Tgt Ion:264 Resp: 499270
Ion Ratio Lower Upper
264 100
260 24.4 19.2 28.8
265 21.9 17.0 25.4

