
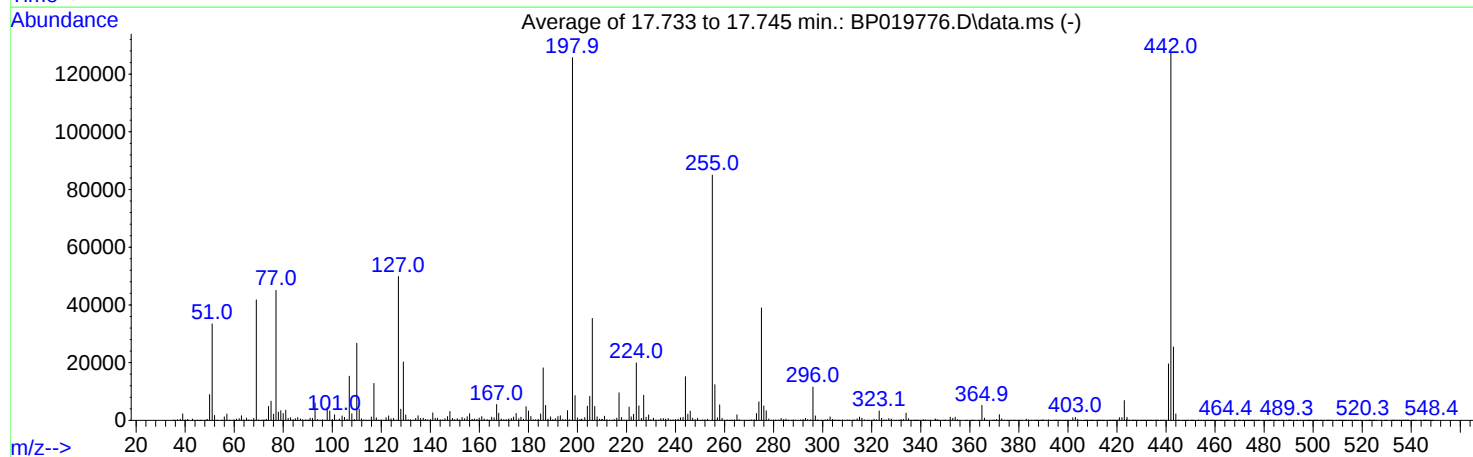


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022024\
Data File : BP019776.D
Acq On : 20 Feb 2024 09:36
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Feb 19 23:35:42 2024

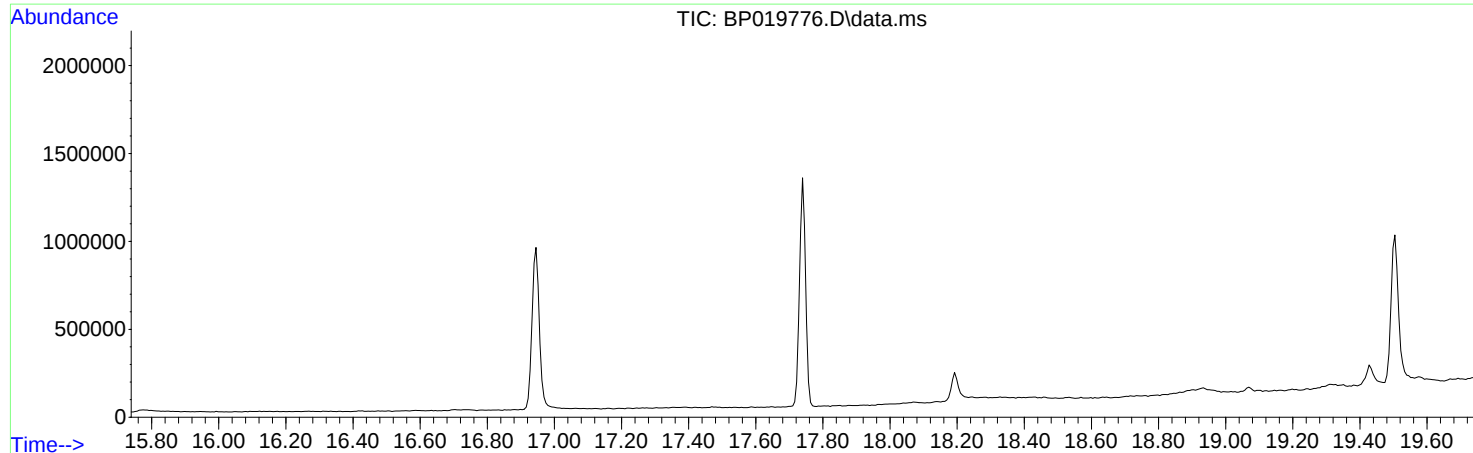




AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.6	33438	PASS
68	69	0.00	2	1.6	671	PASS
69	198	0.00	100	33.2	41772	PASS
70	69	0.00	2	0.3	144	PASS
127	198	10	80	39.7	49859	PASS
197	198	0.00	2	0.2	249	PASS
198	198	100	100	100.0	125673	PASS
199	198	5	9	6.8	8595	PASS
275	198	10	60	31.0	38976	PASS
365	198	1	100	4.1	5215	PASS
441	198	0.01	100	15.6	19593	PASS
442	442	100	100	100.0	127472	PASS
443	442	15	24	20.0	25458	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022024\
Data File : BP019776.D
Acq On : 20 Feb 2024 09:36
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 20 10:36:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 19 23:35:42 2024
Response via : Initial Calibration

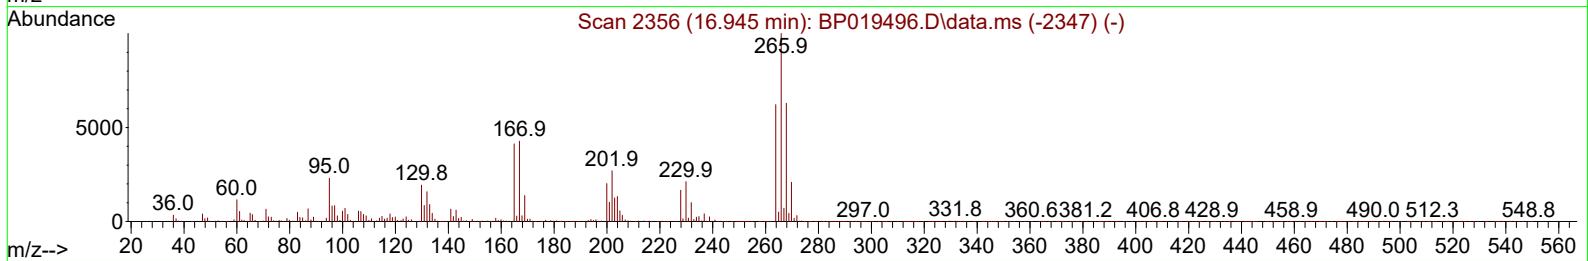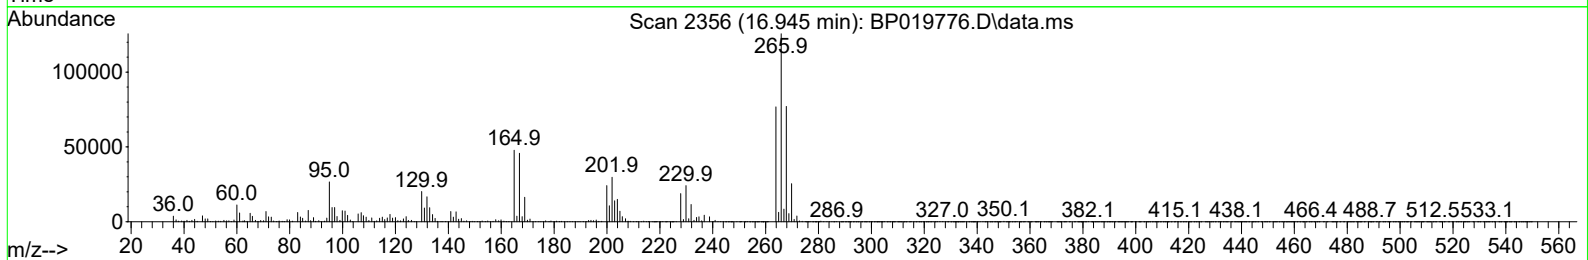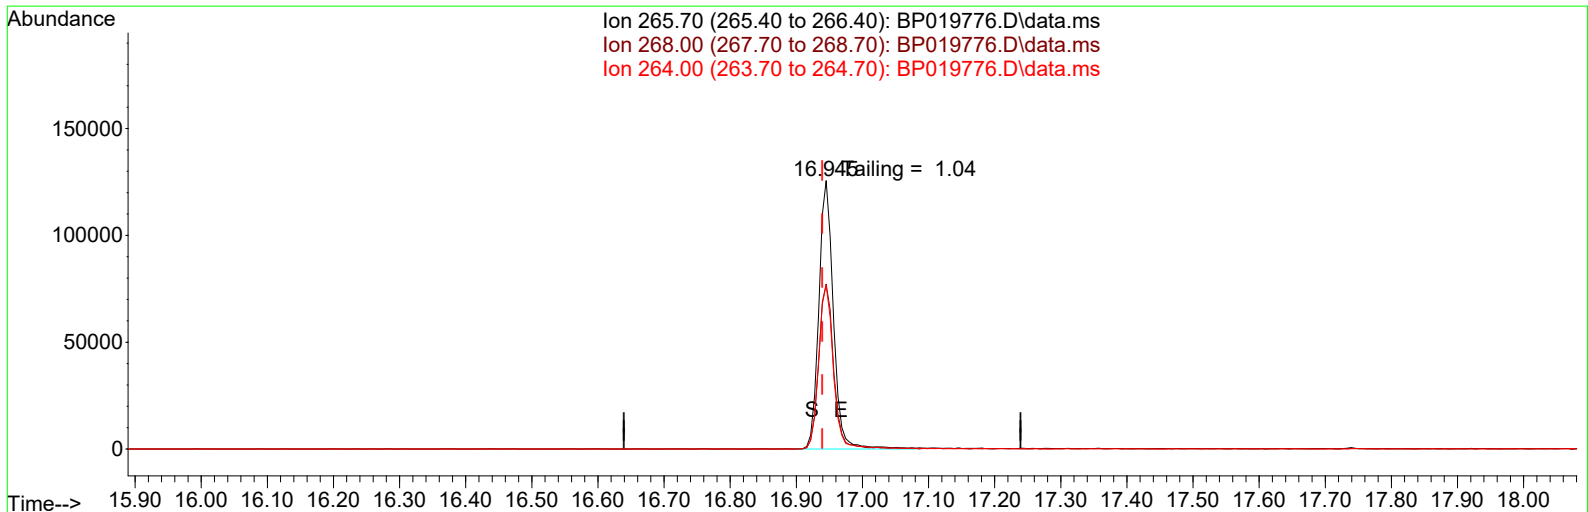

TIC: BP019776.D\data.ms

(70) Pentachlorophenol (C)

16.945min (+ 0.006) 133831.05 ng




response 192236

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	61.39
264.00	62.10	61.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022024\
Data File : BP019776.D
Acq On : 20 Feb 2024 09:36
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 20 10:36:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP013124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 19 23:35:42 2024
Response via : Initial Calibration

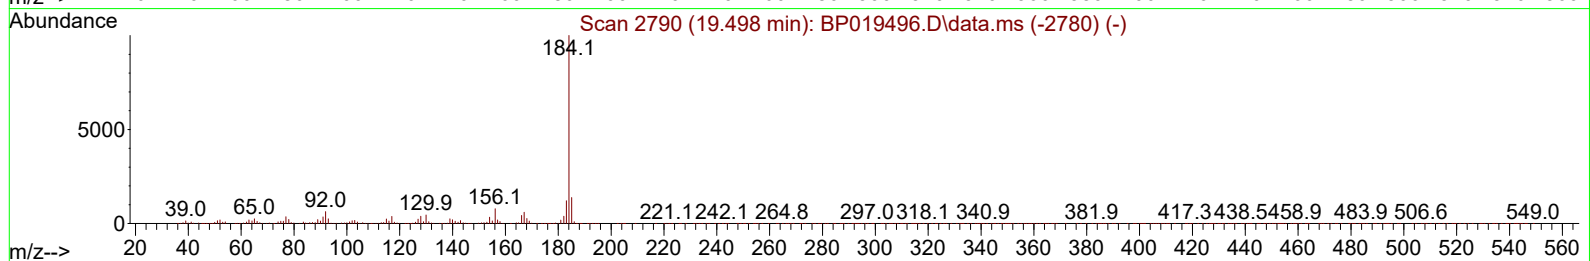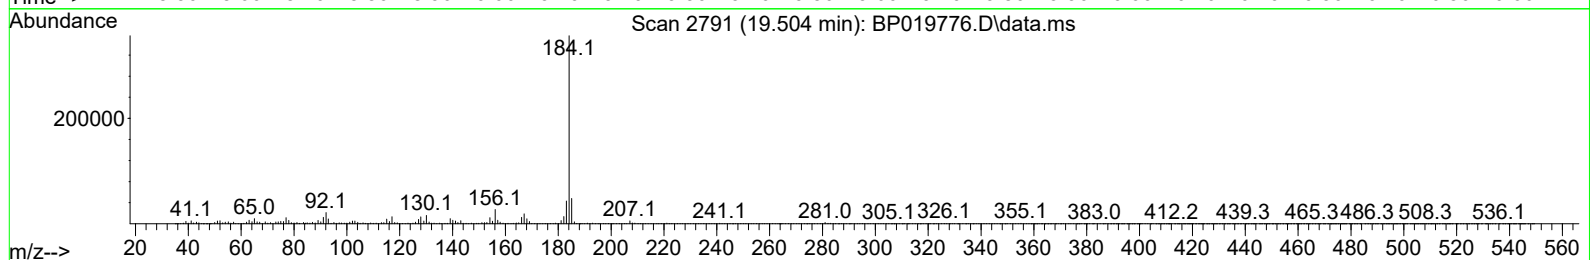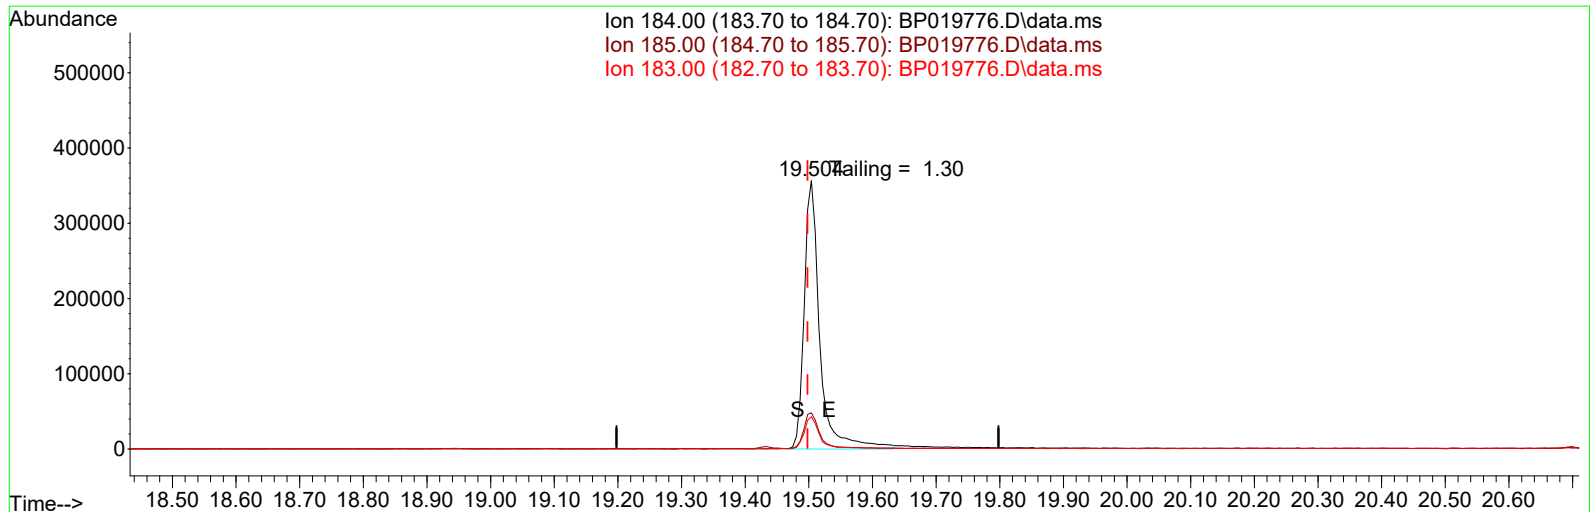

TIC: BP019776.D\data.ms

(77) Benzidine

19.504min (+ 0.006) 54622.56 ng

response 621235

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.49
183.00	12.10	12.07
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/19/2024	BNA_P	<u>BP019776.D</u>
Compound Name	Response	Retention Time
DDT	446258	20.698
DDD	18512	20.269
DDE	1433	19.769
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19945	466203	4.28

Instrument :
BNA_P
ClientSampleId :
DFTPP