

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022025\
 Data File : BP024102.D
 Acq On : 20 Feb 2025 10:22
 Operator : RC/JU
 Sample : PB166258BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB166258BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP024102.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.375	382	389	403	rBV	9122899	12301359	51.20%	10.554%
2	6.940	647	655	676	rBV	7998268	12304407	51.22%	10.556%
3	7.757	787	794	807	rBV	1991177	2869327	11.94%	2.462%
4	8.904	981	989	1004	rBV	4725999	7876071	32.78%	6.757%
5	10.534	1255	1266	1281	rBV	2372374	3961664	16.49%	3.399%
6	12.998	1677	1685	1702	rBV	12427623	19354064	80.56%	16.604%
7	14.392	1914	1922	1930	rBV	3577169	5212023	21.69%	4.471%
8	15.910	2171	2180	2204	rBV	8623955	13079810	54.44%	11.221%
9	17.192	2391	2398	2410	rBV	3830841	5660238	23.56%	4.856%
10	19.910	2854	2860	2873	rBV	16589082	24024433	100.00%	20.611%
11	21.627	3146	3152	3164	rBV	3520132	5170229	21.52%	4.436%
12	25.015	3720	3728	3747	rVB	1897081	4747801	19.76%	4.073%




Sum of corrected areas: 116561426

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022025\
Data File : BP024102.D
Acq On : 20 Feb 2025 10:22
Operator : RC/JU
Sample : PB166258BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB166258BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

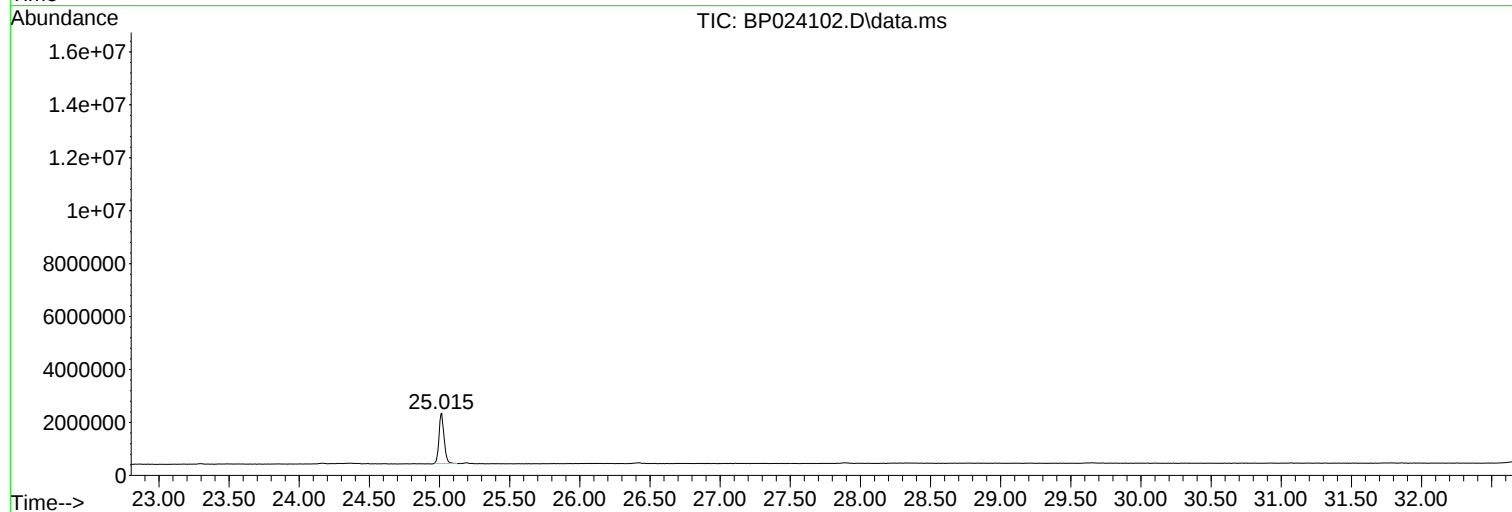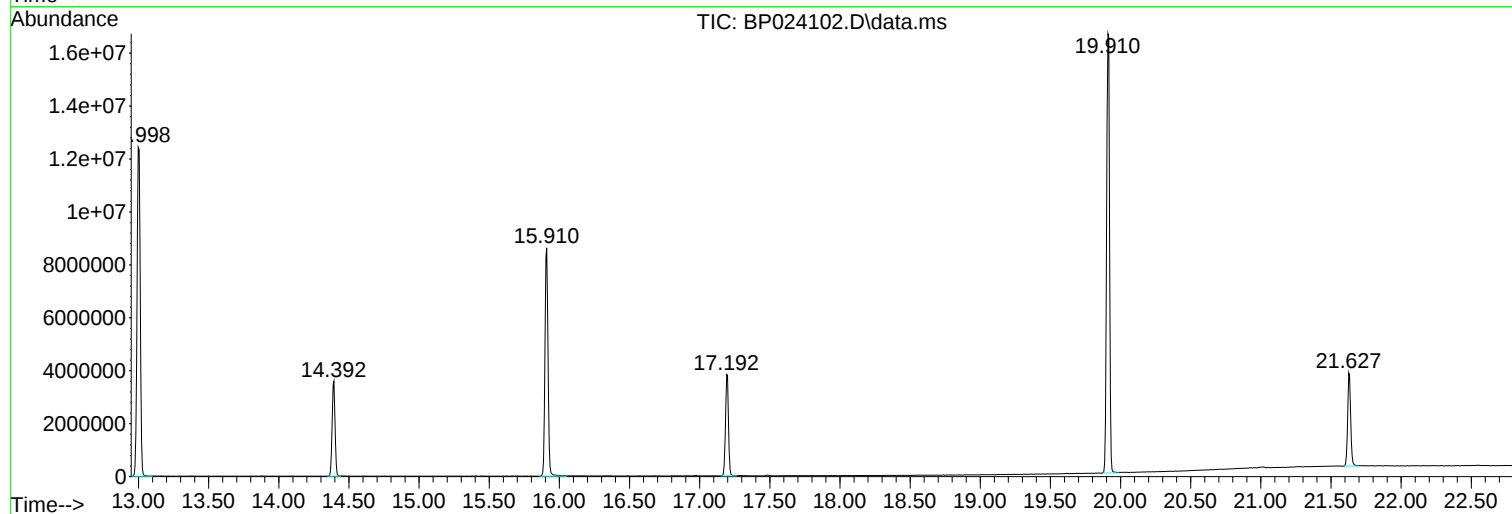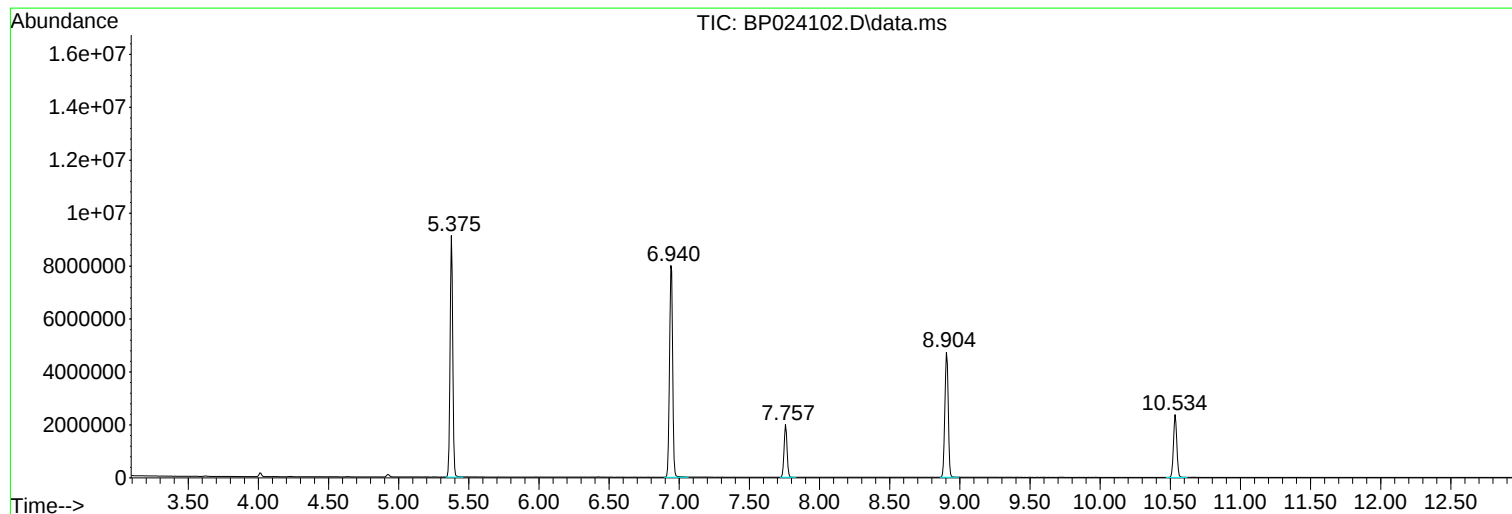

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022025\
Data File : BP024102.D
Acq On : 20 Feb 2025 10:22
Operator : RC/JU
Sample : PB166258BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB166258BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022025\
Data File : BP024102.D
Acq On : 20 Feb 2025 10:22
Operator : RC/JU
Sample : PB166258BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB166258BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------