

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022025\
Data File : BP024107.D
Acq On : 20 Feb 2025 13:46
Operator : RC/JU
Sample : PB166363BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB166363BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP024107.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.375	382	389	407	rBV	8561374	11979971	54.96%	10.940%
2	6.940	647	655	680	rBV	7736079	12066974	55.36%	11.019%
3	7.757	786	794	802	rBV	1785411	2758080	12.65%	2.519%
4	8.910	981	990	1003	rBV	4598385	7539460	34.59%	6.885%
5	10.534	1258	1266	1280	rBV	2218443	3752290	17.21%	3.426%
6	13.004	1677	1686	1699	rBV	11977861	18405978	84.44%	16.808%
7	14.392	1914	1922	1938	rBV	3139393	4872422	22.35%	4.449%
8	15.904	2171	2179	2206	rBV	9058531	12336437	56.60%	11.265%
9	17.192	2391	2398	2410	rBV2	3246719	5220411	23.95%	4.767%
10	19.921	2856	2862	2873	rBV	17631121	21797748	100.00%	19.905%
11	21.651	3150	3156	3168	rBV2	2832648	4610552	21.15%	4.210%
12	25.039	3723	3732	3746	rVB2	1403452	4168673	19.12%	3.807%




Sum of corrected areas: 109508996

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022025\
Data File : BP024107.D
Acq On : 20 Feb 2025 13:46
Operator : RC/JU
Sample : PB166363BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB166363BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

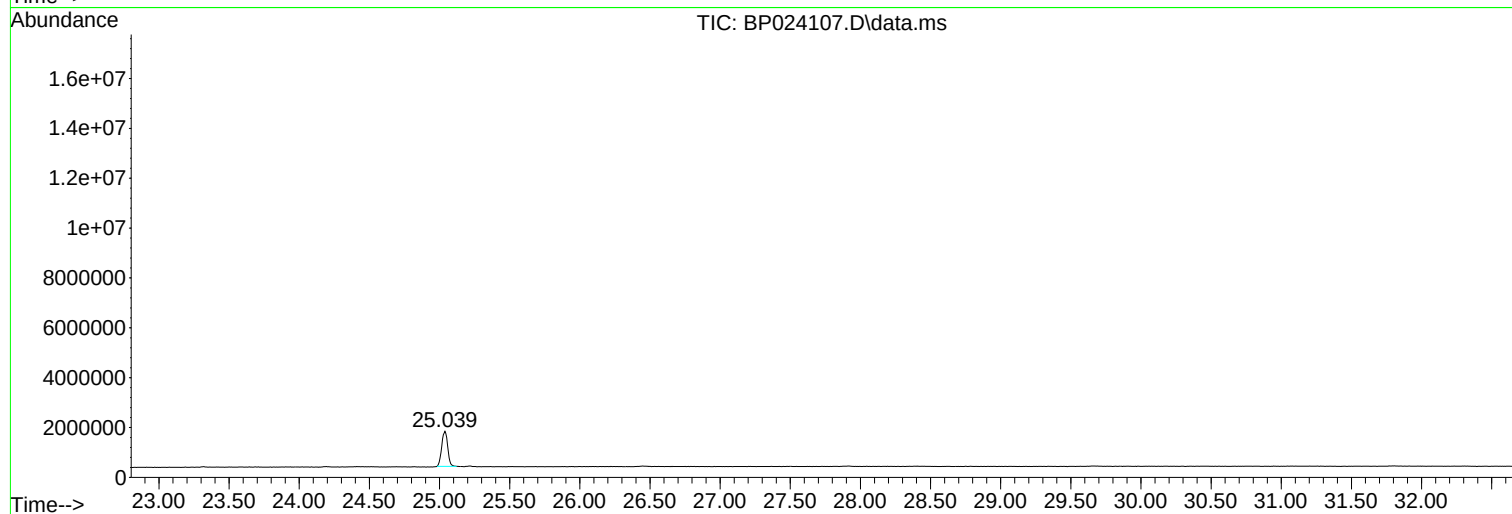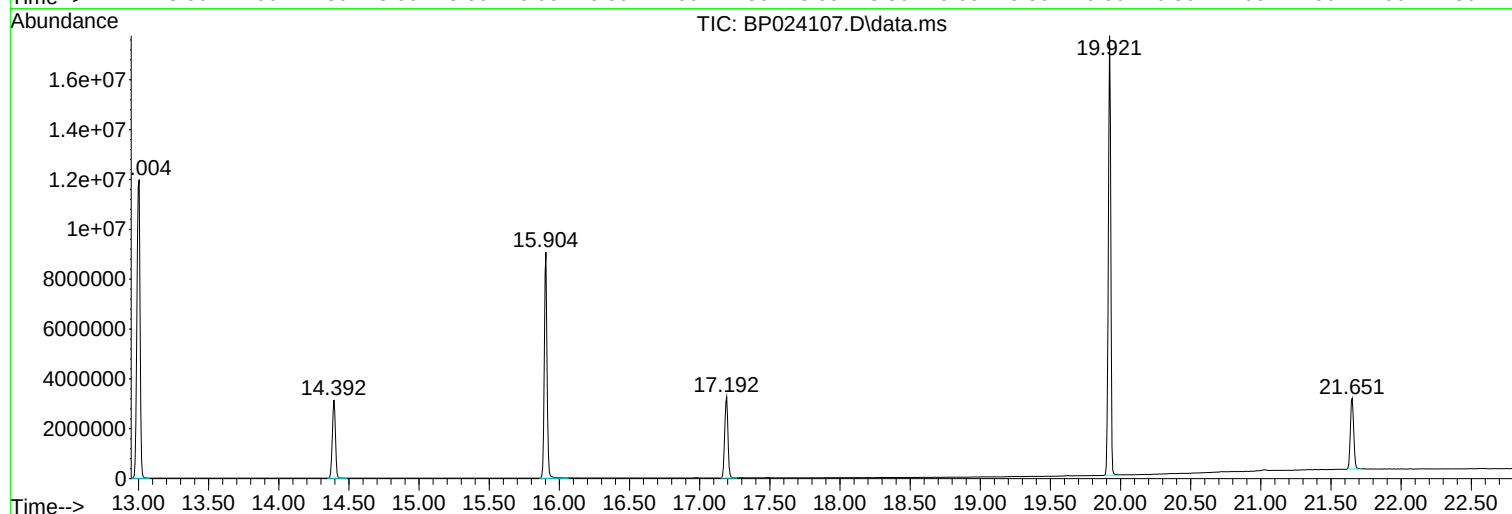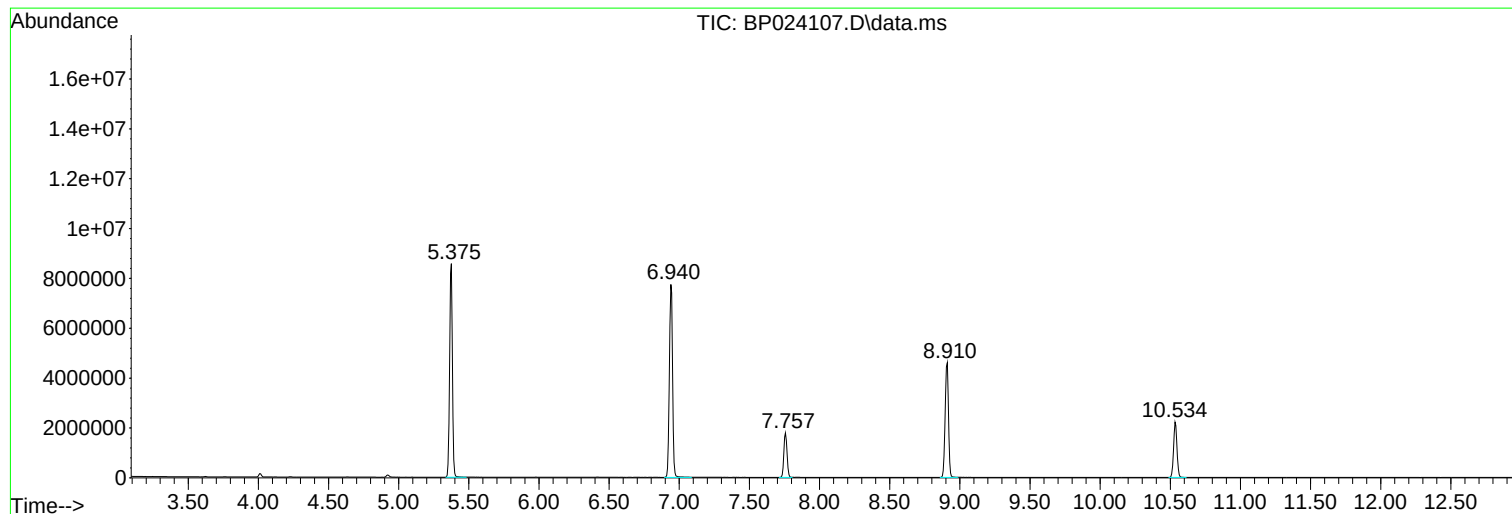

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022025\
Data File : BP024107.D
Acq On : 20 Feb 2025 13:46
Operator : RC/JU
Sample : PB166363BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB166363BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022025\
Data File : BP024107.D
Acq On : 20 Feb 2025 13:46
Operator : RC/JU
Sample : PB166363BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB166363BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------