


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022025\
Data File : BP024100.D
Acq On : 20 Feb 2025 09:01
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Feb 18 02:25:07 2025

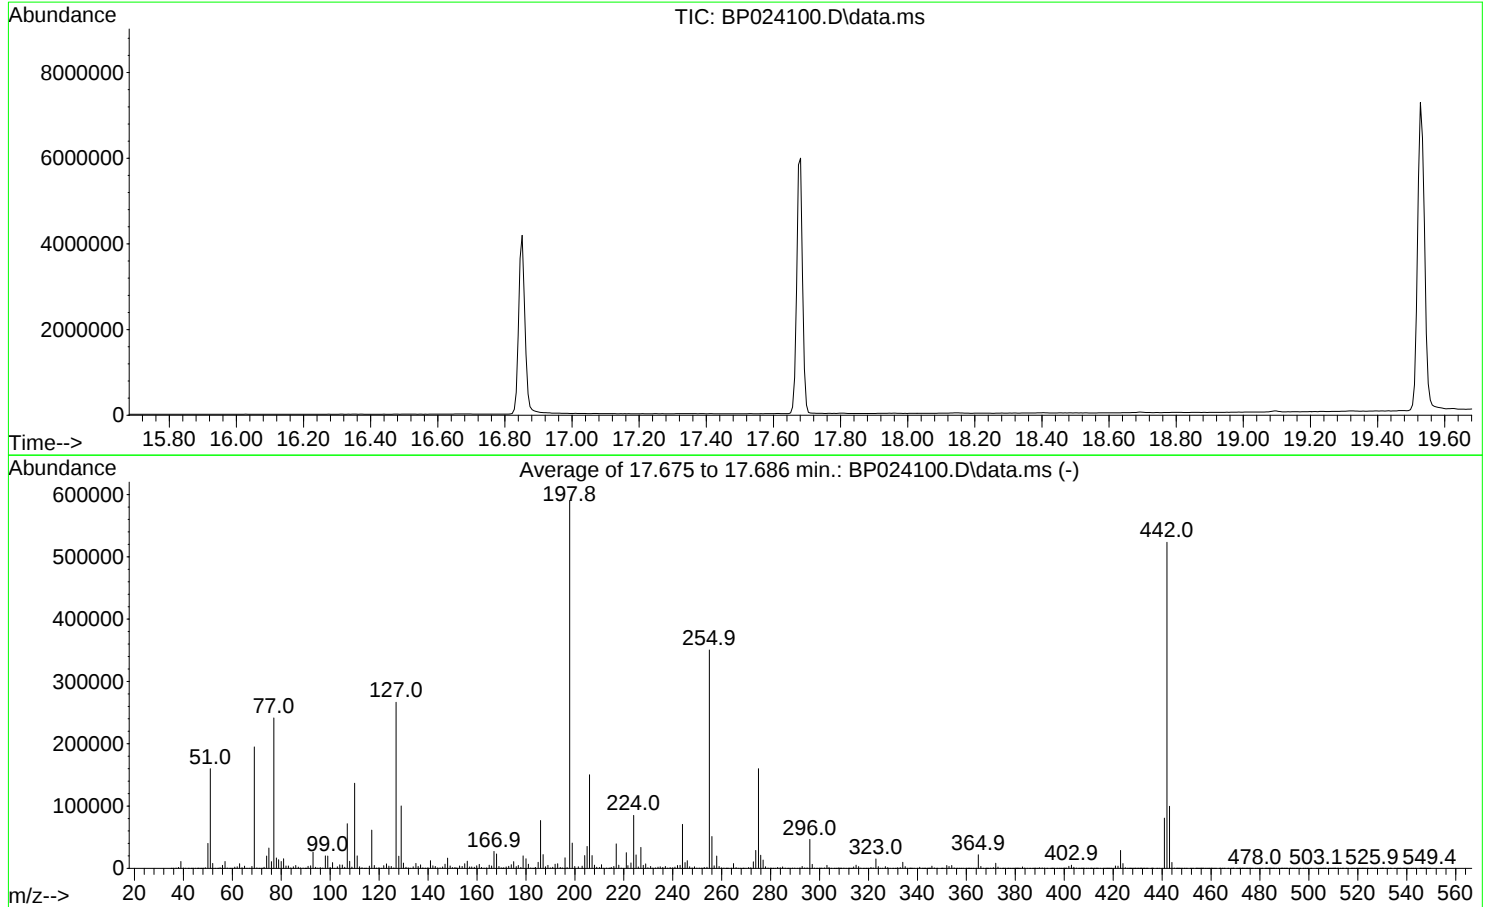

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.1	159942	PASS
68	69	0.00	2	1.6	3034	PASS
69	198	0.00	100	33.0	194905	PASS
70	69	0.00	2	0.5	913	PASS
127	198	10	80	45.2	266628	PASS
197	198	0.00	2	0.2	1407	PASS
198	198	100	100	100.0	590442	PASS
199	198	5	9	6.9	40677	PASS
275	198	10	60	27.1	160104	PASS
365	198	1	100	3.7	21768	PASS
441	198	0.01	100	13.6	80551	PASS
442	442	100	100	100.0	523411	PASS
443	442	15	24	19.0	99553	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/20/2025	BNA_P	<u>BP024100.D</u>
Compound Name	Response	Retention Time
DDT	2067426	20.828
DDD	18753	20.41
DDE	783	19.839
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19536	2086962	0.94

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022025\
Data File : BP024100.D
Acq On : 20 Feb 2025 09:01
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 20 13:17:26 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 18 02:25:07 2025
Response via : Initial Calibration

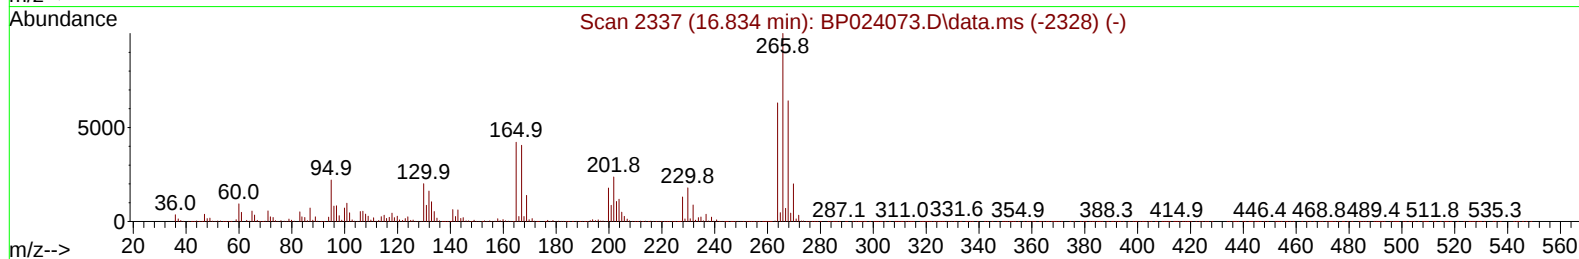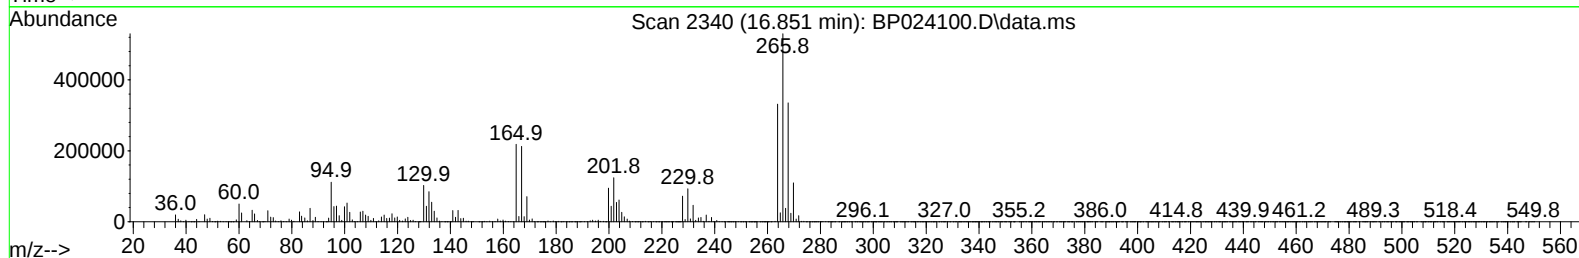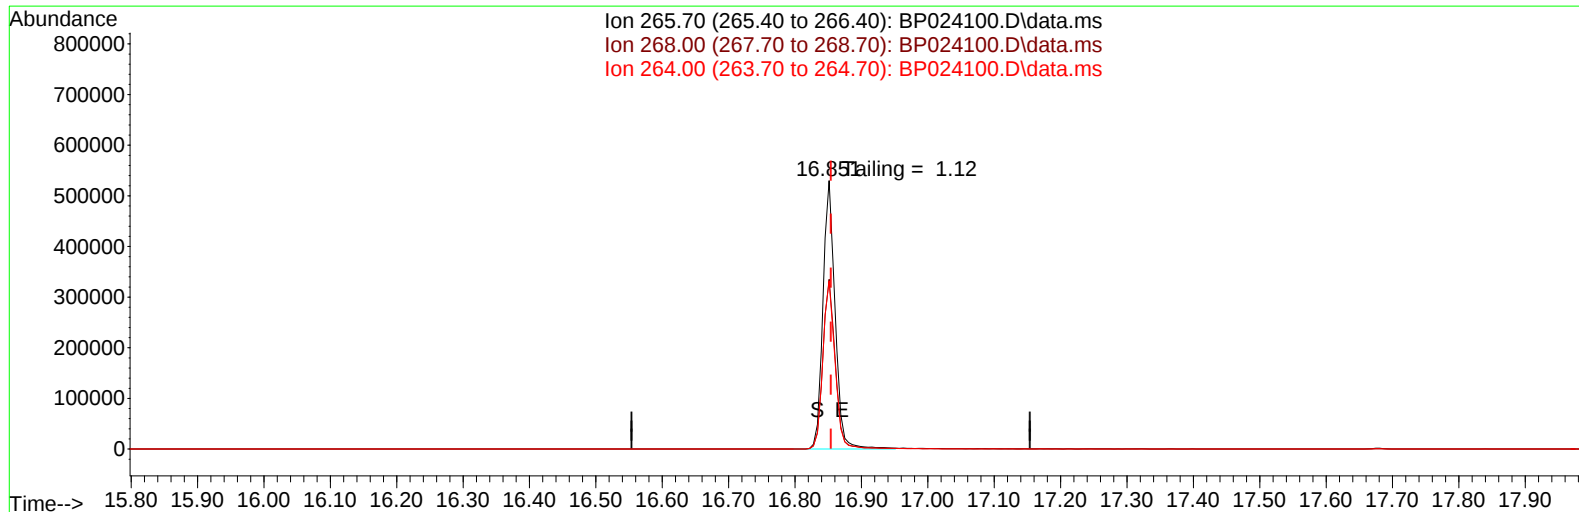

TIC: BP024100.D\data.ms

(70) Pentachlorophenol (C)

16.851min (-0.003) 87238.15 ng




response 677554

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	63.22
264.00	63.10	62.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022025\
Data File : BP024100.D
Acq On : 20 Feb 2025 09:01
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 20 13:17:26 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 18 02:25:07 2025
Response via : Initial Calibration

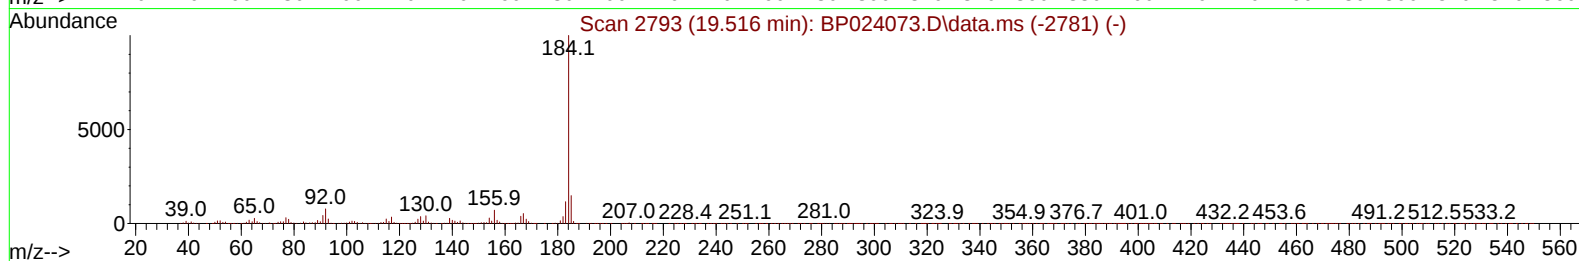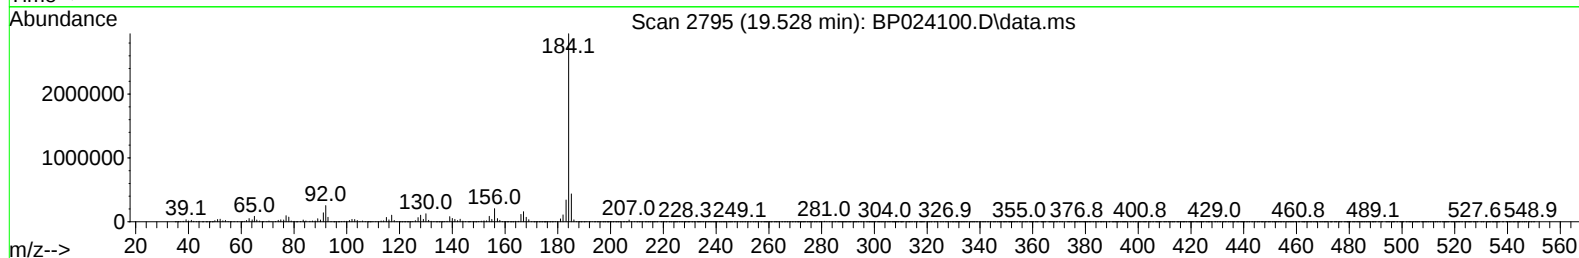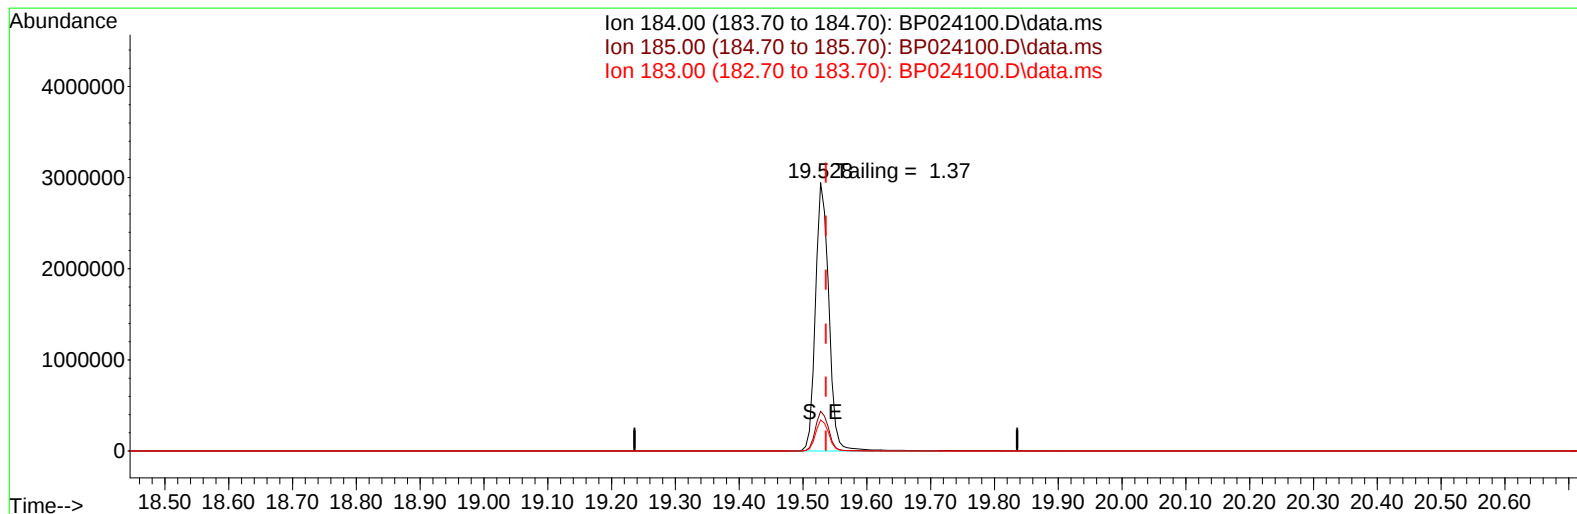

TIC: BP024100.D\data.ms

(77) Benzidine

19.528min (-0.008) 164259.39 ng

response 4303425

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.85
183.00	11.60	11.58
0.00	0.00	0.00